

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051731.D
 Acq On : 22 Dec 2021 1:02
 Operator : CG/JU
 Sample : M5177-05
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051731.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.544	7	9	13	rVB2	1159	1107	0.17%	0.036%
2	3.784	48	50	54	rVB2	956	1190	0.19%	0.039%
3	3.931	73	75	76	rBV	1158	773	0.12%	0.025%
4	3.978	81	83	86	rBV2	1399	1247	0.20%	0.041%
5	4.160	113	114	119	rVB3	1145	756	0.12%	0.025%
6	4.384	149	152	159	rVB4	2170	3679	0.58%	0.120%
7	4.554	179	181	184	rVB2	1227	1216	0.19%	0.040%
8	4.689	202	204	209	rVB	1152	1692	0.27%	0.055%
9	4.983	251	254	256	rVB2	948	1103	0.17%	0.036%
10	5.265	297	302	305	rVB2	810	914	0.14%	0.030%
11	5.347	313	316	319	rBV	771	942	0.15%	0.031%
12	5.394	323	324	327	rBV	890	1199	0.19%	0.039%
13	5.588	353	357	359	rBV	546	794	0.12%	0.026%
14	5.664	368	370	374	rVB2	876	870	0.14%	0.028%
15	5.770	385	388	391	rVB2	992	1102	0.17%	0.036%
16	5.846	400	401	405	rBV	708	763	0.12%	0.025%
17	5.899	408	410	414	rVB2	933	1514	0.24%	0.050%
18	6.052	434	436	438	rBV2	968	790	0.12%	0.026%
19	6.099	438	444	447	rVB	714	1381	0.22%	0.045%
20	6.457	502	505	508	rVB	720	920	0.14%	0.030%
21	6.598	527	529	533	rVB	625	780	0.12%	0.026%
22	7.532	684	688	690	rVB	854	760	0.12%	0.025%
23	8.272	805	814	822	rVB	132806	225098	35.40%	7.372%
24	8.472	843	848	850	rBV	684	939	0.15%	0.031%
25	8.590	865	868	870	rBV	629	891	0.14%	0.029%
26	8.878	914	917	920	rVB2	616	794	0.12%	0.026%
27	8.983	931	935	938	rBV	556	870	0.14%	0.028%
28	9.071	947	950	953	rBV2	603	884	0.14%	0.029%
29	9.154	961	964	967	rVB	729	968	0.15%	0.032%
30	9.277	981	985	988	rBV2	918	1392	0.22%	0.046%
31	9.530	1027	1028	1033	rBV	623	874	0.14%	0.029%
32	9.582	1033	1037	1039	rVB2	613	822	0.13%	0.027%
33	9.700	1055	1057	1063	rBV	673	815	0.13%	0.027%
34	9.794	1069	1073	1075	rBV2	575	772	0.12%	0.025%
35	10.552	1199	1202	1204	rBV	588	758	0.12%	0.025%
36	11.110	1289	1297	1306	rBV	188220	345681	54.37%	11.321%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051731.D
 Acq On : 22 Dec 2021 1:02
 Operator : CG/JU
 Sample : M5177-05
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	11.239	1318	1319	1322	rBV	847	1014	0.16%	0.033%
38	11.327	1330	1334	1337	rVB	482	813	0.13%	0.027%
39	11.644	1384	1388	1390	rBV	736	867	0.14%	0.028%
40	12.185	1478	1480	1485	rBV2	675	1055	0.17%	0.035%

41	12.490	1529	1532	1536	rVB	658	960	0.15%	0.031%
42	12.625	1554	1555	1561	rBV2	745	1203	0.19%	0.039%
43	12.684	1561	1565	1569	rBV2	546	1024	0.16%	0.034%
44	13.401	1684	1687	1689	rBV	980	787	0.12%	0.026%
45	13.548	1710	1712	1717	rBV	693	949	0.15%	0.031%

46	13.624	1719	1725	1728	rBV	673	1218	0.19%	0.040%
47	13.683	1731	1735	1737	rBV2	748	1024	0.16%	0.034%
48	13.824	1754	1759	1762	rBV	951	1635	0.26%	0.054%
49	14.341	1843	1847	1849	rBV2	662	983	0.15%	0.032%
50	14.388	1853	1855	1859	rBV2	658	1011	0.16%	0.033%

51	14.911	1937	1944	1955	rVB	328774	519150	81.65%	17.002%
52	15.104	1976	1977	1981	rBV2	648	923	0.15%	0.030%
53	15.292	2006	2009	2012	rBV2	732	878	0.14%	0.029%
54	15.733	2081	2084	2086	rVV2	783	780	0.12%	0.026%
55	15.756	2086	2088	2091	rVB	899	891	0.14%	0.029%

56	16.068	2139	2141	2145	rVB2	761	755	0.12%	0.025%
57	16.450	2205	2206	2209	rBV	607	786	0.12%	0.026%
58	16.820	2266	2269	2272	rBV2	629	797	0.13%	0.026%
59	16.949	2288	2291	2293	rBV	845	812	0.13%	0.027%
60	17.442	2371	2375	2379	rVB2	1296	1465	0.23%	0.048%

61	17.654	2404	2411	2421	rBV	395710	614691	96.67%	20.131%
62	17.754	2423	2428	2430	rVV2	1070	1494	0.23%	0.049%
63	17.854	2444	2445	2449	rVB	851	976	0.15%	0.032%
64	18.024	2471	2474	2478	rVB2	723	1145	0.18%	0.037%
65	18.218	2506	2507	2513	rVB2	808	1097	0.17%	0.036%

66	18.335	2525	2527	2529	rBV2	814	1051	0.17%	0.034%
67	18.623	2573	2576	2580	rVB	947	1270	0.20%	0.042%
68	18.852	2613	2615	2616	rBV	1390	833	0.13%	0.027%
69	18.970	2632	2635	2637	rBV2	1495	1686	0.27%	0.055%
70	19.029	2643	2645	2647	rBV	703	799	0.13%	0.026%

71	19.175	2668	2670	2672	rBV	898	816	0.13%	0.027%
72	19.211	2674	2676	2677	rVB2	1592	925	0.15%	0.030%
73	19.234	2677	2680	2681	rBV2	760	762	0.12%	0.025%
74	19.310	2689	2693	2694	rBV	1154	903	0.14%	0.030%
75	19.322	2694	2695	2701	rVV3	1006	1431	0.23%	0.047%

76	19.387	2705	2706	2709	rBV2	1114	1036	0.16%	0.034%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051731.D
 Acq On : 22 Dec 2021 1:02
 Operator : CG/JU
 Sample : M5177-05
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	19.440	2713	2715	2717	rVB2	976	787	0.12%	0.026%
78	19.628	2745	2747	2749	rBV3	1043	879	0.14%	0.029%
79	19.681	2754	2756	2757	rBV2	1099	876	0.14%	0.029%
80	20.203	2843	2845	2846	rBV	1577	1075	0.17%	0.035%
81	20.397	2877	2878	2879	rVB	2527	891	0.14%	0.029%
82	20.703	2928	2930	2933	rBV4	2228	2037	0.32%	0.067%
83	21.977	3140	3147	3157	rVB	371532	635841	100.00%	20.824%
84	23.440	3394	3396	3397	rBV2	3614	3028	0.48%	0.099%
85	23.534	3410	3412	3415	rBV4	4553	3662	0.58%	0.120%
86	25.473	3732	3742	3763	rVB2	189165	614266	96.61%	20.117%
87	25.984	3828	3829	3830	rBV	3129	1348	0.21%	0.044%
88	26.501	3915	3917	3918	rBV2	4348	2113	0.33%	0.069%
89	31.200	4713	4717	4720	rBV5	4209	6902	1.09%	0.226%




Sum of corrected areas: 3053450

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051731.D
Acq On : 22 Dec 2021 1:02
Operator : CG/JU
Sample : M5177-05
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

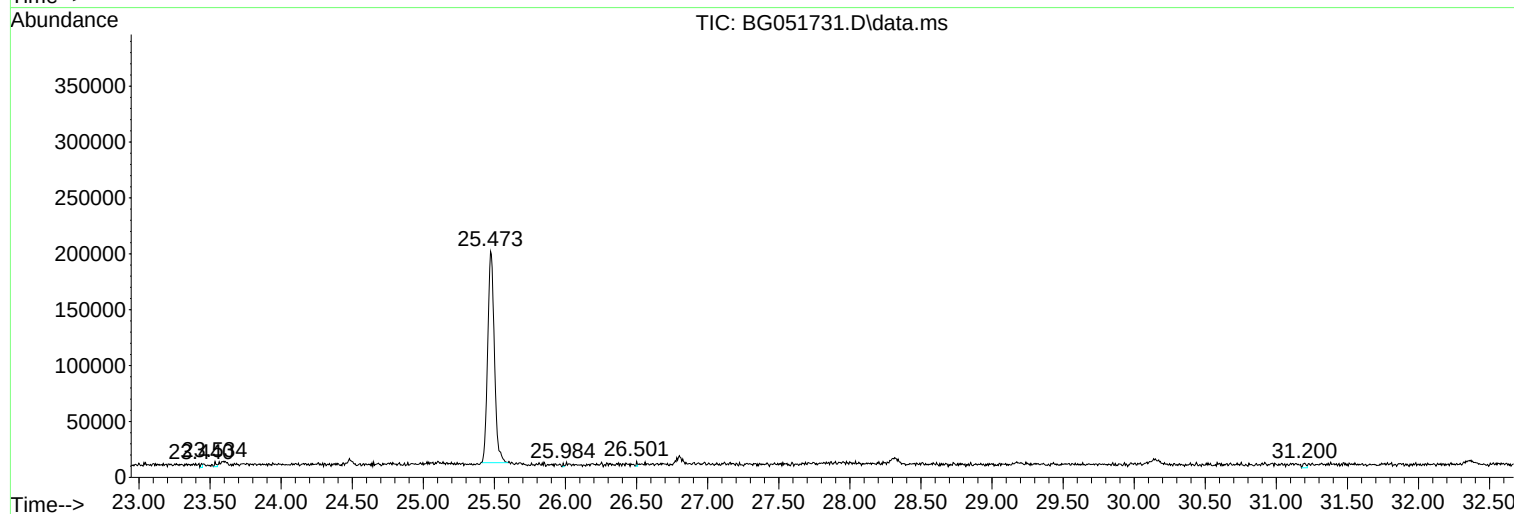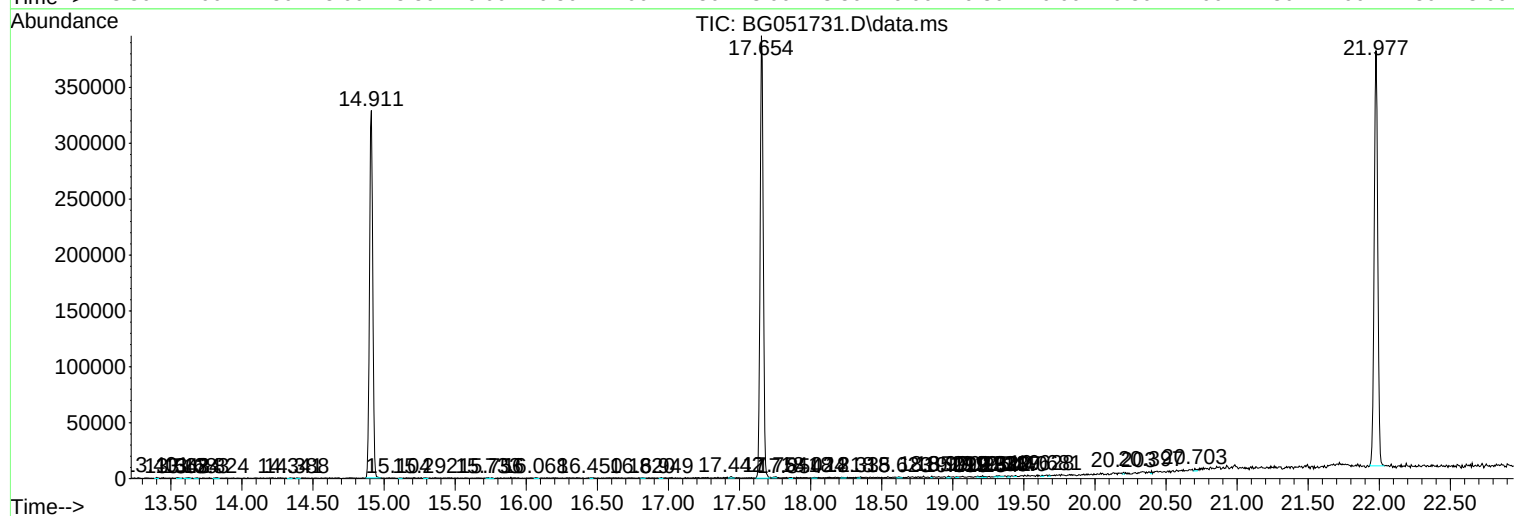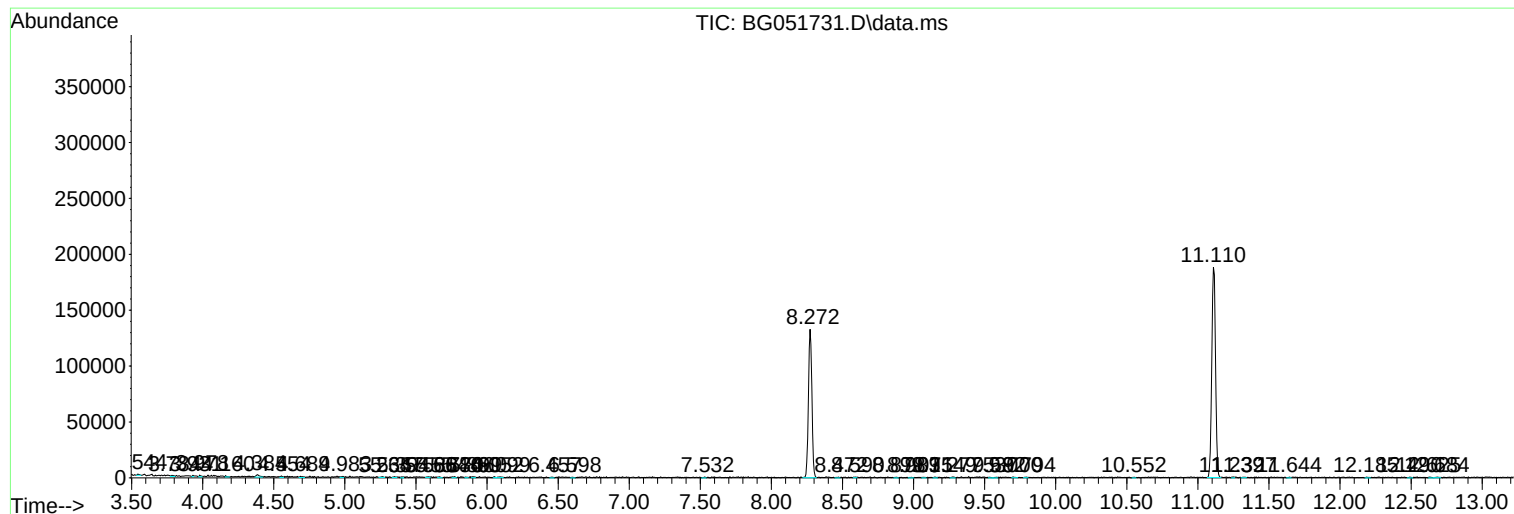

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051731.D
Acq On : 22 Dec 2021 1:02
Operator : CG/JU
Sample : M5177-05
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051731.D
Acq On : 22 Dec 2021 1:02
Operator : CG/JU
Sample : M5177-05
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------