

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051732.D
 Acq On : 22 Dec 2021 1:42
 Operator : CG/JU
 Sample : M5177-10
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051732.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.609	18	20	24	rVB3	917	1062	0.16%	0.034%
2	3.661	27	29	34	rVB4	780	1107	0.16%	0.036%
3	3.726	39	40	42	rBV	1273	863	0.13%	0.028%
4	3.932	73	75	78	rBV	1046	993	0.15%	0.032%
5	4.378	148	151	154	rBV3	2014	2348	0.35%	0.076%
6	4.455	160	164	165	rBV	848	1043	0.16%	0.034%
7	4.590	185	187	191	rVB	563	890	0.13%	0.029%
8	4.748	211	214	218	rVB3	855	1048	0.16%	0.034%
9	5.430	327	330	333	rBV	864	895	0.13%	0.029%
10	5.541	346	349	352	rBV	750	1130	0.17%	0.037%
11	5.788	389	391	394	rVB	856	904	0.13%	0.029%
12	5.823	394	397	401	rBV2	1136	1401	0.21%	0.045%
13	6.064	436	438	441	rVB2	1068	944	0.14%	0.031%
14	6.516	509	515	516	rBV	760	834	0.12%	0.027%
15	6.898	576	580	583	rBV2	529	863	0.13%	0.028%
16	7.210	631	633	637	rBV	742	1126	0.17%	0.036%
17	7.568	692	694	696	rBV2	903	810	0.12%	0.026%
18	8.026	769	772	775	rVB	796	1018	0.15%	0.033%
19	8.273	807	814	822	rVB	131459	228397	34.03%	7.402%
20	8.467	844	847	849	rBV	776	953	0.14%	0.031%
21	8.802	901	904	907	rVB2	560	804	0.12%	0.026%
22	9.307	987	990	993	rVB	779	905	0.13%	0.029%
23	9.342	993	996	999	rBB2	907	888	0.13%	0.029%
24	11.110	1290	1297	1306	rVB	199388	360943	53.78%	11.697%
25	11.498	1358	1363	1366	rBV	717	1145	0.17%	0.037%
26	11.891	1425	1430	1431	rBV2	643	909	0.14%	0.029%
27	12.215	1482	1485	1488	rBV	827	1003	0.15%	0.033%
28	12.403	1516	1517	1523	rVB	1003	1223	0.18%	0.040%
29	12.972	1612	1614	1620	rVB	752	1109	0.17%	0.036%
30	13.014	1620	1621	1626	rBV	646	987	0.15%	0.032%
31	13.337	1671	1676	1678	rBV	713	910	0.14%	0.029%
32	13.948	1776	1780	1782	rBV	466	809	0.12%	0.026%
33	14.094	1802	1805	1808	rBV	544	1018	0.15%	0.033%
34	14.694	1904	1907	1910	rBV2	631	978	0.15%	0.032%
35	14.905	1936	1943	1956	rVB2	324362	519037	77.34%	16.821%
36	15.463	2036	2038	2041	rBV	570	837	0.12%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051732.D
 Acq On : 22 Dec 2021 1:42
 Operator : CG/JU
 Sample : M5177-10
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	16.491	2209	2213	2215	rBV	641	832	0.12%	0.027%
38	16.526	2215	2219	2221	rBV2	676	823	0.12%	0.027%
39	17.443	2371	2375	2377	rVB3	2220	2175	0.32%	0.070%
40	17.654	2404	2411	2422	rBV	415449	625259	93.16%	20.263%
41	17.836	2439	2442	2444	rBV2	725	829	0.12%	0.027%
42	18.218	2504	2507	2509	rVB2	924	860	0.13%	0.028%
43	18.676	2581	2585	2587	rBV2	667	814	0.12%	0.026%
44	19.082	2652	2654	2657	rVB	1223	1024	0.15%	0.033%
45	19.158	2665	2667	2670	rBV3	930	1195	0.18%	0.039%
46	19.422	2709	2712	2713	rBV3	1581	1418	0.21%	0.046%
47	19.593	2740	2741	2746	rVB4	1633	1871	0.28%	0.061%
48	19.628	2746	2747	2750	rBV	1175	1029	0.15%	0.033%
49	19.763	2766	2770	2772	rBV3	1368	1901	0.28%	0.062%
50	19.869	2786	2788	2790	rVB	1202	966	0.14%	0.031%
51	19.922	2796	2797	2802	rBV3	1734	1826	0.27%	0.059%
52	20.045	2814	2818	2821	rBV4	1887	2965	0.44%	0.096%
53	20.233	2849	2850	2853	rVB2	2633	1451	0.22%	0.047%
54	20.262	2853	2855	2856	rBV2	1332	942	0.14%	0.031%
55	20.280	2856	2858	2859	rBV2	1463	962	0.14%	0.031%
56	20.374	2872	2874	2876	rBV3	2376	2051	0.31%	0.066%
57	21.197	3012	3014	3016	rBV2	3617	3372	0.50%	0.109%
58	21.643	3088	3090	3091	rBV2	3059	2206	0.33%	0.071%
59	21.978	3139	3147	3159	rBV	389342	671137	100.00%	21.750%
60	23.088	3334	3336	3338	rBV3	3368	2657	0.40%	0.086%
61	25.473	3733	3742	3755	rBV2	198538	605429	90.21%	19.621%
62	27.559	4096	4097	4101	rVB4	3714	3511	0.52%	0.114%
63	29.521	4429	4431	4434	rVB4	3672	2672	0.40%	0.087%
64	32.099	4868	4870	4871	rVB2	2939	1361	0.20%	0.044%




Sum of corrected areas: 3085672

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051732.D
Acq On : 22 Dec 2021 1:42
Operator : CG/JU
Sample : M5177-10
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

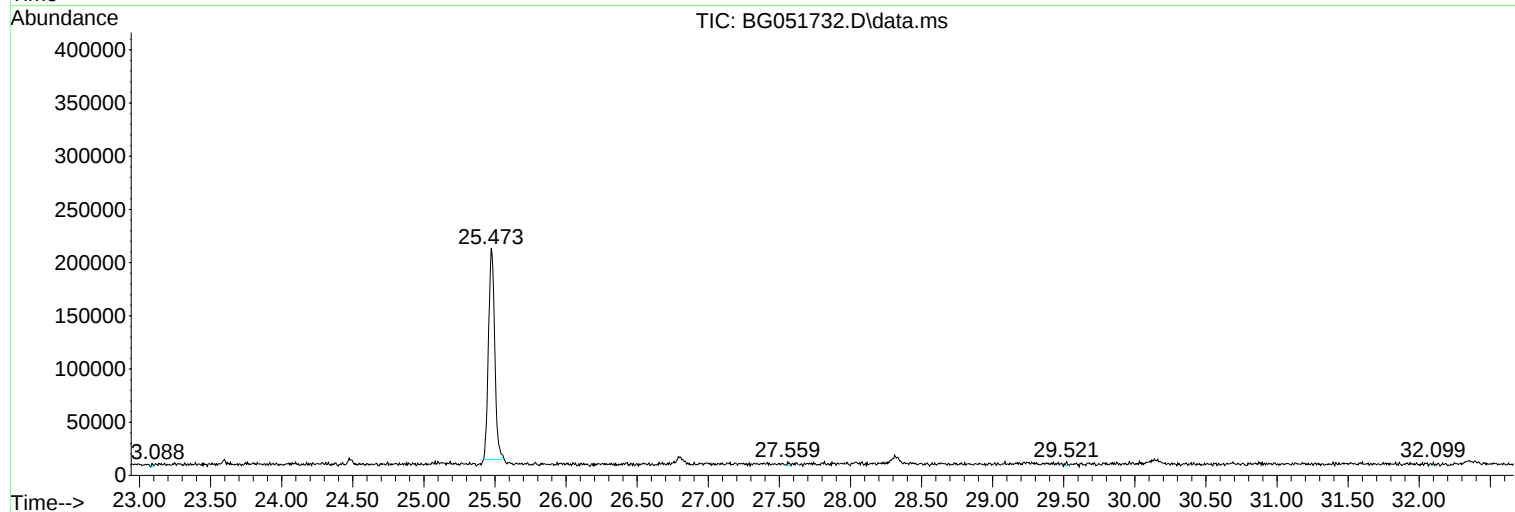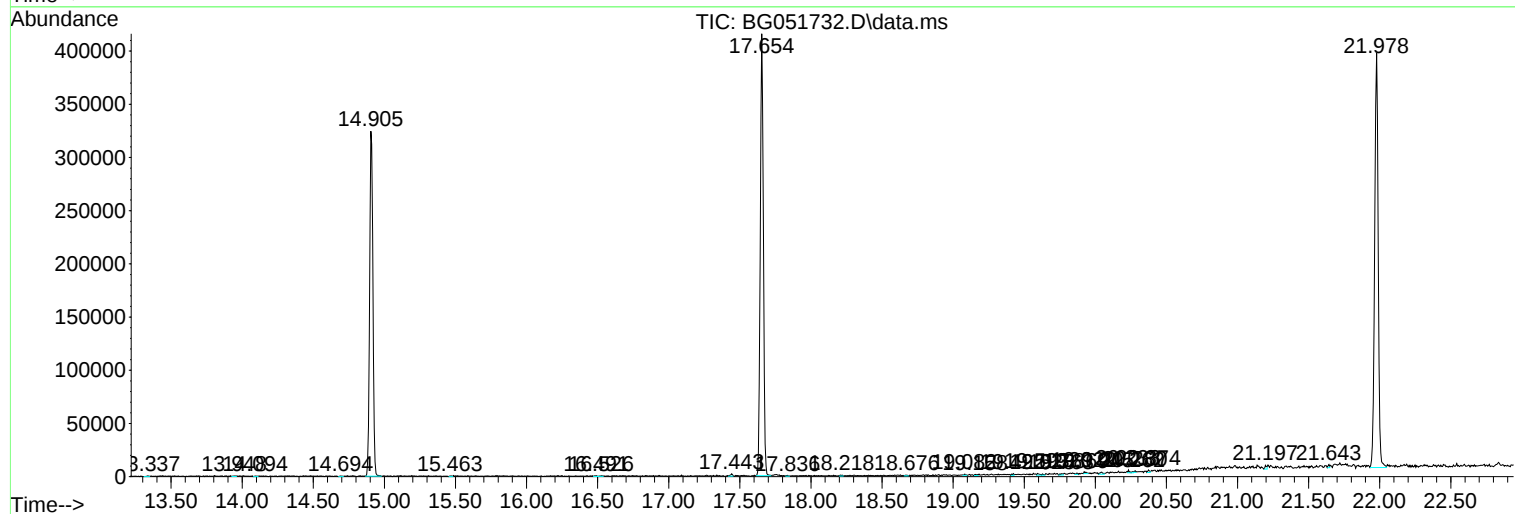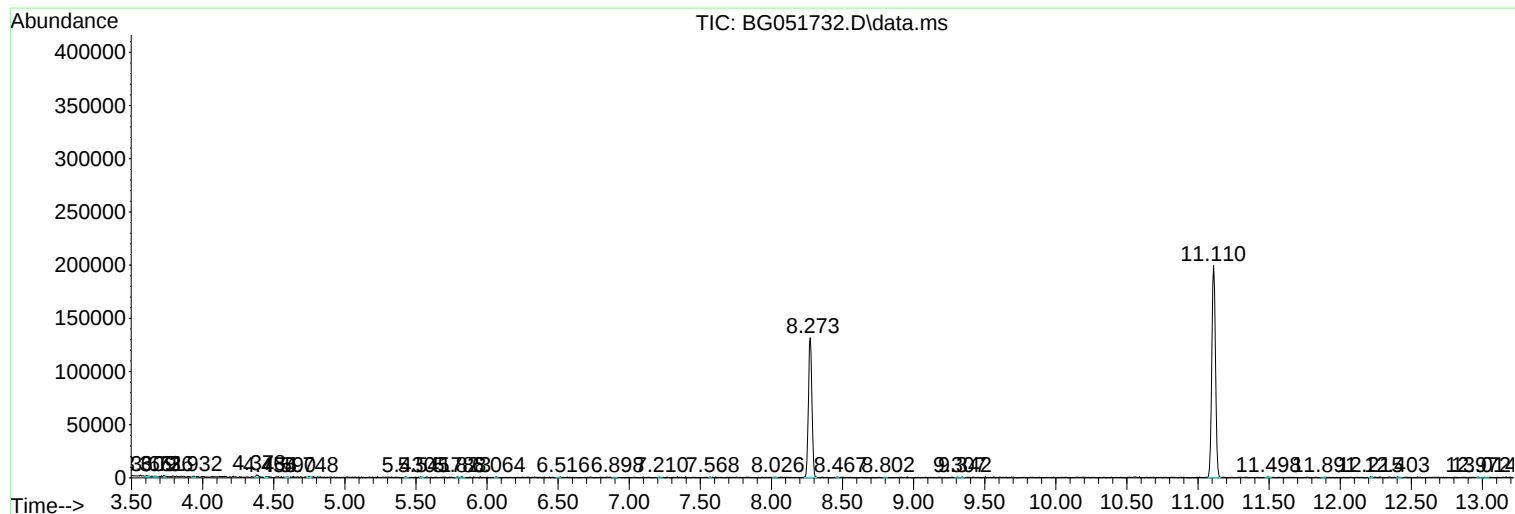

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051732.D
Acq On : 22 Dec 2021 1:42
Operator : CG/JU
Sample : M5177-10
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051732.D
Acq On : 22 Dec 2021 1:42
Operator : CG/JU
Sample : M5177-10
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc