

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051742.D
 Acq On : 22 Dec 2021 9:06
 Operator : CG/JU
 Sample : M5090-04
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3C6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.600	14	19	24	rBV	10156	15988	1.21%	0.133%
2	4.035	88	93	101	rBV	30591	55051	4.16%	0.459%
3	4.281	129	135	138	rBV4	2536	3696	0.28%	0.031%
4	4.381	149	152	157	rVB4	2556	3813	0.29%	0.032%
5	5.321	308	312	317	rBV2	2798	3132	0.24%	0.026%
6	7.406	660	667	676	rBV	48746	87605	6.62%	0.730%
7	7.577	689	696	704	rVB	135561	228305	17.26%	1.902%
8	7.800	725	734	743	rBV	147843	255015	19.28%	2.124%
9	8.276	808	815	827	rBV	134723	238573	18.04%	1.987%
10	8.969	925	933	942	rVB	126751	221667	16.76%	1.846%
11	9.439	1006	1013	1024	rVB	184140	331221	25.05%	2.759%
12	9.868	1081	1086	1091	rBV2	2959	3732	0.28%	0.031%
13	10.173	1130	1138	1146	rBV	151298	263137	19.90%	2.192%
14	10.720	1223	1231	1242	rBV	222330	395843	29.93%	3.297%
15	10.861	1250	1255	1260	rBV2	3670	6859	0.52%	0.057%
16	11.113	1291	1298	1307	rVB	193907	349901	26.46%	2.915%
17	11.231	1311	1318	1327	rBV2	179355	322858	24.41%	2.689%
18	12.682	1556	1565	1570	rVB3	4172	7248	0.55%	0.060%
19	13.522	1703	1708	1713	rVB4	2375	4394	0.33%	0.037%
20	13.727	1739	1743	1748	rVB5	2956	5106	0.39%	0.043%
21	13.956	1779	1782	1786	rBV4	2606	3915	0.30%	0.033%
22	14.297	1832	1840	1847	rBV	469616	687409	51.98%	5.726%
23	14.532	1875	1880	1884	rBV4	3786	4716	0.36%	0.039%
24	14.603	1885	1892	1900	rVV	472701	771874	58.37%	6.430%
25	14.785	1919	1923	1928	rVB3	1874	2202	0.17%	0.018%
26	14.908	1937	1944	1951	rBV	324885	505270	38.21%	4.209%
27	15.073	1966	1972	1985	rBV2	44758	78837	5.96%	0.657%
28	15.689	2074	2077	2081	rVB3	2956	3871	0.29%	0.032%
29	15.730	2081	2084	2089	rVB2	1747	2723	0.21%	0.023%
30	15.895	2105	2112	2120	rBV	645348	1010819	76.44%	8.420%
31	15.995	2123	2129	2137	rBV	185479	286126	21.64%	2.383%
32	16.136	2146	2153	2157	rBV4	3421	5457	0.41%	0.045%
33	16.565	2221	2226	2229	rBV3	2471	3730	0.28%	0.031%
34	16.676	2241	2245	2250	rVB2	1517	2710	0.20%	0.023%
35	17.346	2353	2359	2360	rBV2	1739	2131	0.16%	0.018%
36	17.393	2362	2367	2369	rVV3	2701	3723	0.28%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051742.D
 Acq On : 22 Dec 2021 9:06
 Operator : CG/JU
 Sample : M5090-04
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3C6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	17.446	2371	2376	2382	rBV4	2651	5286	0.40%	0.044%
38	17.546	2390	2393	2397	rBV2	4117	3910	0.30%	0.033%
39	17.657	2404	2412	2419	rBV	416476	630345	47.67%	5.251%
40	17.757	2421	2429	2439	rVB2	730323	1145602	86.63%	9.543%
41	17.951	2457	2462	2464	rVB2	1597	2288	0.17%	0.019%
42	18.127	2489	2492	2495	rBV3	2535	3540	0.27%	0.029%
43	18.309	2518	2523	2524	rBV4	2546	3296	0.25%	0.027%
44	18.521	2556	2559	2561	rBV3	2400	2417	0.18%	0.020%
45	18.597	2570	2572	2575	rVB4	2346	1914	0.14%	0.016%
46	19.220	2675	2678	2683	rVB4	1814	2526	0.19%	0.021%
47	19.273	2683	2687	2689	rBV4	1667	2533	0.19%	0.021%
48	19.384	2702	2706	2708	rBV4	3305	5158	0.39%	0.043%
49	19.596	2738	2742	2747	rBV4	9957	14350	1.09%	0.120%
50	19.666	2750	2754	2757	rBV2	8598	10748	0.81%	0.090%
51	20.031	2809	2816	2823	rBV	946475	1322386	100.00%	11.015%
52	20.718	2930	2933	2934	rBV2	2189	2348	0.18%	0.020%
53	21.182	3010	3012	3015	rBV3	3467	3086	0.23%	0.026%
54	21.581	3078	3080	3085	rBV5	6477	8770	0.66%	0.073%
55	21.975	3140	3147	3157	rVB	387829	665429	50.32%	5.543%
56	25.235	3691	3702	3716	rVB2	431174	1268910	95.96%	10.570%
57	25.476	3730	3743	3760	rBV2	206020	698789	52.84%	5.821%
58	28.308	4218	4225	4226	rBV5	10749	20586	1.56%	0.171%
59	31.938	4841	4843	4845	rBV2	3007	2201	0.17%	0.018%




Sum of corrected areas: 12005075

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051742.D
Acq On : 22 Dec 2021 9:06
Operator : CG/JU
Sample : M5090-04
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3C6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

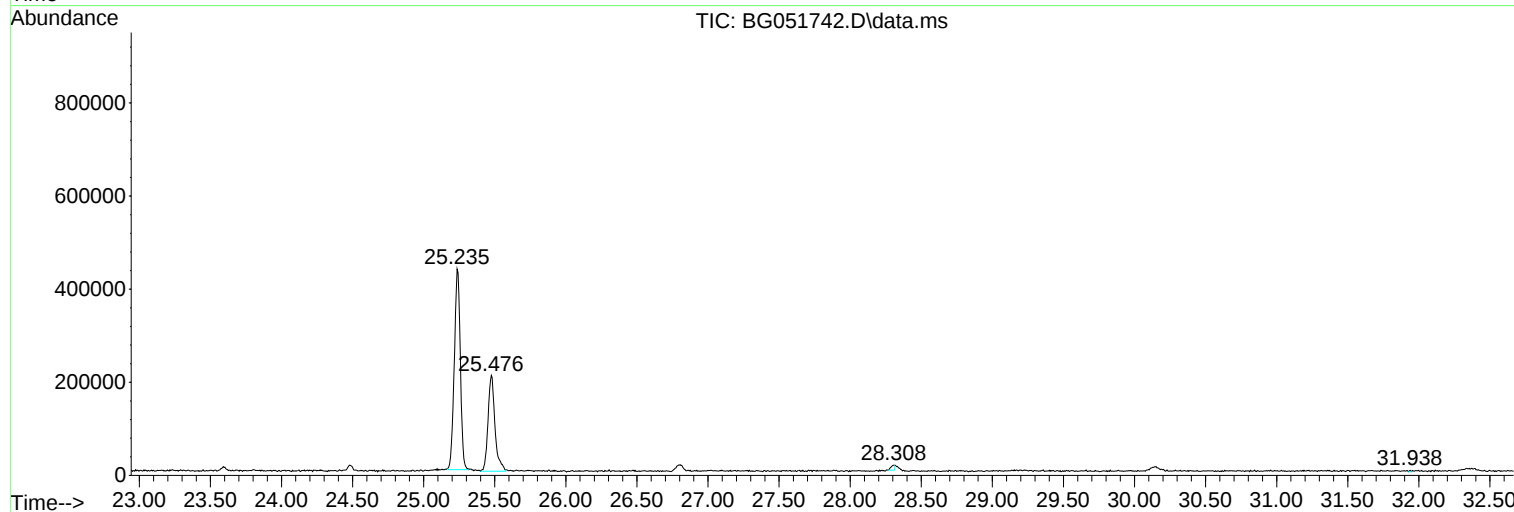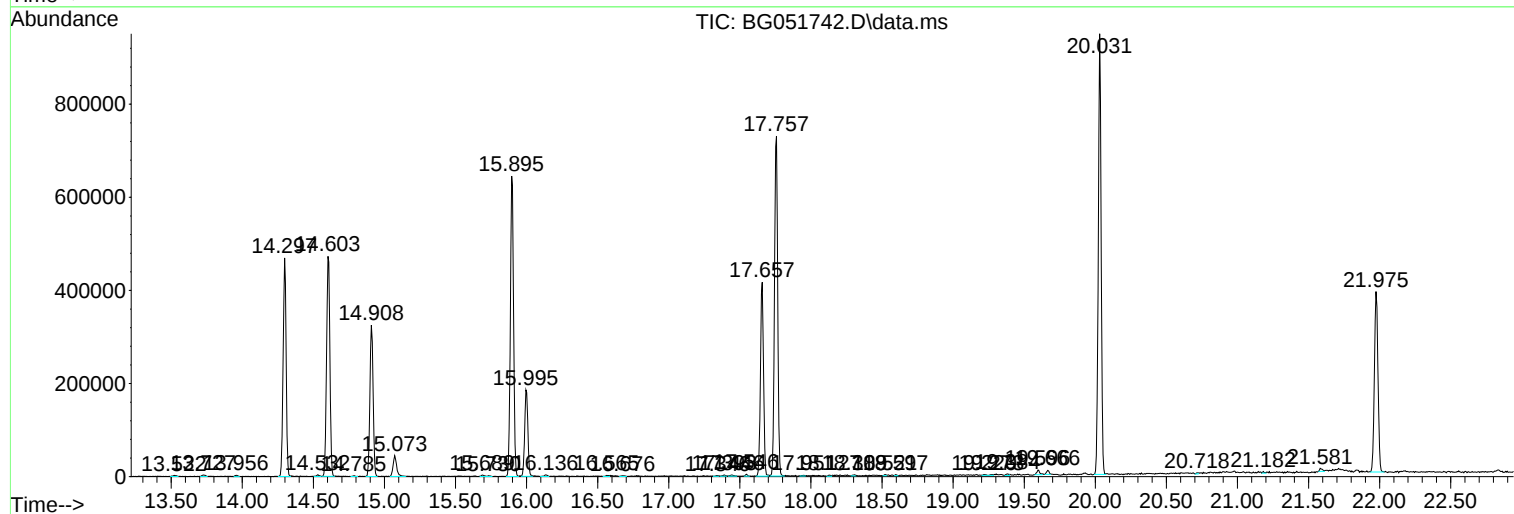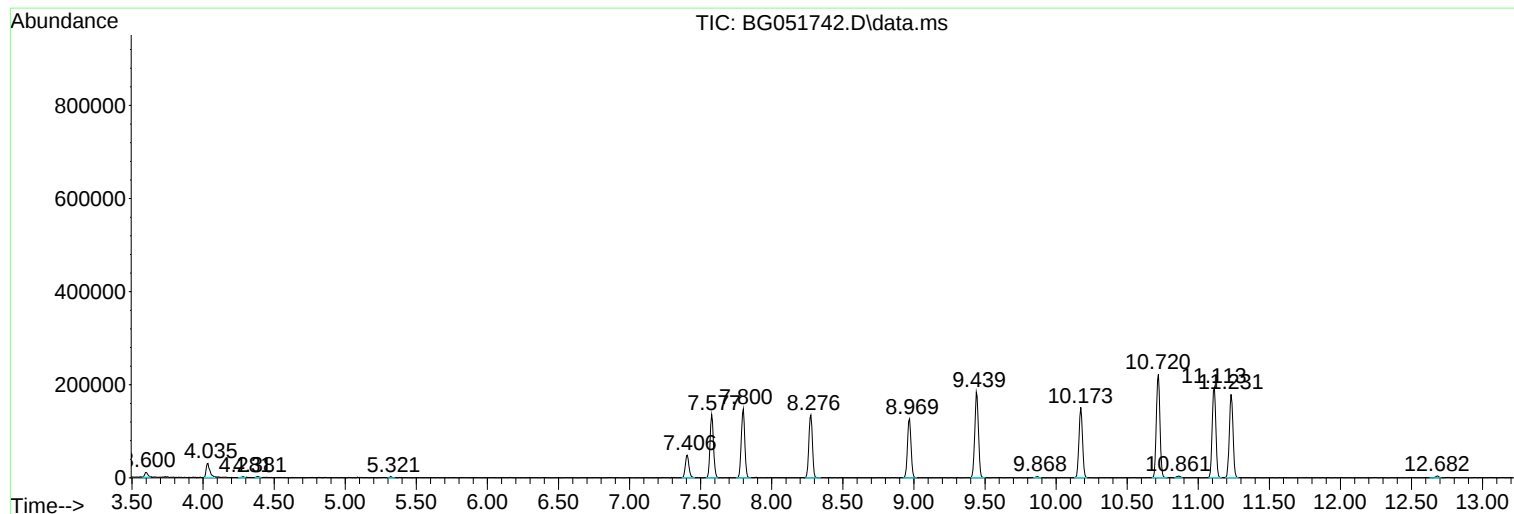

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051742.D
Acq On : 22 Dec 2021 9:06
Operator : CG/JU
Sample : M5090-04
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3C6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051742.D
Acq On : 22 Dec 2021 9:06
Operator : CG/JU
Sample : M5090-04
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3C6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc