

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051744.D
 Acq On : 22 Dec 2021 10:28
 Operator : CG/JU
 Sample : M5090-01
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3C0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051744.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.600	15	19	25	rBV2	9909	15604	1.27%	0.127%
2	3.864	63	64	69	rBV2	1181	1692	0.14%	0.014%
3	4.029	88	92	109	rVB	52258	94970	7.71%	0.773%
4	4.146	109	112	115	rBV2	1476	1728	0.14%	0.014%
5	4.293	131	137	138	rVB5	1617	2730	0.22%	0.022%
6	4.393	149	154	157	rBV3	3012	4518	0.37%	0.037%
7	4.446	160	163	167	rVB	1324	1974	0.16%	0.016%
8	5.321	308	312	317	rVB2	2744	3412	0.28%	0.028%
9	7.407	660	667	675	rVB2	56812	92910	7.54%	0.756%
10	7.577	689	696	704	rBV	137002	233094	18.92%	1.897%
11	7.800	727	734	741	rBV	151825	262116	21.28%	2.133%
12	8.276	807	815	822	rVB	166087	285574	23.18%	2.324%
13	8.969	925	933	941	rBV	141104	241071	19.57%	1.961%
14	9.445	1006	1014	1021	rBV	186395	335231	27.21%	2.728%
15	10.173	1131	1138	1147	rVB	152890	273280	22.18%	2.223%
16	10.720	1224	1231	1240	rBV2	222787	406825	33.02%	3.310%
17	11.113	1287	1298	1308	rBV	235791	425108	34.51%	3.459%
18	11.231	1310	1318	1326	rBV	164825	311563	25.29%	2.535%
19	12.605	1546	1552	1559	rVB2	23653	39333	3.19%	0.320%
20	12.676	1559	1564	1570	rBV4	3243	6321	0.51%	0.051%
21	13.528	1703	1709	1710	rBV	2372	2272	0.18%	0.018%
22	13.962	1779	1783	1787	rVB	2296	2907	0.24%	0.024%
23	14.297	1831	1840	1847	rBV	453356	663076	53.82%	5.395%
24	14.603	1886	1892	1900	rBV	479945	778121	63.16%	6.331%
25	14.908	1937	1944	1954	rVB	385464	604227	49.05%	4.916%
26	15.073	1966	1972	1986	rBV2	43182	77046	6.25%	0.627%
27	15.302	2008	2011	2012	rBV2	1798	1642	0.13%	0.013%
28	15.625	2062	2066	2071	rVB	6052	8426	0.68%	0.069%
29	15.690	2074	2077	2082	rVB2	1407	1856	0.15%	0.015%
30	15.895	2105	2112	2121	rBV	608213	964624	78.30%	7.848%
31	16.001	2123	2130	2139	rVV	175143	265873	21.58%	2.163%
32	16.136	2149	2153	2159	rBV3	2503	3695	0.30%	0.030%
33	16.624	2232	2236	2240	rVB3	1845	2411	0.20%	0.020%
34	17.446	2370	2376	2382	rBV3	4143	6501	0.53%	0.053%
35	17.657	2405	2412	2419	rBV	484660	743990	60.39%	6.053%
36	17.757	2422	2429	2436	rBV2	686140	1050329	85.26%	8.546%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051744.D
 Acq On : 22 Dec 2021 10:28
 Operator : CG/JU
 Sample : M5090-01
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3C0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	18.104	2485	2488	2490	rBV2	996	1625	0.13%	0.013%
38	18.909	2622	2625	2627	rBV2	1321	1840	0.15%	0.015%
39	19.308	2690	2693	2695	rBV3	2230	2796	0.23%	0.023%
40	19.526	2727	2730	2731	rBV3	1586	1757	0.14%	0.014%
41	19.602	2739	2743	2747	rVB5	10269	16261	1.32%	0.132%
42	19.667	2747	2754	2759	rBV2	9083	16825	1.37%	0.137%
43	19.725	2762	2764	2766	rBV3	1562	1636	0.13%	0.013%
44	19.925	2795	2798	2801	rBV4	3305	4712	0.38%	0.038%
45	20.031	2808	2816	2826	rBV	844825	1231976	100.00%	10.024%
46	20.136	2831	2834	2835	rBV3	2440	1898	0.15%	0.015%
47	21.975	3140	3147	3156	rBV	443709	781940	63.47%	6.362%
48	22.839	3289	3294	3297	rBV7	7068	14141	1.15%	0.115%
49	24.254	3533	3535	3537	rBV3	3937	3571	0.29%	0.029%
50	24.484	3570	3574	3580	rVB4	12338	25547	2.07%	0.208%
51	25.241	3691	3703	3716	rVB2	383097	1138554	92.42%	9.264%
52	25.476	3732	3743	3760	rBV2	239757	786906	63.87%	6.402%
53	26.798	3961	3968	3975	rVB6	12704	38122	3.09%	0.310%
54	28.948	4332	4334	4336	rBV3	3156	2653	0.22%	0.022%
55	29.365	4404	4405	4406	rBV	3840	1855	0.15%	0.015%




Sum of corrected areas: 12290665

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051744.D
Acq On : 22 Dec 2021 10:28
Operator : CG/JU
Sample : M5090-01
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3C0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

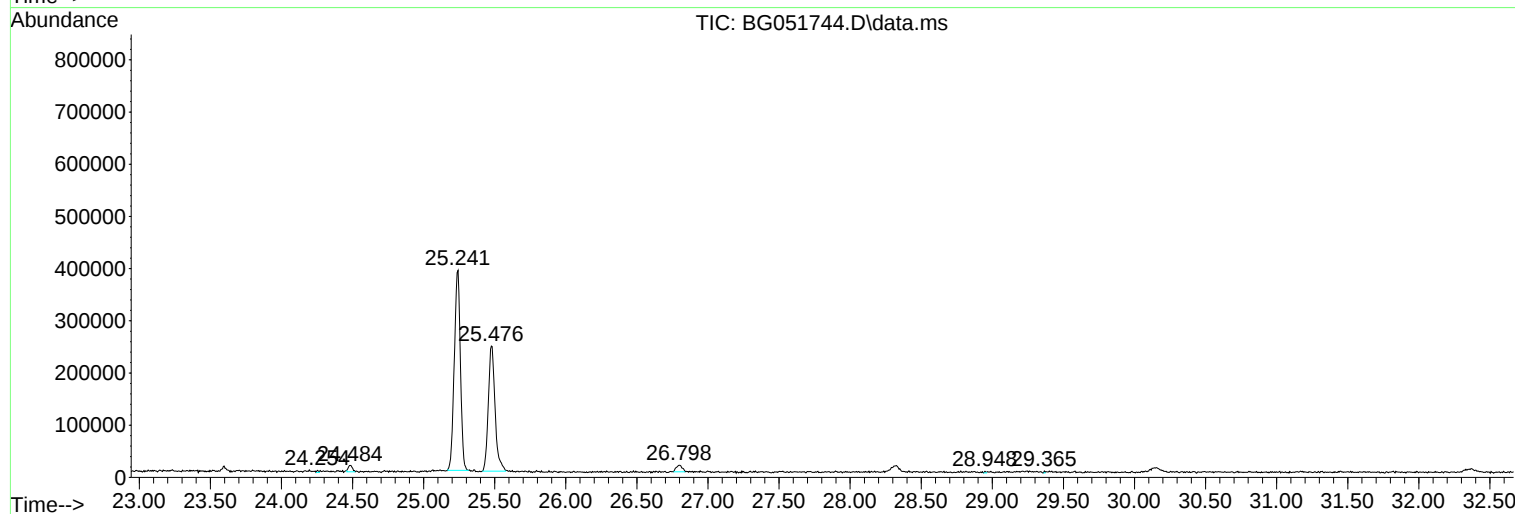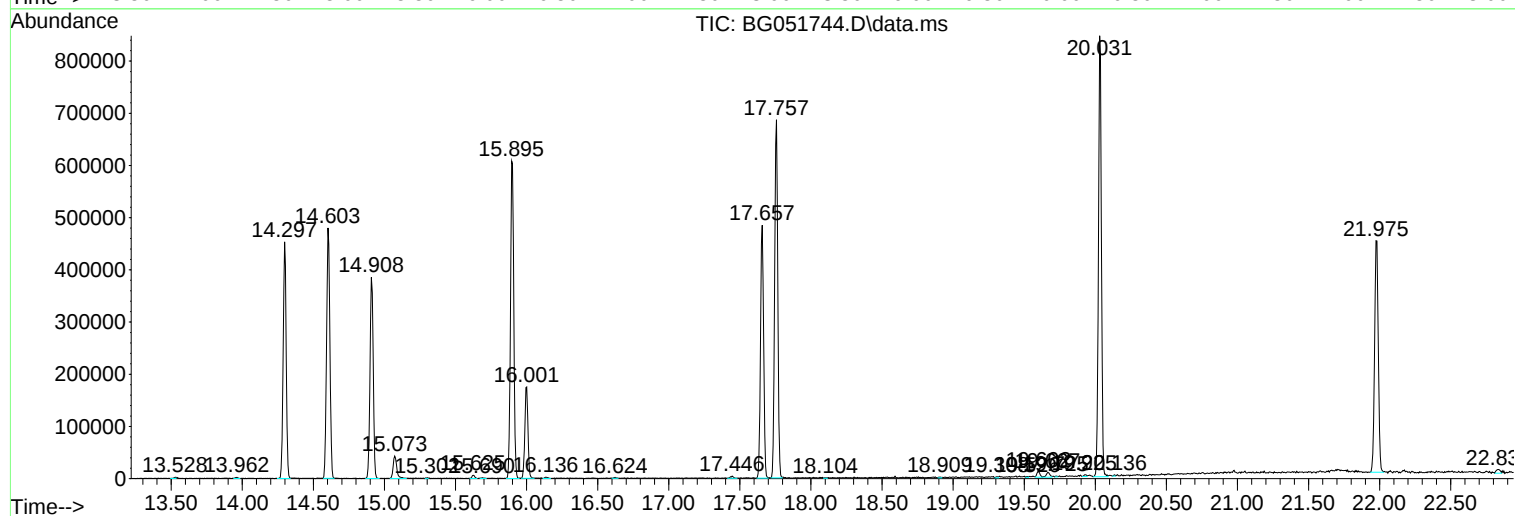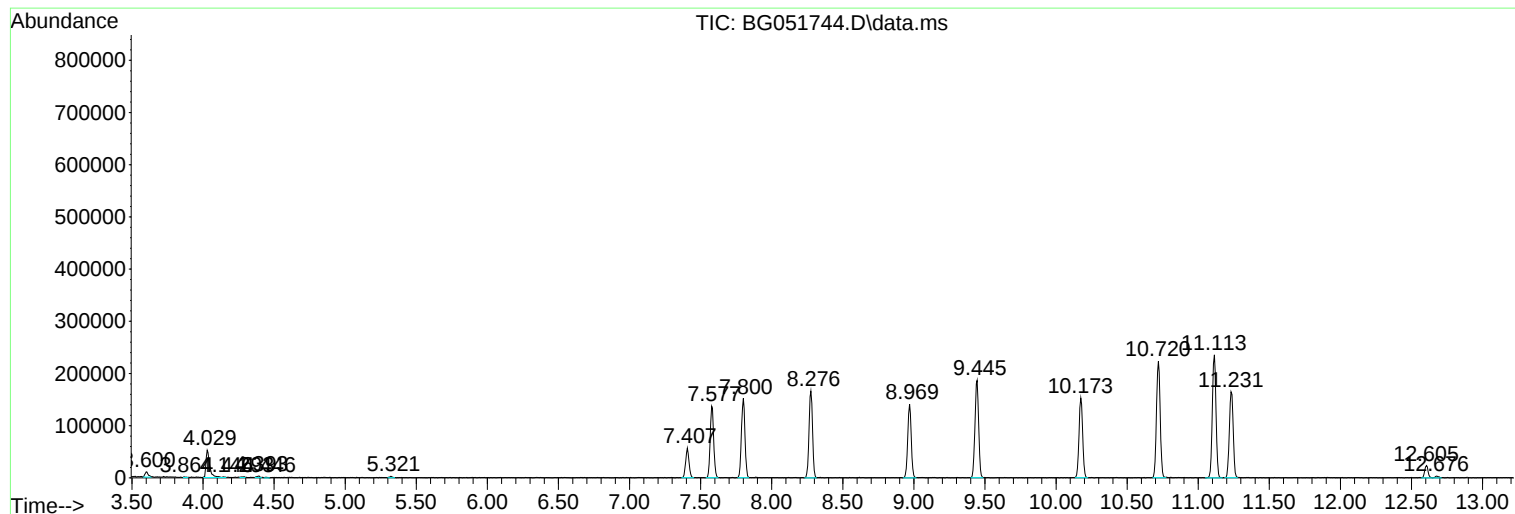

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051744.D
Acq On : 22 Dec 2021 10:28
Operator : CG/JU
Sample : M5090-01
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3C0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051744.D
Acq On : 22 Dec 2021 10:28
Operator : CG/JU
Sample : M5090-01
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3C0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc