

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051745.D
 Acq On : 22 Dec 2021 11:09
 Operator : CG/JU
 Sample : M5090-05
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3D3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051745.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.599	15	19	28	rVB	11293	18374	1.15%	0.125%
2	4.028	88	92	107	rBV	52922	92131	5.78%	0.627%
3	4.281	131	135	139	rBV2	2535	3472	0.22%	0.024%
4	4.380	147	152	153	rBV3	2536	3387	0.21%	0.023%
5	5.326	308	313	315	rBV2	1816	2634	0.17%	0.018%
6	7.406	661	667	677	rBV	68767	125971	7.91%	0.857%
7	7.576	688	696	704	rBV	159229	275092	17.27%	1.872%
8	7.799	727	734	743	rBV2	180785	310333	19.49%	2.112%
9	8.275	808	815	822	rBV	169342	287071	18.02%	1.954%
10	8.968	926	933	942	rVB	172630	294148	18.47%	2.002%
11	9.444	1006	1014	1023	rVB	219941	402048	25.24%	2.736%
12	9.861	1080	1085	1090	rBV3	3874	5346	0.34%	0.036%
13	10.173	1130	1138	1148	rVB	175499	323217	20.29%	2.200%
14	10.719	1224	1231	1244	rBV	272876	491895	30.89%	3.348%
15	10.860	1249	1255	1262	rVV2	5335	8881	0.56%	0.060%
16	11.112	1290	1298	1305	rBV	241574	429923	26.99%	2.926%
17	11.230	1310	1318	1328	rBV	228715	426908	26.81%	2.906%
18	12.681	1560	1565	1571	rVB3	4930	7354	0.46%	0.050%
19	13.527	1701	1709	1714	rBV4	2856	5689	0.36%	0.039%
20	13.727	1738	1743	1749	rVV4	4485	7003	0.44%	0.048%
21	13.803	1752	1756	1762	rVB4	9329	14135	0.89%	0.096%
22	14.296	1834	1840	1847	rBV	560377	829580	52.09%	5.646%
23	14.531	1874	1880	1885	rBV4	4056	7535	0.47%	0.051%
24	14.608	1886	1893	1901	rVB	575454	930999	58.46%	6.336%
25	14.790	1920	1924	1928	rVB2	2634	4043	0.25%	0.028%
26	14.913	1936	1945	1952	rBV	388513	631750	39.67%	4.300%
27	15.072	1966	1972	1979	rBV	64852	108634	6.82%	0.739%
28	15.307	2008	2012	2016	rBV3	1880	2402	0.15%	0.016%
29	15.624	2062	2066	2070	rBV3	2416	3512	0.22%	0.024%
30	15.694	2072	2078	2082	rVV3	4956	8610	0.54%	0.059%
31	15.736	2082	2085	2089	rVB4	2707	3620	0.23%	0.025%
32	15.900	2106	2113	2124	rBV	808319	1201891	75.47%	8.180%
33	16.000	2124	2130	2138	rBV2	232858	355205	22.30%	2.418%
34	16.135	2150	2153	2158	rVB6	3399	5451	0.34%	0.037%
35	16.294	2177	2180	2183	rVB2	2105	2392	0.15%	0.016%
36	16.576	2224	2228	2229	rBV2	2422	3013	0.19%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051745.D
 Acq On : 22 Dec 2021 11:09
 Operator : CG/JU
 Sample : M5090-05
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3D3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	16.675	2241	2245	2248	rVB4	2105	2825	0.18%	0.019%
38	16.781	2259	2263	2266	rVB4	2457	3306	0.21%	0.023%
39	16.887	2278	2281	2286	rVB2	1623	2187	0.14%	0.015%
40	16.957	2289	2293	2296	rBV2	1569	2155	0.14%	0.015%
41	17.116	2316	2320	2322	rBV4	1979	2863	0.18%	0.019%
42	17.392	2363	2367	2370	rVB3	4768	4823	0.30%	0.033%
43	17.433	2372	2374	2381	rVB3	2919	3814	0.24%	0.026%
44	17.545	2387	2393	2398	rBV4	6670	10803	0.68%	0.074%
45	17.657	2406	2412	2421	rBV	521633	773026	48.54%	5.261%
46	17.756	2422	2429	2438	rVB	902905	1360561	85.43%	9.260%
47	17.921	2454	2457	2459	rBV3	1734	2412	0.15%	0.016%
48	18.126	2488	2492	2496	rBV4	2195	3979	0.25%	0.027%
49	18.309	2519	2523	2526	rBV5	8832	8526	0.54%	0.058%
50	18.520	2556	2559	2563	rBV3	7558	8814	0.55%	0.060%
51	18.779	2601	2603	2607	rVB4	2571	2463	0.15%	0.017%
52	18.808	2607	2608	2611	rBV2	2664	2870	0.18%	0.020%
53	19.601	2739	2743	2747	rBV4	11737	19048	1.20%	0.130%
54	19.666	2750	2754	2762	rVB2	13405	19944	1.25%	0.136%
55	19.742	2765	2767	2770	rVB3	2904	3116	0.20%	0.021%
56	19.783	2772	2774	2778	rBV5	3315	3910	0.25%	0.027%
57	20.036	2810	2817	2825	rVB	1101377	1592634	100.00%	10.840%
58	21.980	3140	3148	3156	rVB	462761	808960	50.79%	5.506%
59	22.168	3178	3180	3182	rBV2	4204	3177	0.20%	0.022%
60	24.483	3570	3574	3580	rVB4	16980	32095	2.02%	0.218%
61	25.240	3691	3703	3716	rVB2	517017	1531249	96.15%	10.422%
62	25.481	3733	3744	3764	rVB3	244870	842762	52.92%	5.736%
63	30.692	4629	4631	4633	rBV3	4022	2959	0.19%	0.020%
64	32.325	4907	4909	4910	rBV2	4992	3943	0.25%	0.027%




Sum of corrected areas: 14692873

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051745.D
Acq On : 22 Dec 2021 11:09
Operator : CG/JU
Sample : M5090-05
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3D3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

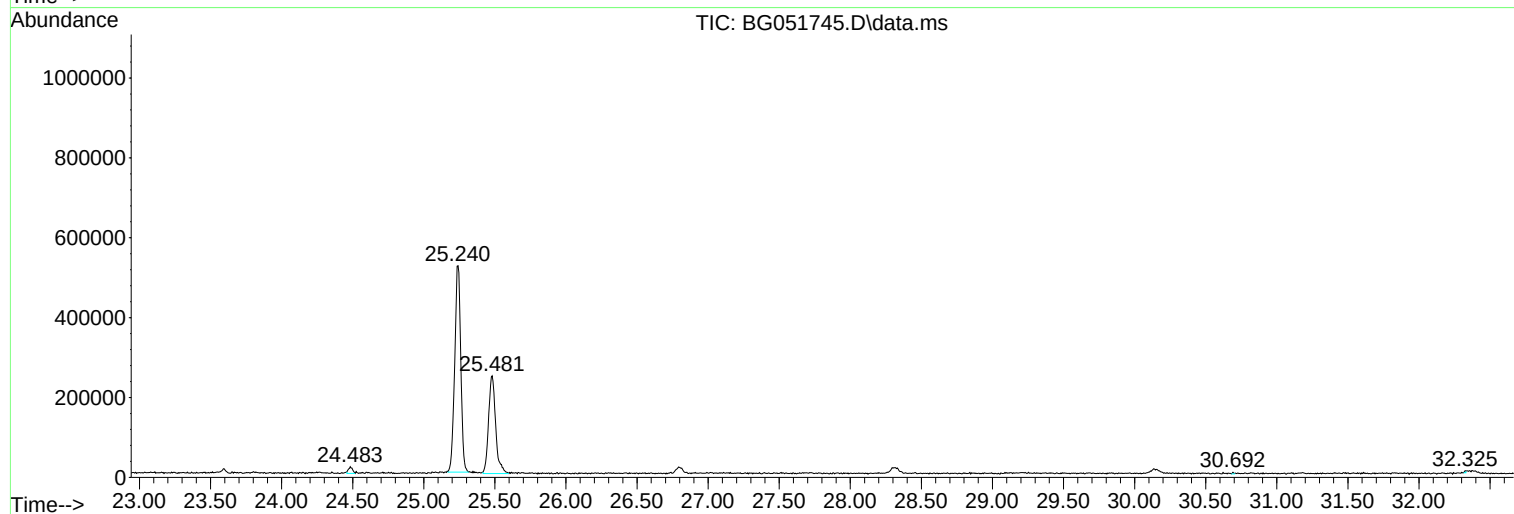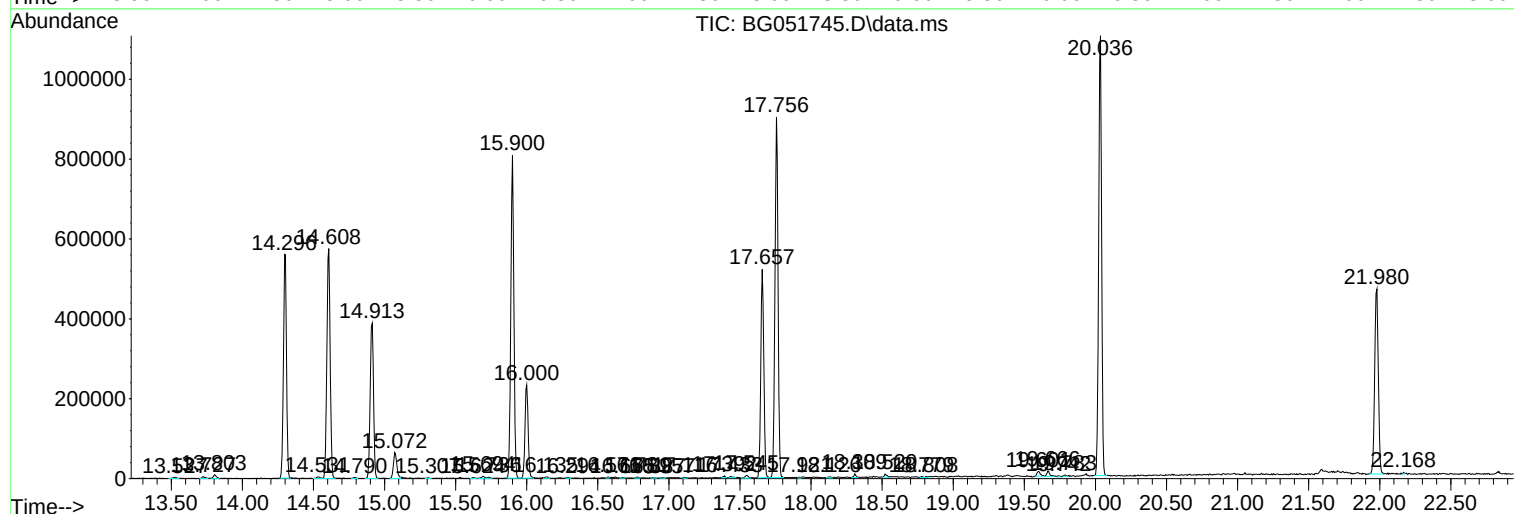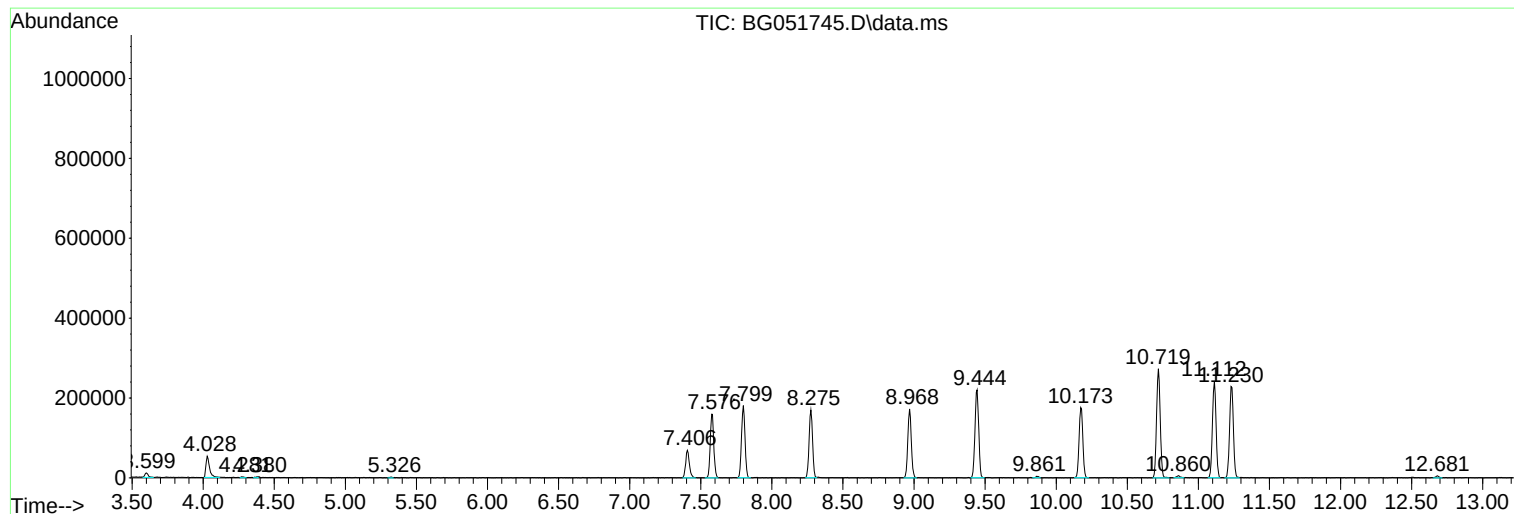

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051745.D
Acq On : 22 Dec 2021 11:09
Operator : CG/JU
Sample : M5090-05
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3D3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051745.D
Acq On : 22 Dec 2021 11:09
Operator : CG/JU
Sample : M5090-05
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3D3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc