

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051746.D
 Acq On : 22 Dec 2021 11:49
 Operator : CG/JU
 Sample : M5090-10
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3C3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051746.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.605	15	20	29	rVB2	9869	17622	1.23%	0.139%
2	4.033	89	93	105	rBV	32809	62933	4.41%	0.495%
3	4.386	145	153	156	rBV4	2317	3714	0.26%	0.029%
4	5.314	308	311	316	rBV	1562	2064	0.14%	0.016%
5	7.405	659	667	675	rBV	58989	101012	7.08%	0.795%
6	7.576	688	696	705	rBV	143305	241051	16.89%	1.896%
7	7.799	726	734	742	rBV	162714	278979	19.54%	2.195%
8	8.275	808	815	825	rVB	136667	238085	16.68%	1.873%
9	8.968	927	933	942	rVB	141218	245225	17.18%	1.929%
10	9.444	1006	1014	1021	rBV	202510	359047	25.15%	2.824%
11	10.178	1130	1139	1146	rBV	159862	289064	20.25%	2.274%
12	10.718	1221	1231	1245	rBV	234908	414297	29.02%	3.259%
13	11.112	1288	1298	1305	rVB	197354	349247	24.47%	2.747%
14	11.235	1311	1319	1326	rBV	166091	316741	22.19%	2.492%
15	12.681	1561	1565	1571	rBV3	3805	6104	0.43%	0.048%
16	13.538	1706	1711	1714	rVB2	3191	4180	0.29%	0.033%
17	14.296	1834	1840	1847	rBV	481317	709017	49.67%	5.578%
18	14.601	1885	1892	1901	rBV	496092	805468	56.43%	6.336%
19	14.913	1936	1945	1953	rVB	324123	513109	35.95%	4.036%
20	15.071	1967	1972	1986	rBV2	54637	95543	6.69%	0.752%
21	15.694	2073	2078	2081	rVB3	1670	2171	0.15%	0.017%
22	15.900	2104	2113	2121	rBV	706773	1070251	74.98%	8.419%
23	16.000	2124	2130	2137	rVV	209380	314117	22.01%	2.471%
24	16.141	2149	2154	2160	rVB2	2997	3181	0.22%	0.025%
25	17.445	2372	2376	2382	rBV4	1760	2546	0.18%	0.020%
26	17.656	2405	2412	2422	rVB	432483	635436	44.51%	4.999%
27	17.756	2422	2429	2437	rBV2	809786	1238343	86.75%	9.742%
28	18.314	2522	2524	2530	rVB4	2608	3102	0.22%	0.024%
29	19.595	2738	2742	2747	rBV2	10556	15131	1.06%	0.119%
30	19.665	2747	2754	2759	rVV	10194	14596	1.02%	0.115%
31	19.930	2796	2799	2804	rVB6	2656	3685	0.26%	0.029%
32	20.035	2810	2817	2826	rVV	970708	1427468	100.00%	11.229%
33	20.253	2850	2854	2856	rBV2	1989	2360	0.17%	0.019%
34	20.441	2883	2886	2888	rVB2	2114	2358	0.17%	0.019%
35	20.464	2888	2890	2891	rBV2	2057	2069	0.14%	0.016%
36	20.752	2937	2939	2942	rBV3	1573	2035	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051746.D
 Acq On : 22 Dec 2021 11:49
 Operator : CG/JU
 Sample : M5090-10
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3C3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	20.911	2964	2966	2970	rVB5	1888	2601	0.18%	0.020%
38	20.969	2974	2976	2977	rBV2	3066	2077	0.15%	0.016%
39	21.357	3040	3042	3046	rBV5	1772	2148	0.15%	0.017%
40	21.445	3055	3057	3058	rVV2	2915	2382	0.17%	0.019%

41	21.480	3062	3063	3065	rVB2	2967	2072	0.15%	0.016%
42	21.586	3077	3081	3084	rBV4	1761	2238	0.16%	0.018%
43	21.674	3093	3096	3098	rBV4	3017	4534	0.32%	0.036%
44	21.839	3122	3124	3128	rBV5	3059	4839	0.34%	0.038%
45	21.980	3140	3148	3156	rVB	385955	669170	46.88%	5.264%

46	22.109	3167	3170	3171	rBV3	3442	3493	0.24%	0.027%
47	22.831	3288	3293	3296	rBV6	3834	6673	0.47%	0.052%
48	22.984	3317	3319	3321	rVB3	2756	2243	0.16%	0.018%
49	23.307	3371	3374	3378	rBV5	2077	3634	0.25%	0.029%
50	23.595	3417	3423	3428	rVB6	7851	14805	1.04%	0.116%

51	23.660	3431	3434	3436	rBV4	3102	2913	0.20%	0.023%
52	23.713	3439	3443	3445	rBV4	2015	2823	0.20%	0.022%
53	23.942	3479	3482	3484	rBV3	2720	2836	0.20%	0.022%
54	24.065	3502	3503	3507	rBV4	2588	2567	0.18%	0.020%
55	24.476	3568	3573	3583	rVB8	10499	26281	1.84%	0.207%

56	24.564	3587	3588	3591	rBV3	2313	2118	0.15%	0.017%
57	24.770	3621	3623	3625	rBV2	2149	2351	0.16%	0.018%
58	24.805	3628	3629	3631	rBV2	2691	2068	0.14%	0.016%
59	24.917	3646	3648	3650	rBV3	2467	2317	0.16%	0.018%
60	25.128	3682	3684	3687	rBV4	2117	2221	0.16%	0.017%

61	25.234	3690	3702	3715	rVV2	447712	1337458	93.69%	10.521%
62	25.481	3731	3744	3764	rBV2	199627	683553	47.89%	5.377%
63	25.945	3821	3823	3825	rVB3	2405	2123	0.15%	0.017%
64	26.344	3889	3891	3894	rVB4	3345	3172	0.22%	0.025%
65	26.385	3894	3898	3900	rBV5	2282	3802	0.27%	0.030%

66	26.779	3960	3965	3966	rBV4	10089	12698	0.89%	0.100%
67	26.955	3991	3995	3997	rBV4	1826	2187	0.15%	0.017%
68	27.196	4033	4036	4039	rBV3	2538	3583	0.25%	0.028%
69	27.267	4047	4048	4050	rBV2	2324	2077	0.15%	0.016%
70	27.431	4075	4076	4081	rVB4	2177	2449	0.17%	0.019%

71	27.572	4098	4100	4103	rVB4	2270	2201	0.15%	0.017%
72	27.819	4140	4142	4146	rBV5	2717	3677	0.26%	0.029%
73	27.960	4163	4166	4169	rBV4	2746	4602	0.32%	0.036%
74	28.189	4203	4205	4209	rVB4	2408	2235	0.16%	0.018%
75	28.218	4209	4210	4213	rBV3	2103	2429	0.17%	0.019%

76	28.306	4218	4225	4226	rBV7	10823	17250	1.21%	0.136%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
 Data File : BG051746.D
 Acq On : 22 Dec 2021 11:49
 Operator : CG/JU
 Sample : M5090-10
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG3C3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	28.418	4242	4244	4248	rBV5	2774	2690	0.19%	0.021%
78	28.541	4263	4265	4268	rBV3	2666	2421	0.17%	0.019%
79	28.624	4277	4279	4282	rBV4	2644	2709	0.19%	0.021%
80	28.729	4295	4297	4299	rVB3	2450	2306	0.16%	0.018%
81	29.052	4351	4352	4355	rVV3	2394	2101	0.15%	0.017%
82	29.105	4357	4361	4365	rBV6	1537	2631	0.18%	0.021%
83	29.334	4399	4400	4403	rBV	1925	2085	0.15%	0.016%
84	29.458	4419	4421	4424	rBV4	2043	2253	0.16%	0.018%
85	29.951	4503	4505	4507	rVV3	3578	2708	0.19%	0.021%
86	30.104	4529	4531	4532	rBV2	3334	2932	0.21%	0.023%
87	30.145	4532	4538	4540	rVV7	4688	8116	0.57%	0.064%
88	30.198	4546	4547	4549	rVB2	4192	2079	0.15%	0.016%
89	30.251	4554	4556	4558	rBV3	2892	2731	0.19%	0.021%
90	30.462	4589	4592	4593	rBV3	2425	2250	0.16%	0.018%
91	30.633	4619	4621	4623	rVB2	3646	2409	0.17%	0.019%
92	31.173	4711	4713	4717	rBV4	1793	2128	0.15%	0.017%
93	31.238	4722	4724	4727	rBV4	2337	2377	0.17%	0.019%
94	31.461	4760	4762	4765	rBV4	3038	2153	0.15%	0.017%
95	31.902	4835	4837	4841	rVB3	2266	2253	0.16%	0.018%
96	32.166	4880	4882	4885	rBV4	1551	2203	0.15%	0.017%
97	32.278	4899	4901	4904	rBV4	2771	2417	0.17%	0.019%
98	32.307	4904	4906	4907	rBV2	2595	2398	0.17%	0.019%
99	32.330	4908	4910	4911	rBV2	3572	2750	0.19%	0.022%
100	32.371	4915	4917	4919	rBV3	2413	2538	0.18%	0.020%




Sum of corrected areas: 12711889

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051746.D
Acq On : 22 Dec 2021 11:49
Operator : CG/JU
Sample : M5090-10
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3C3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

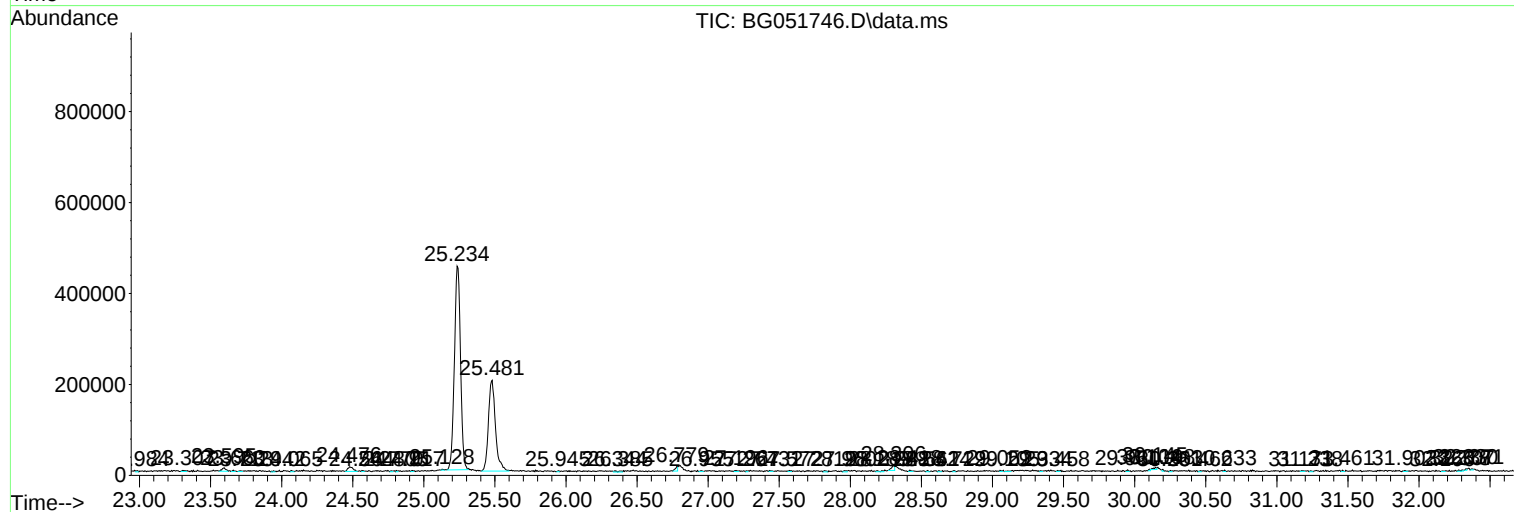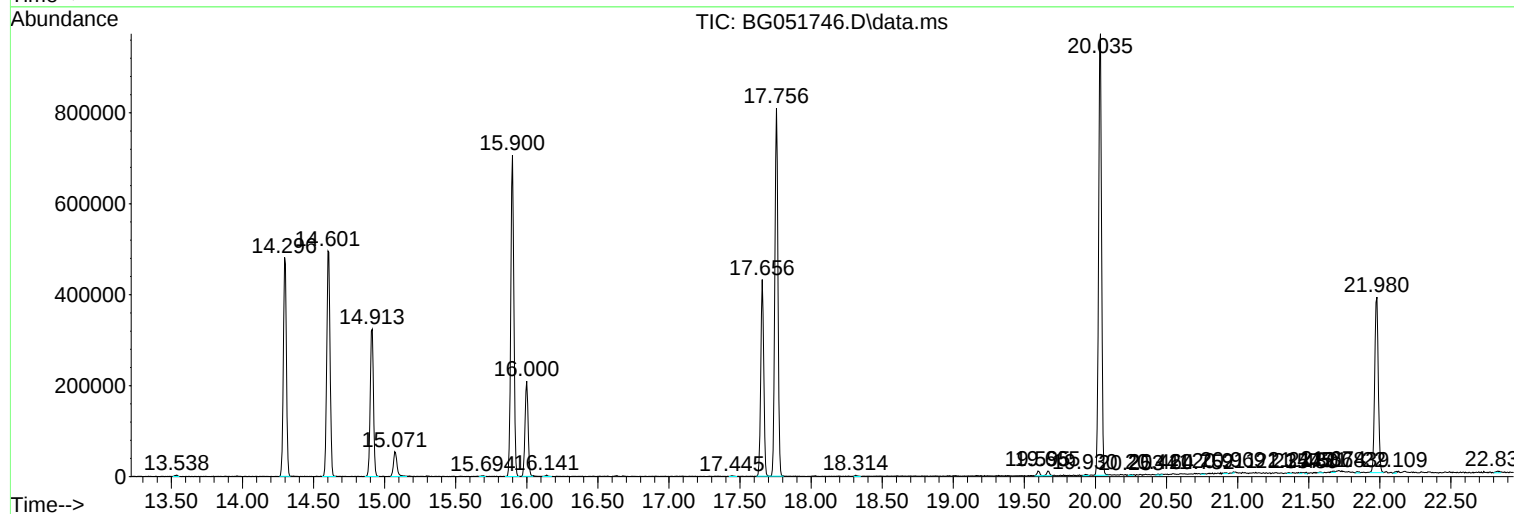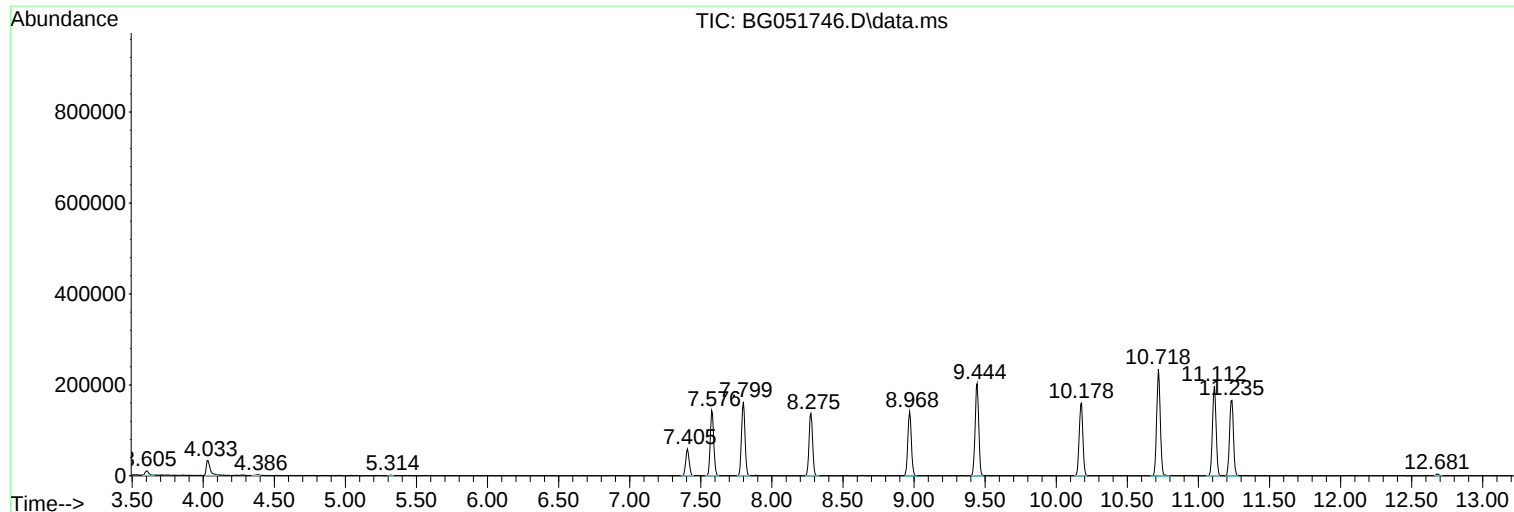

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051746.D
Acq On : 22 Dec 2021 11:49
Operator : CG/JU
Sample : M5090-10
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3C3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122021\
Data File : BG051746.D
Acq On : 22 Dec 2021 11:49
Operator : CG/JU
Sample : M5090-10
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG3C3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc