


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122022\
Data File : BG056024.D
Acq On : 20 Dec 2022 10:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 21 01:11:10 2022

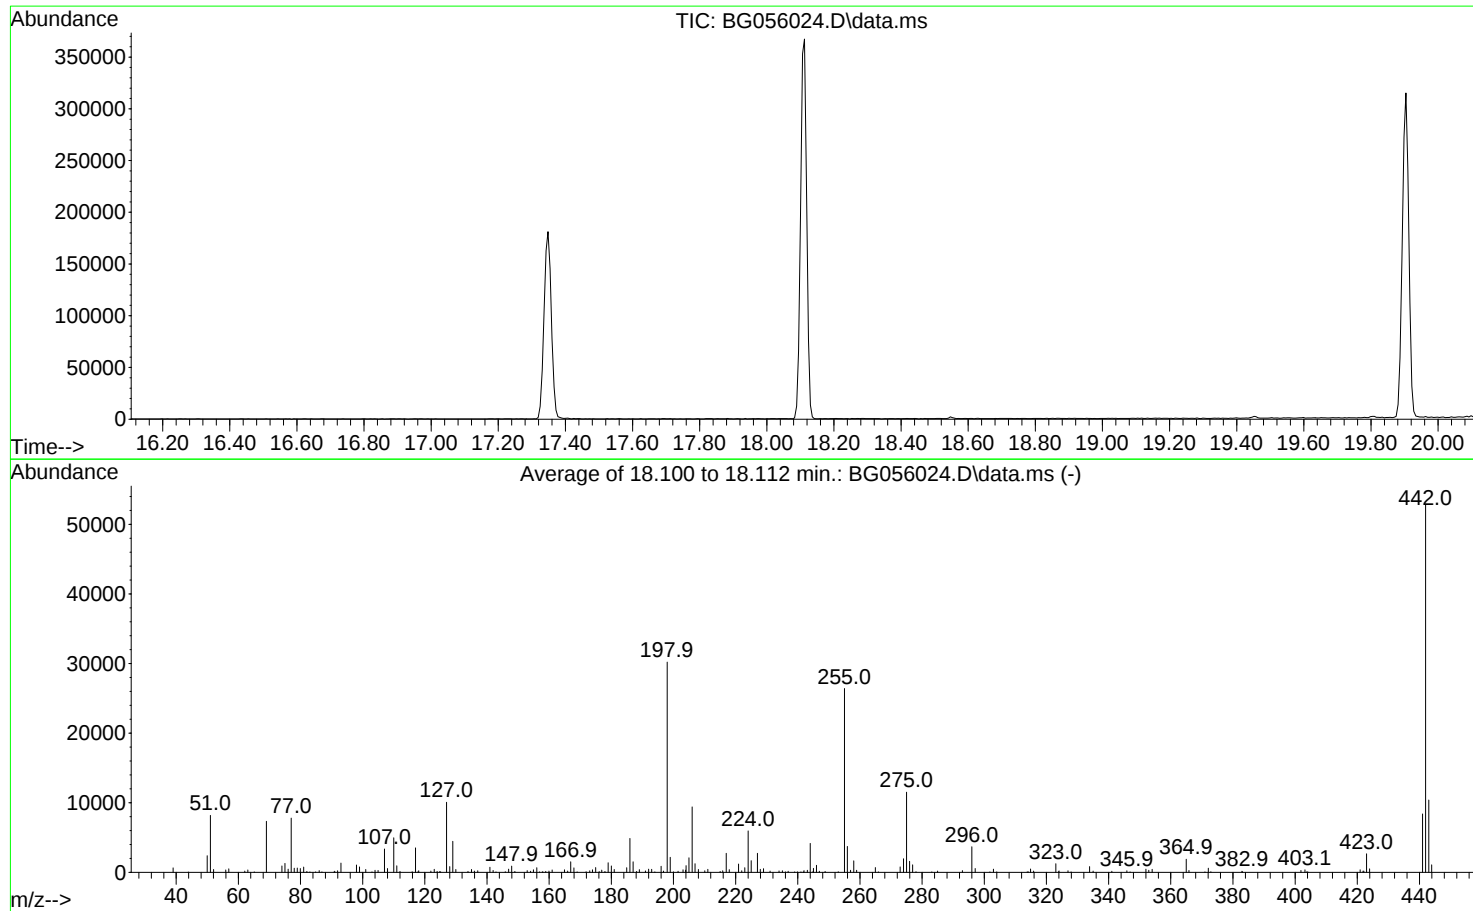




AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	8186	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	24.3	7324	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.3	10050	PASS
197	198	0.00	2	0.5	166	PASS
198	198	100	100	100.0	30192	PASS
199	198	5	9	7.1	2147	PASS
275	198	10	60	38.1	11505	PASS
365	198	1	100	6.2	1882	PASS
441	198	0.01	100	27.8	8385	PASS
442	442	50	100	100.0	52861	PASS
443	442	15	24	19.6	10377	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122022\
Data File : BG056024.D
Acq On : 20 Dec 2022 10:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 21 03:55:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 01:11:10 2022
Response via : Initial Calibration

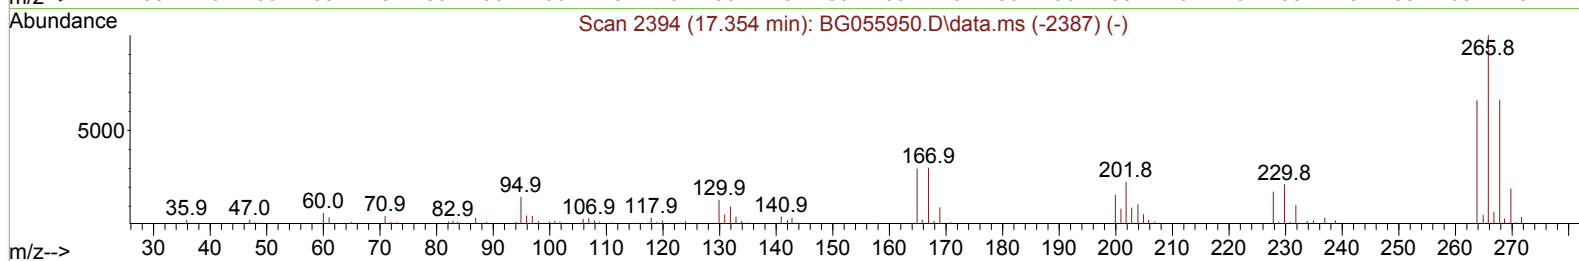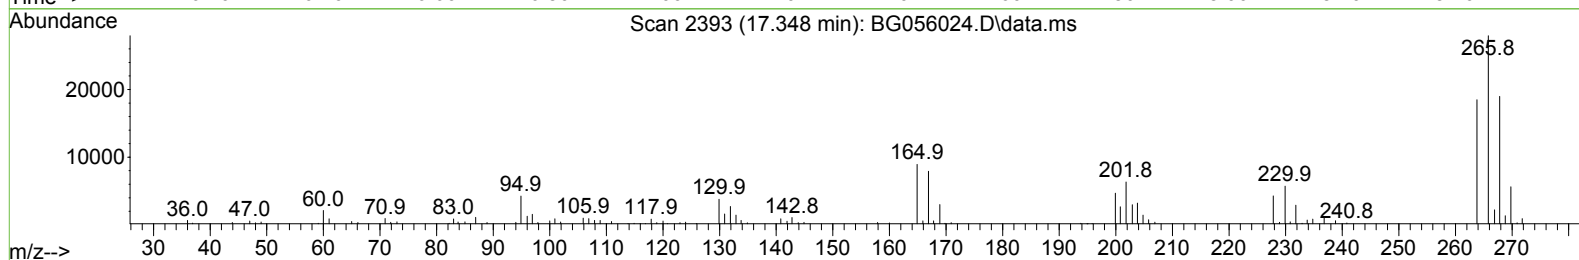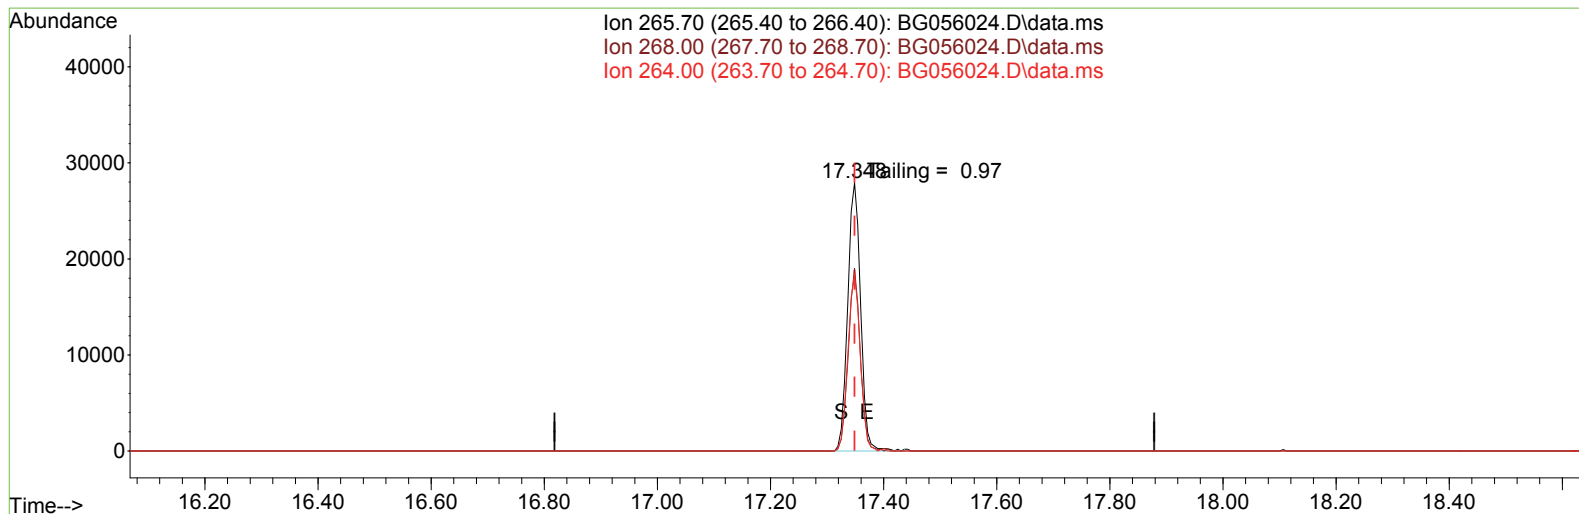

TIC: BG056024.D\data.ms

(70) Pentachlorophenol (C)

17.348min (-0.000) 33499.71 ng




response 44245

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.40	67.96
264.00	65.70	66.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122022\
Data File : BG056024.D
Acq On : 20 Dec 2022 10:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 21 03:55:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 01:11:10 2022
Response via : Initial Calibration

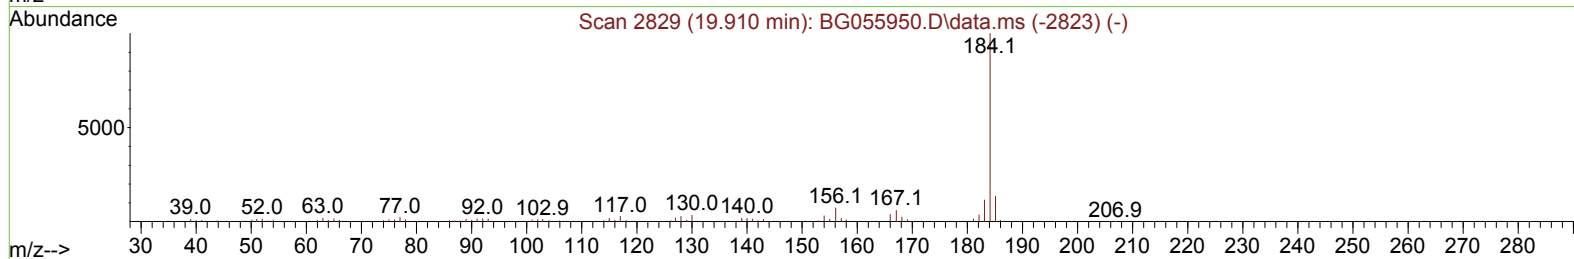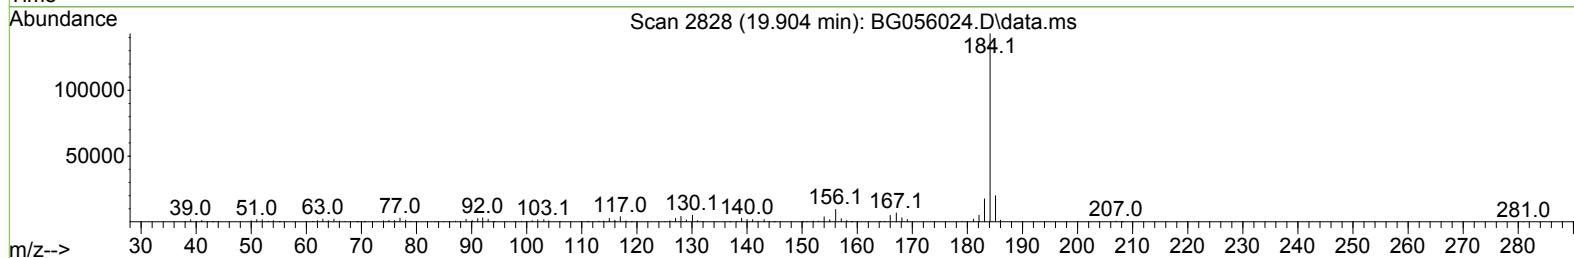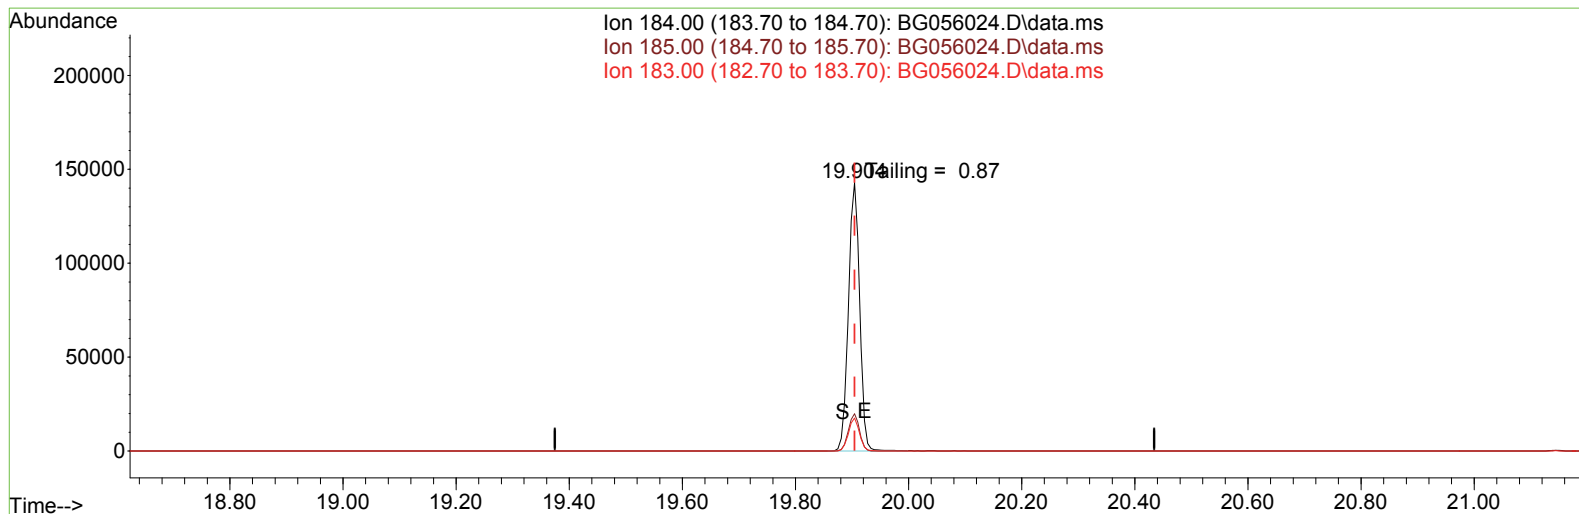

TIC: BG056024.D\data.ms

(77) Benzidine

19.904min (-0.000) 0.00 ng m

response 197424

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.93
183.00	11.50	12.29
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/20/2022	BNA_G	<u>BG056024.D</u>
Compound Name	Response	Retention Time
DDT	105120	21.144
DDD	1956	20.744
DDE	0	20.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1956	107076	1.83

Instrument :
BNA_G
ClientSampleId :
DFTPP