
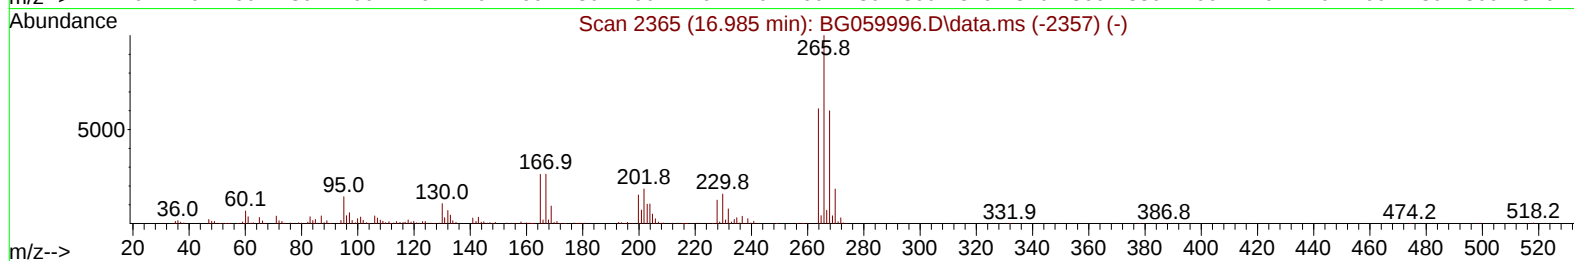
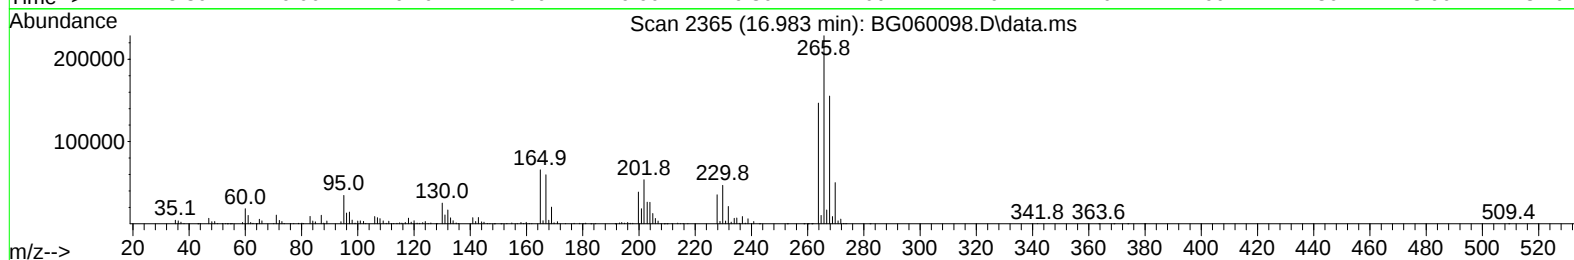


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122023\  
Data File : BG060098.D  
Acq On : 20 Dec 2023 9:59  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 12:30:48 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG121323.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 19 04:37:23 2023  
Response via : Initial Calibration

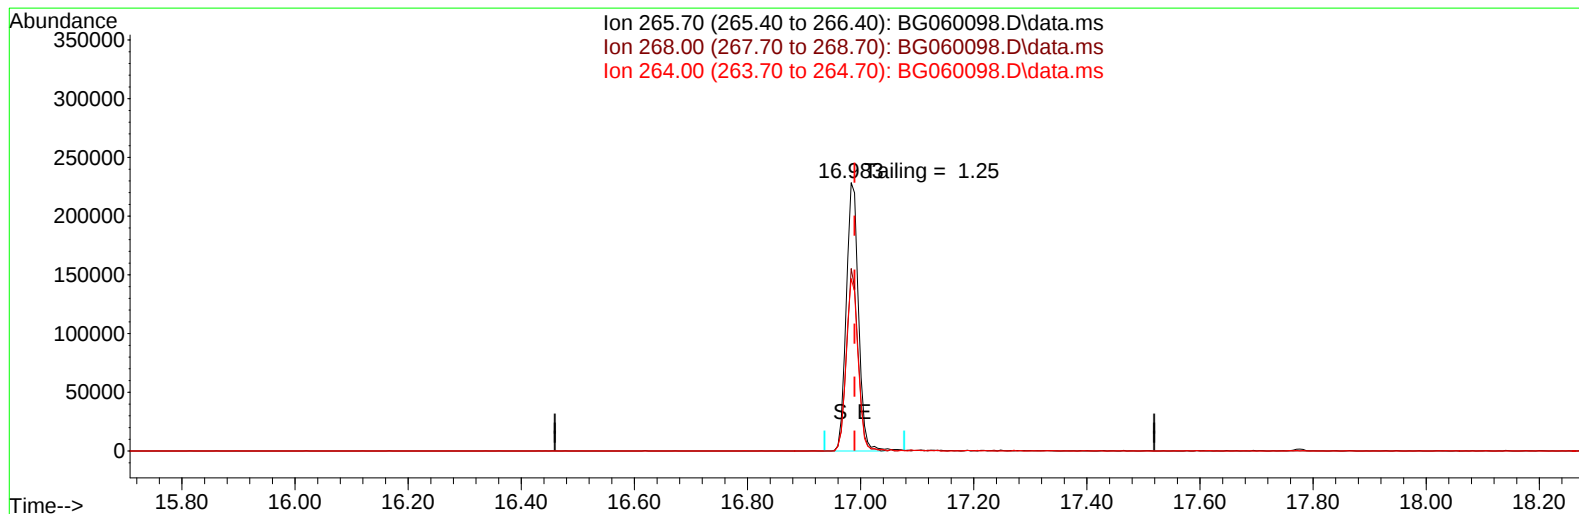

TIC: BG060098.D\data.ms

**(70) Pentachlorophenol (C)**




16.983min (-0.006) 301712.27 ng

response 344954

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 59.90  | 67.96  |
| 264.00 | 61.00  | 64.21  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122023\  
 Data File : BG060098.D  
 Acq On : 20 Dec 2023 9:59  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 12:30:48 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG121323.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Dec 19 04:37:23 2023  
 Response via : Initial Calibration

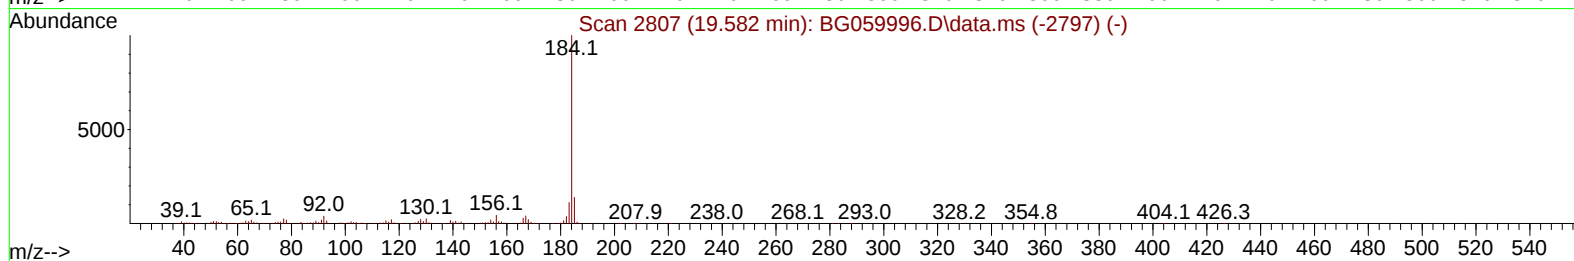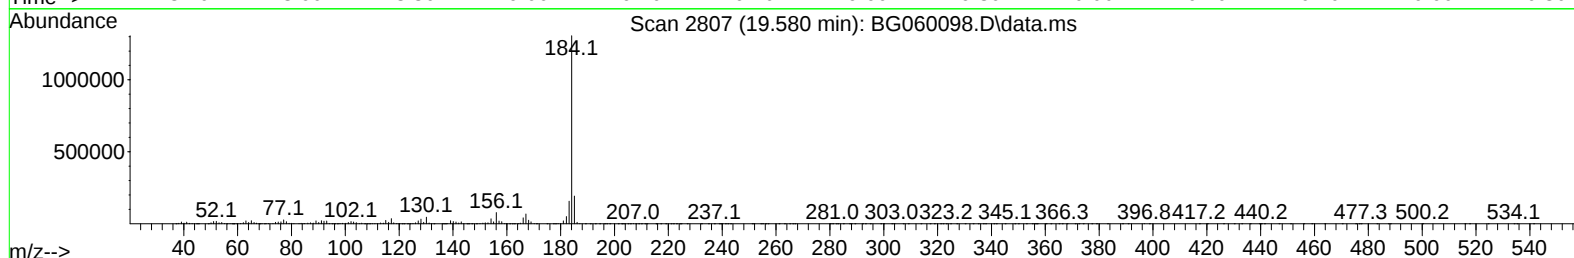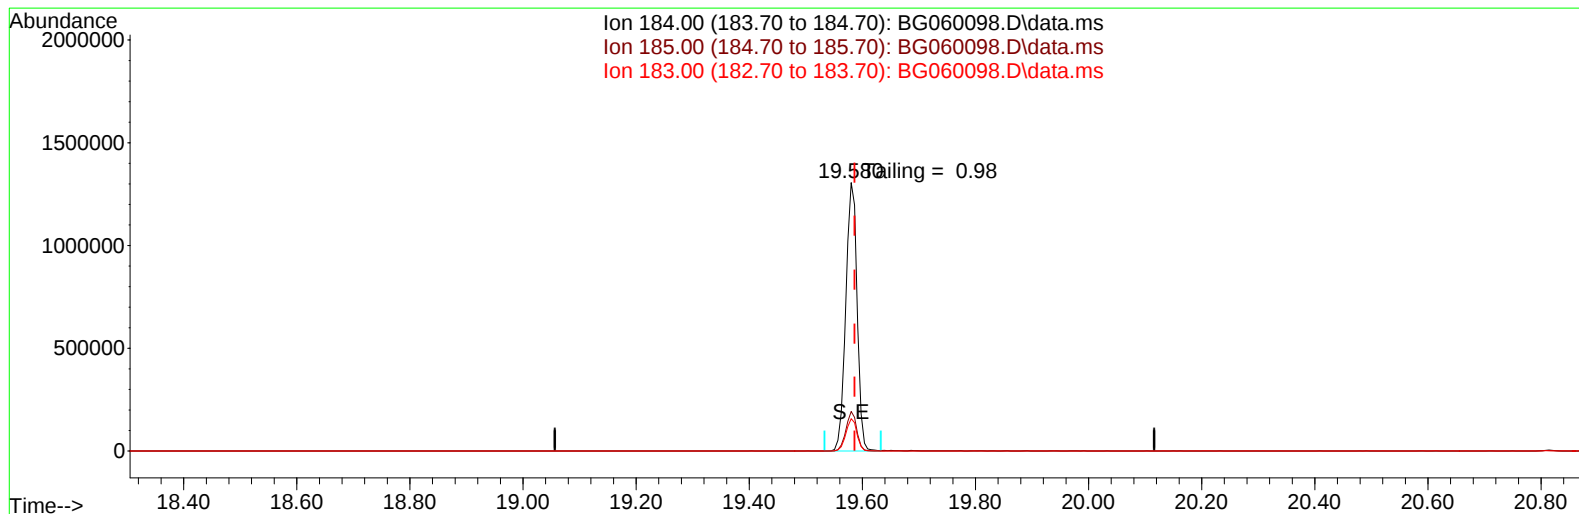

TIC: BG060098.D\data.ms

**(77) Benzidine****19.580min (-0.006) 326413.98 ng****response 1815437**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.90  | 14.72  |
| 183.00 | 11.20  | 12.04  |
| 0.00   | 0.00   | 0.00   |