
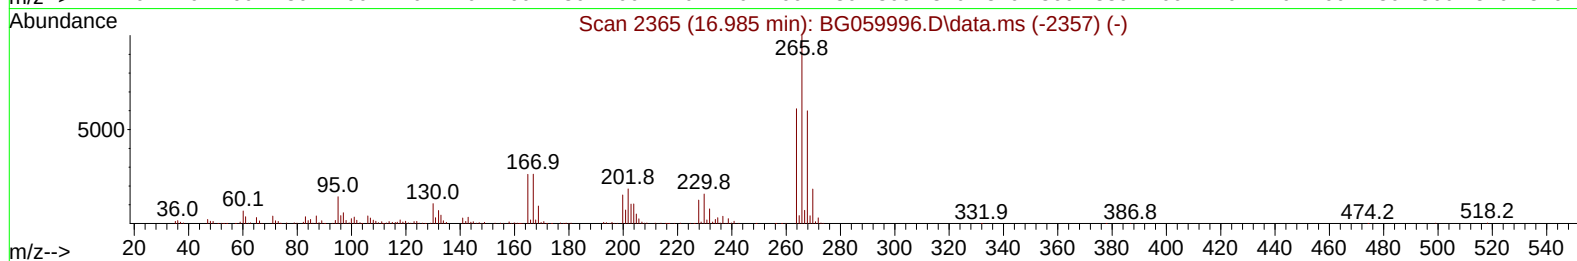
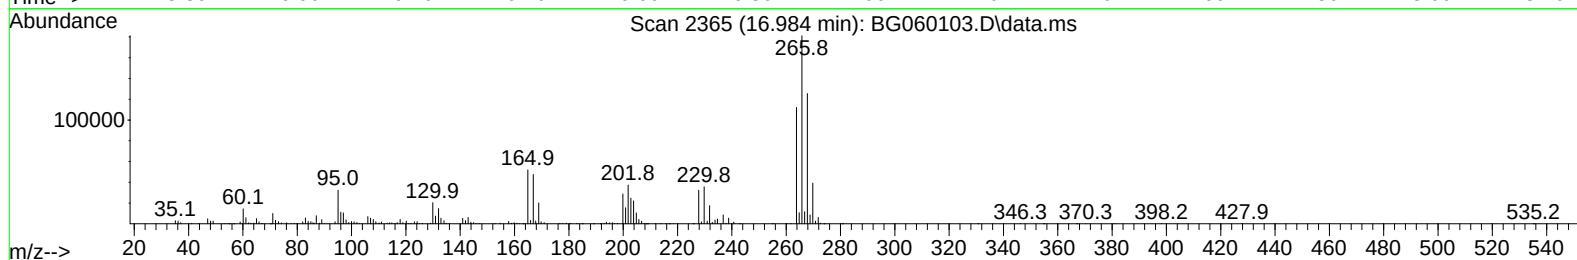


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122023\
Data File : BG060103.D
Acq On : 20 Dec 2023 17:04
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 17:51:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 04:37:23 2023
Response via : Initial Calibration

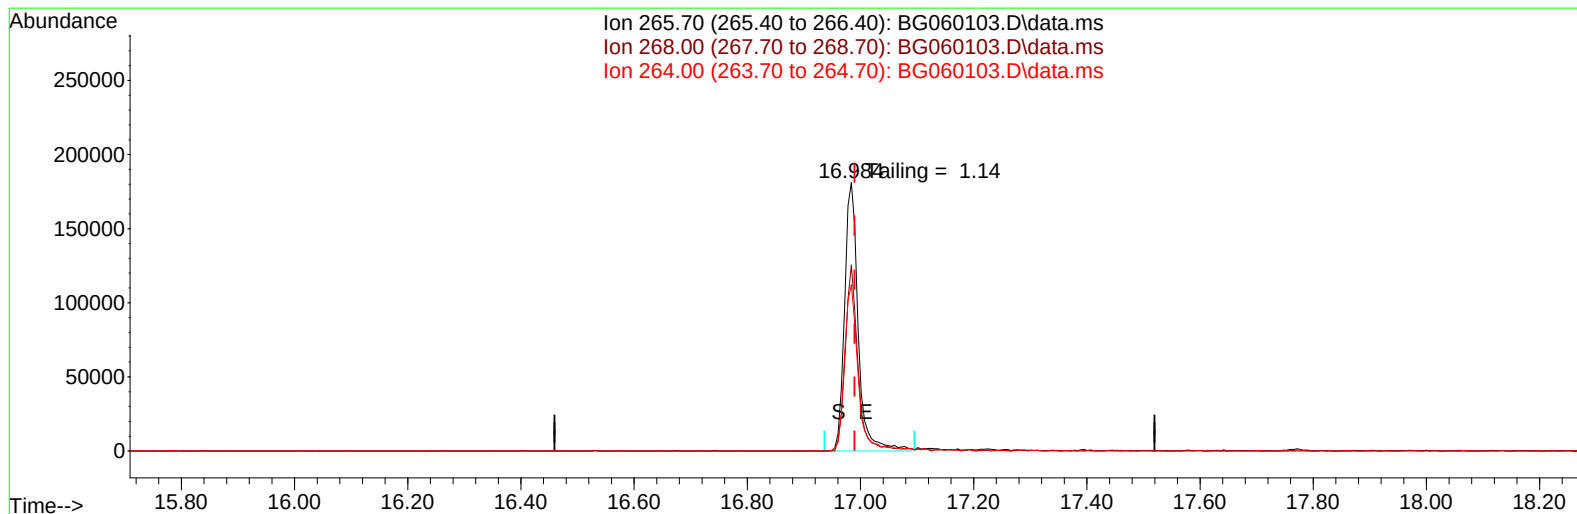

TIC: BG060103.D\data.ms

(70) Pentachlorophenol (C)




16.984min (-0.005) 429063.81 ng

response 302587

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	69.33
264.00	61.00	61.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122023\
Data File : BG060103.D
Acq On : 20 Dec 2023 17:04
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 17:51:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 04:37:23 2023
Response via : Initial Calibration

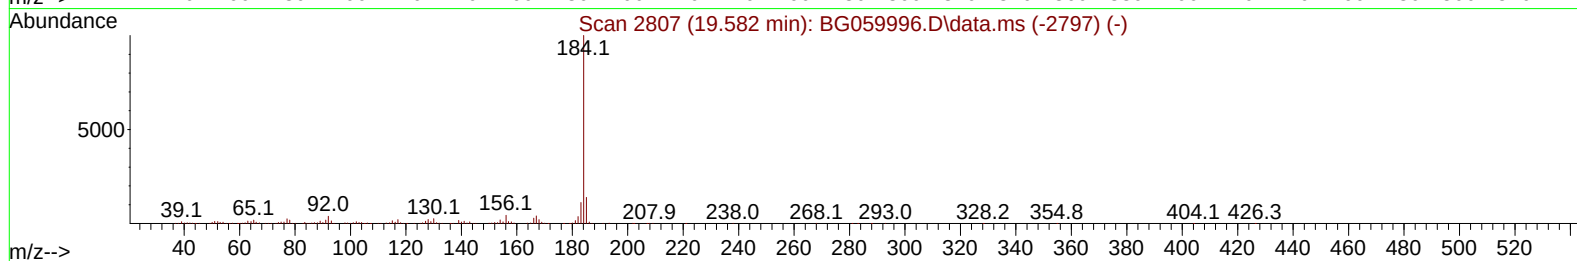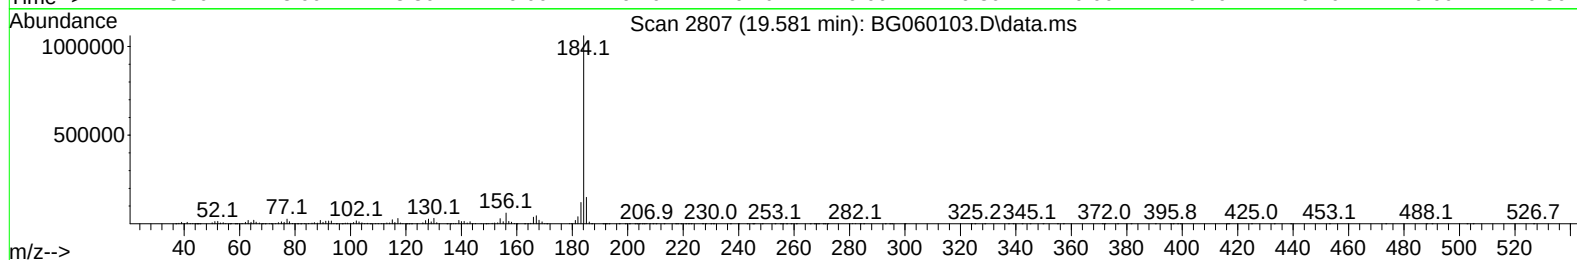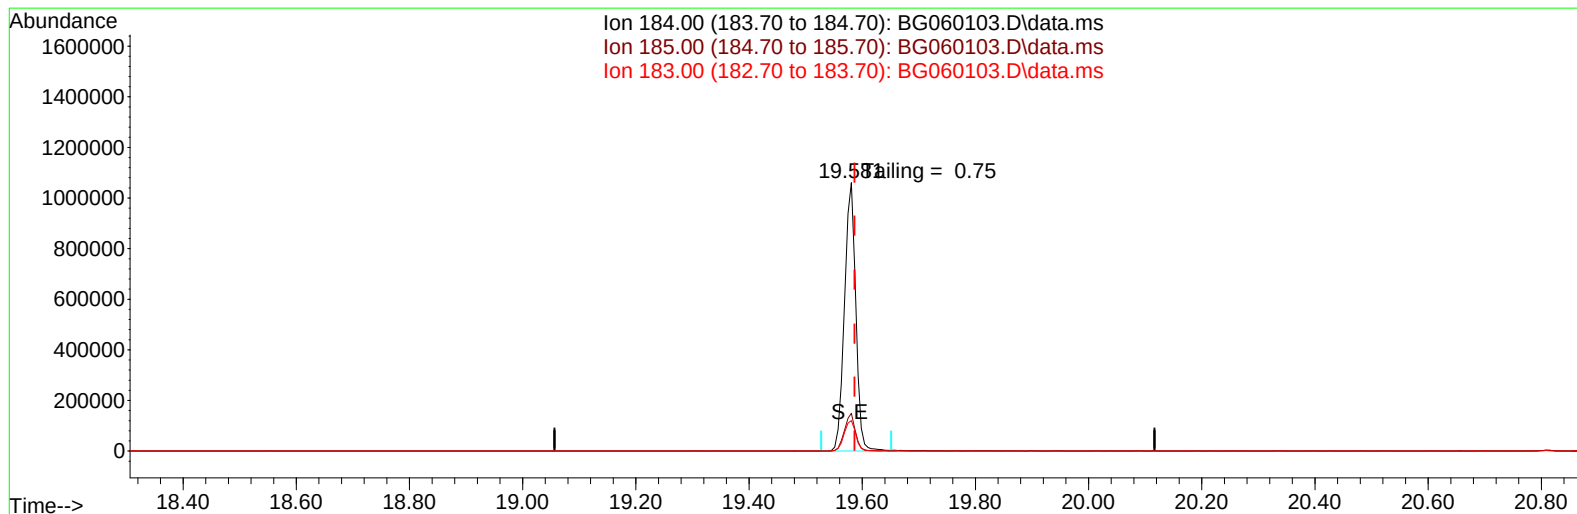

TIC: BG060103.D\data.ms

(77) Benzidine**19.581min (-0.005) 495881.43 ng****response 1464975**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.08
183.00	11.20	11.35
0.00	0.00	0.00