

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122023\
 Data File : BG060100.D
 Acq On : 20 Dec 2023 12:00
 Operator : MA/JU
 Sample : PB157861BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB157861BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060100.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.523	404	414	421	rBV	929204	1412307	15.24%	5.328%
2	7.109	677	684	692	rBV	1004711	1626528	17.55%	6.136%
3	7.950	819	827	833	rVB	181645	299806	3.23%	1.131%
4	9.113	1018	1025	1034	rVB	576349	1004439	10.84%	3.789%
5	10.752	1298	1304	1311	rVB	217000	394096	4.25%	1.487%
6	13.214	1716	1723	1729	rBV	2101273	3180017	34.30%	11.997%
7	14.589	1947	1957	1963	rBV	475234	714324	7.71%	2.695%
8	16.075	2203	2210	2218	rBV	2519512	3788821	40.87%	14.294%
9	17.339	2417	2425	2431	rBV	857745	1257655	13.57%	4.745%
10	19.959	2864	2871	2878	rBV	6861106	9269908	100.00%	34.973%
11	21.610	3145	3152	3158	rBV	1113832	1809907	19.52%	6.828%
12	24.794	3684	3694	3707	rVB	631725	1748238	18.86%	6.596%




Sum of corrected areas: 26506046

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122023\
Data File : BG060100.D
Acq On : 20 Dec 2023 12:00
Operator : MA/JU
Sample : PB157861BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157861BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

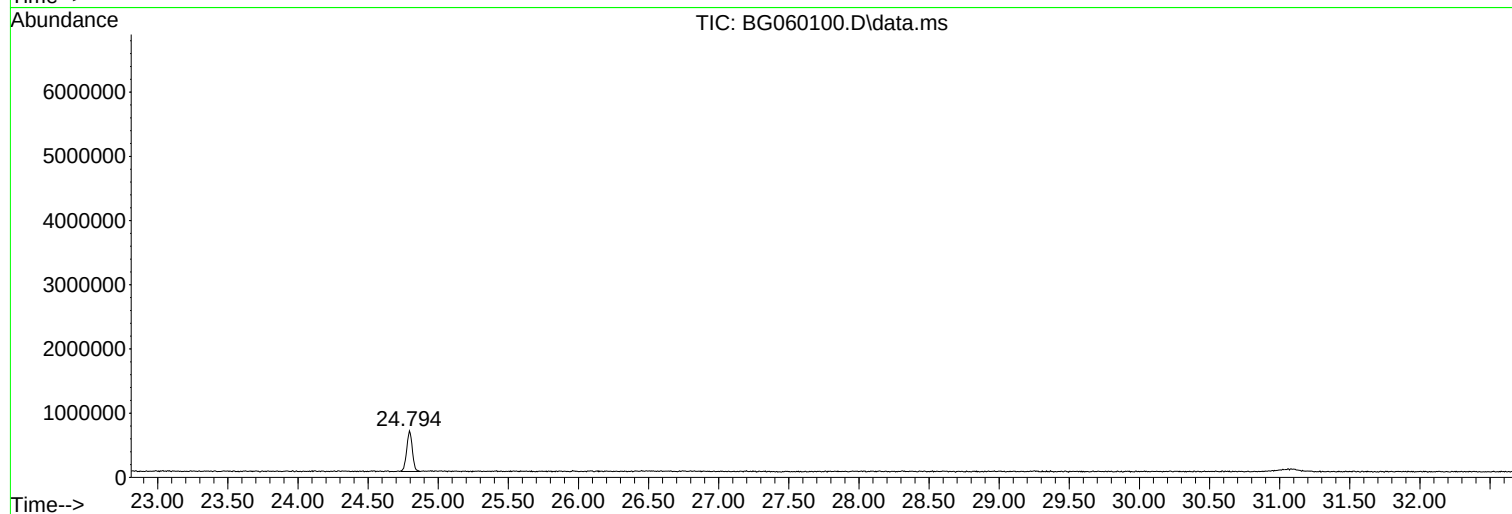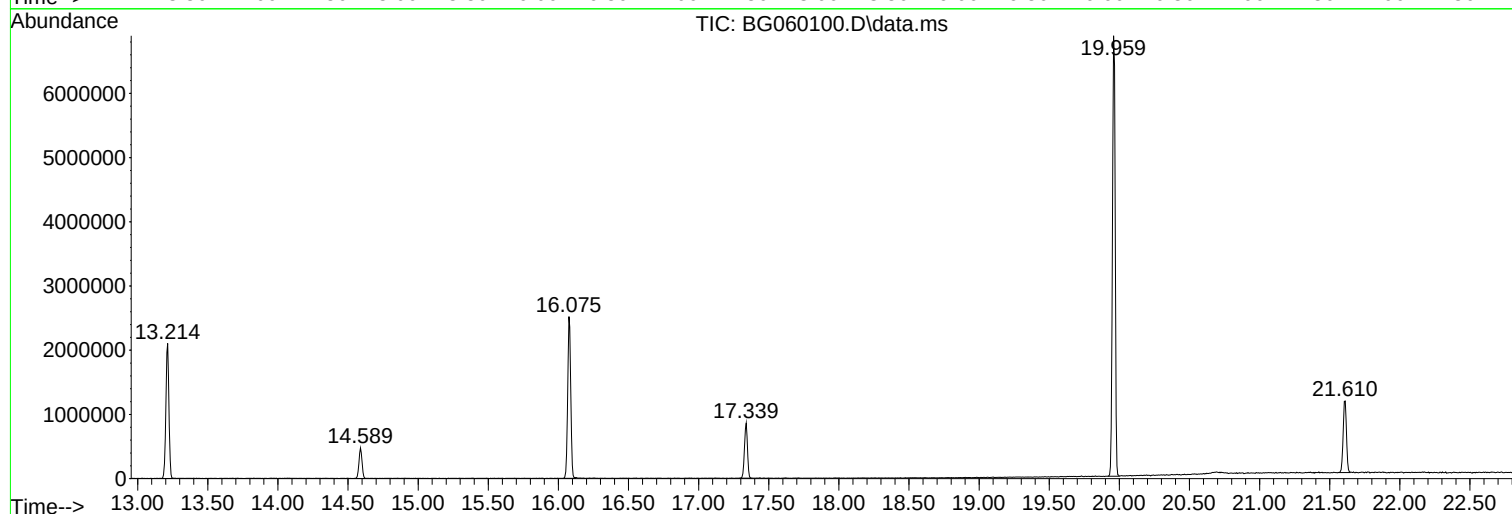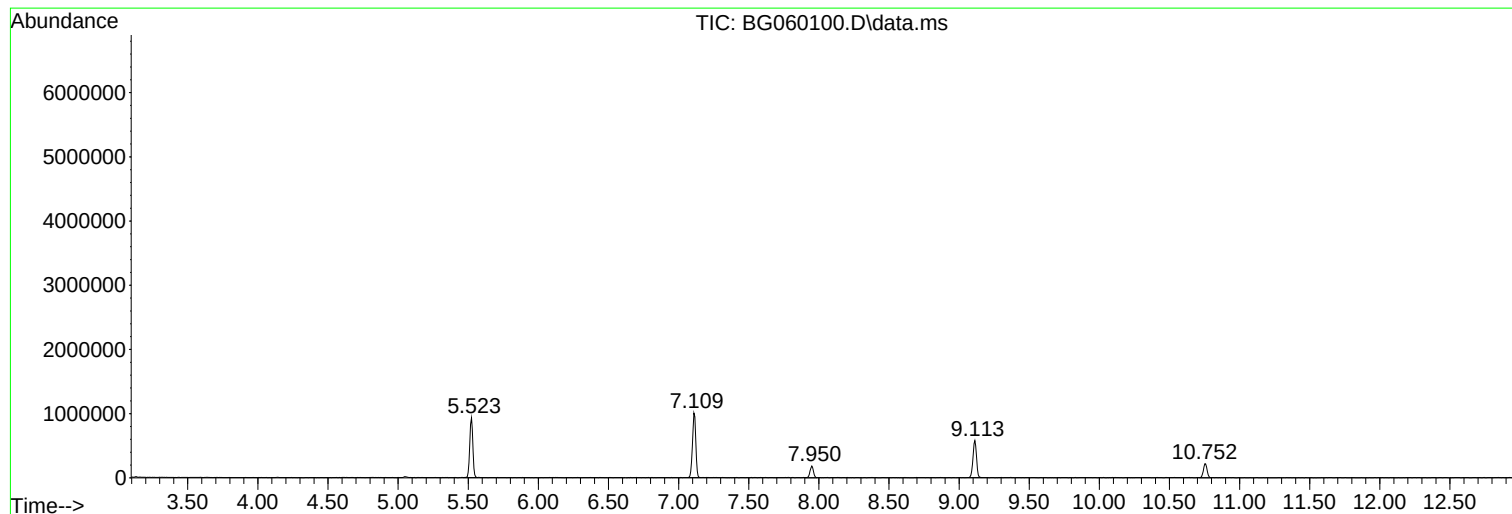

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122023\
Data File : BG060100.D
Acq On : 20 Dec 2023 12:00
Operator : MA/JU
Sample : PB157861BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157861BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122023\
Data File : BG060100.D
Acq On : 20 Dec 2023 12:00
Operator : MA/JU
Sample : PB157861BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157861BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------