
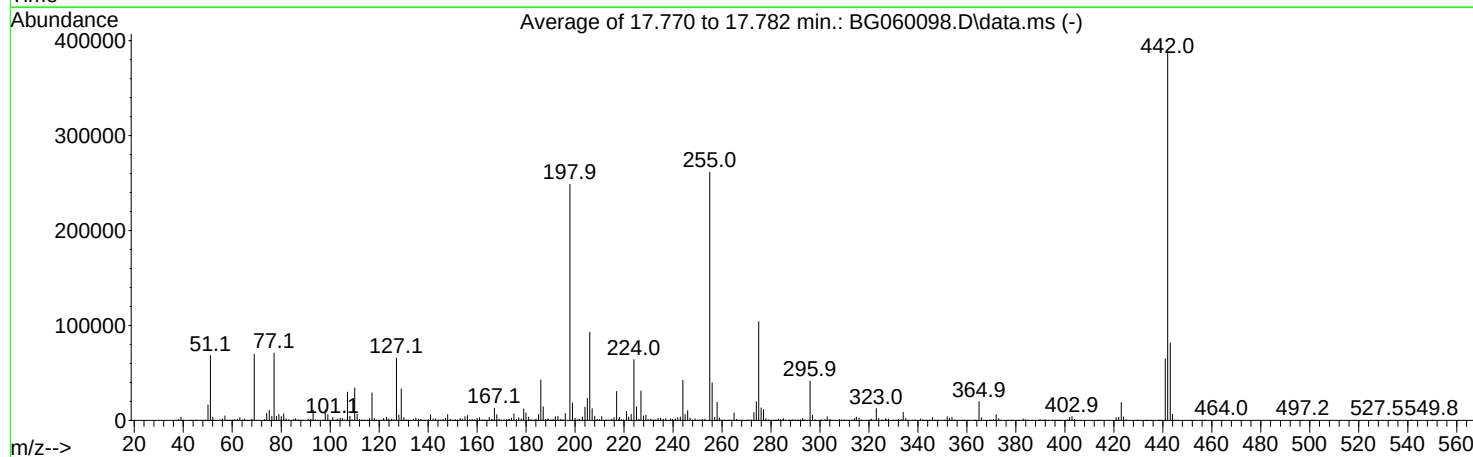


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122023\
Data File : BG060098.D
Acq On : 20 Dec 2023 9:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Dec 19 04:37:23 2023

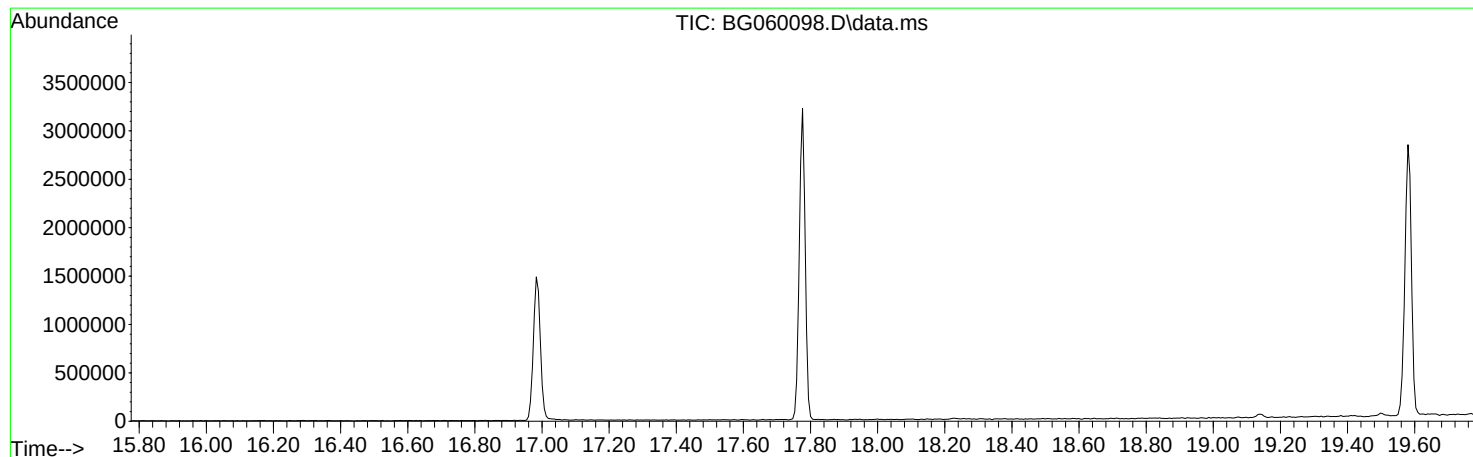




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	68259	PASS
68	69	0.00	2	1.8	1262	PASS
69	198	0.00	100	28.0	69688	PASS
70	69	0.00	2	0.3	214	PASS
127	198	10	80	26.4	65565	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	248747	PASS
199	198	5	9	7.4	18441	PASS
275	198	10	60	41.8	103955	PASS
365	198	1	100	8.0	19843	PASS
441	198	0.01	100	26.0	64752	PASS
442	442	50	100	100.0	387584	PASS
443	442	15	24	21.0	81384	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122023\
Data File : BG060098.D
Acq On : 20 Dec 2023 9:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 20 12:30:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 04:37:23 2023
Response via : Initial Calibration

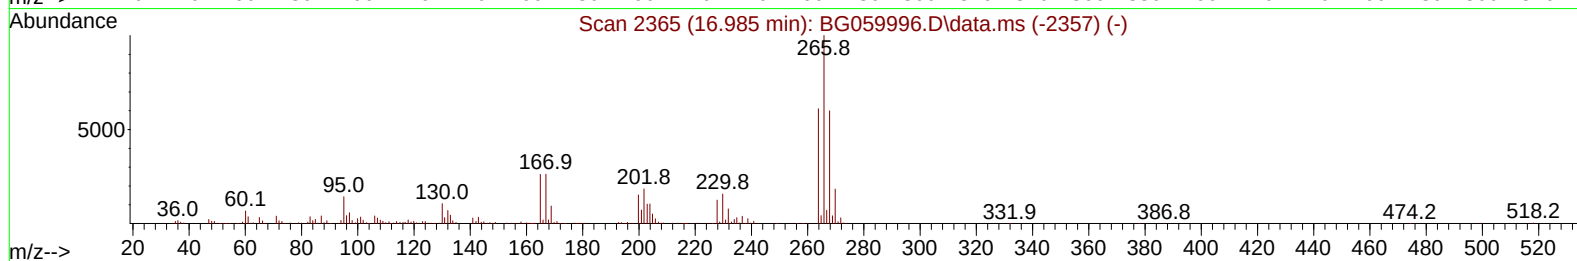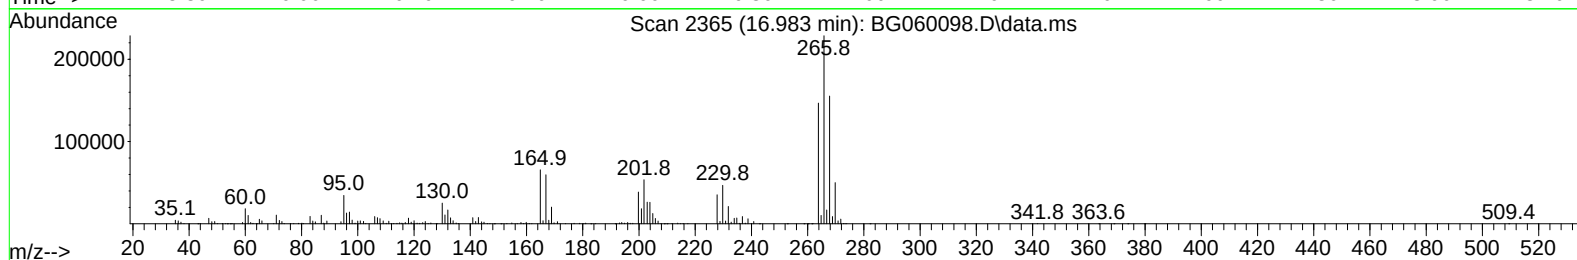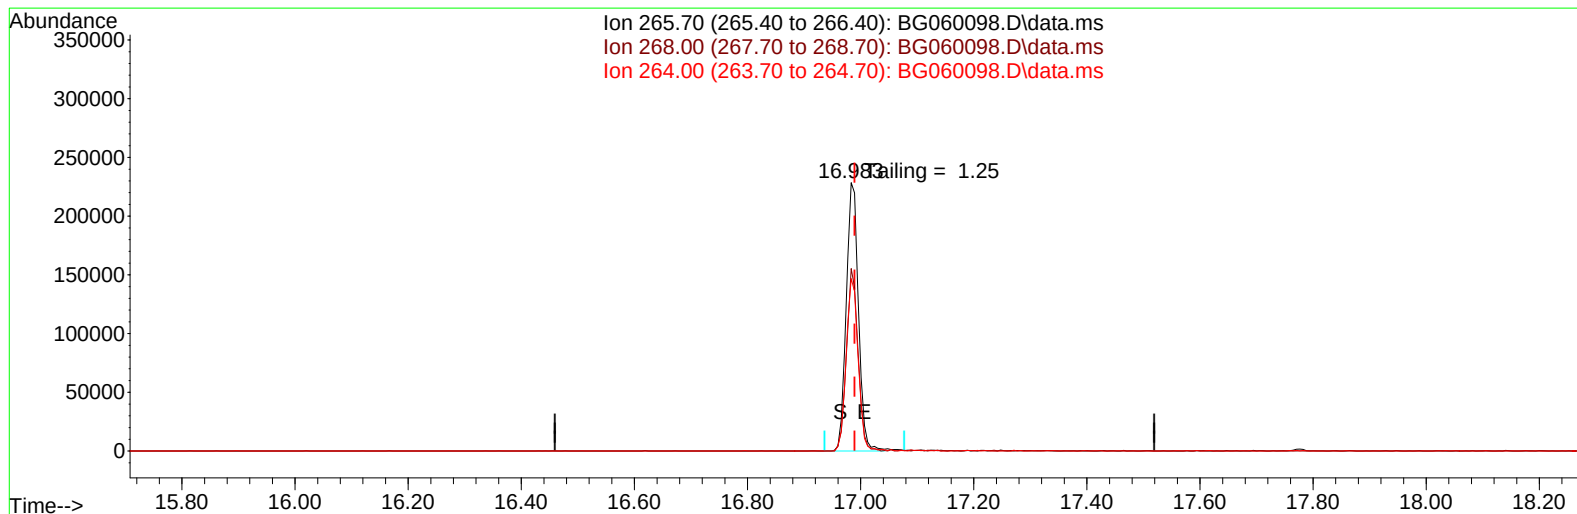

TIC: BG060098.D\data.ms

(70) Pentachlorophenol (C)

16.983min (-0.006) 301712.27 ng




response 344954

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.90	67.96
264.00	61.00	64.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122023\
 Data File : BG060098.D
 Acq On : 20 Dec 2023 9:59
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Dec 20 12:30:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 04:37:23 2023
 Response via : Initial Calibration

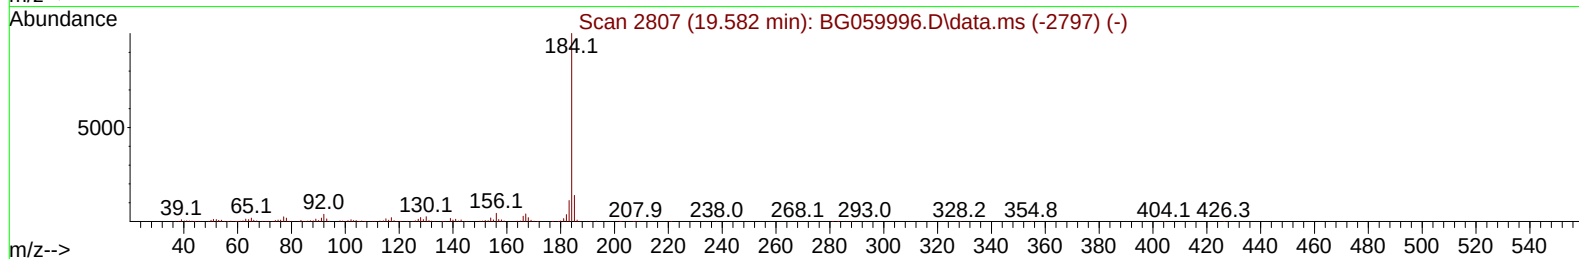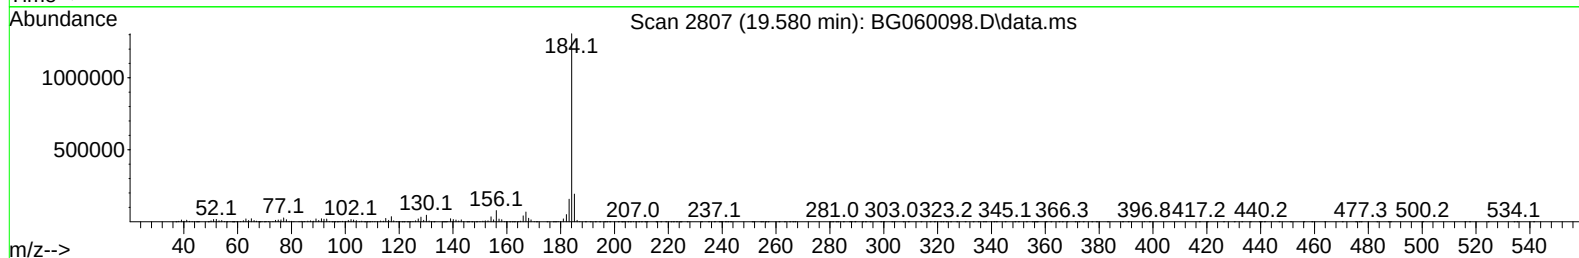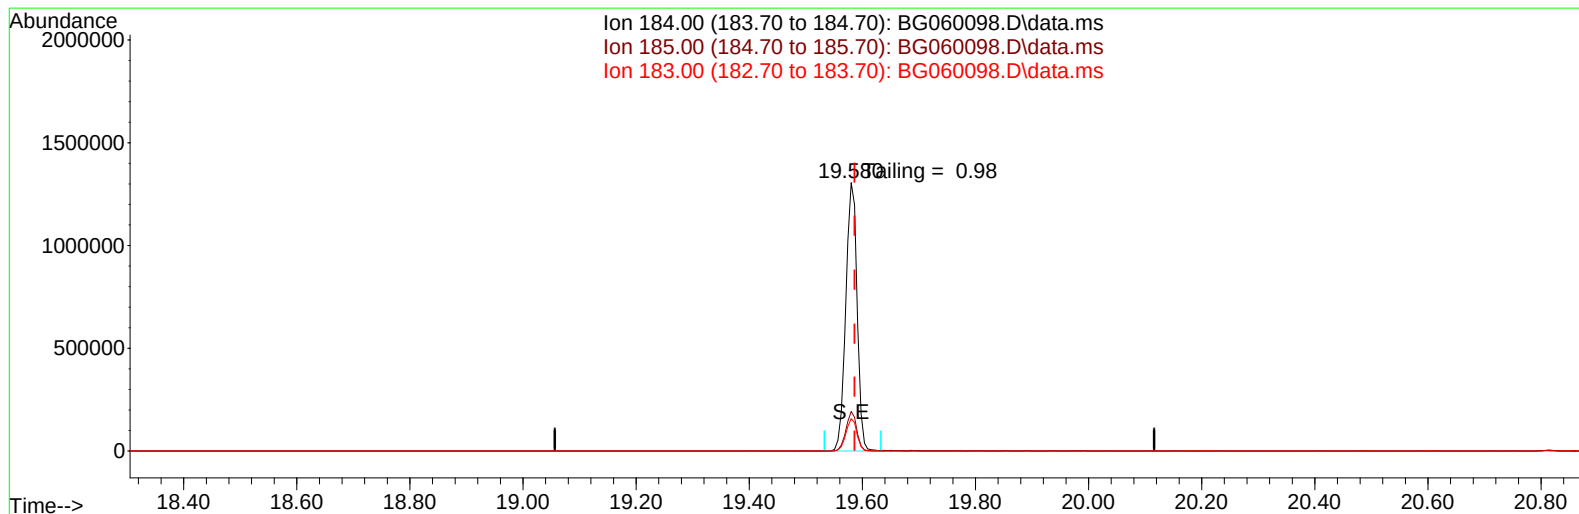

TIC: BG060098.D\data.ms

(77) Benzidine

19.580min (-0.006) 326413.98 ng

response 1815437

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.72
183.00	11.20	12.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/20/2023	BNA_G	<u>BG060098.D</u>
Compound Name	Response	Retention Time
DDT	1073965	20.814
DDD	26619	20.367
DDE	0	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26619	1100584	2.42

Instrument :
BNA_G
ClientSampleId :
DFTPP