

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122115\
 Data File : BG020381.D
 Acq On : 21 Dec 2015 17:48
 Operator : UM/SJ
 Sample : G4768-01DL 5X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9N27DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	41	47	55	rBV3	12514	25158	7.15%	1.142%
2	3.193	57	60	66	rVB2	2823	4088	1.16%	0.186%
3	3.387	89	93	96	rBV3	366	509	0.14%	0.023%
4	3.445	100	103	106	rBV3	556	559	0.16%	0.025%
5	3.598	127	129	131	rBV2	475	542	0.15%	0.025%
6	3.863	172	174	177	rBV	441	586	0.17%	0.027%
7	3.962	189	191	194	rBV2	611	699	0.20%	0.032%
8	4.015	198	200	202	rVB2	572	478	0.14%	0.022%
9	4.397	263	265	267	rVB	501	489	0.14%	0.022%
10	4.544	286	290	292	rBV	411	620	0.18%	0.028%
11	4.573	294	295	301	rVB	568	743	0.21%	0.034%
12	4.620	301	303	304	rBV	583	533	0.15%	0.024%
13	4.779	327	330	332	rVB2	689	814	0.23%	0.037%
14	4.902	346	351	353	rVB3	592	719	0.20%	0.033%
15	5.002	367	368	372	rBV	629	488	0.14%	0.022%
16	5.090	380	383	384	rBV	597	574	0.16%	0.026%
17	5.508	453	454	459	rVB	533	479	0.14%	0.022%
18	5.743	493	494	498	rVB	590	550	0.16%	0.025%
19	5.819	505	507	510	rBB	581	643	0.18%	0.029%
20	5.860	510	514	516	rBV	460	696	0.20%	0.032%
21	5.913	518	523	525	rVV	446	483	0.14%	0.022%
22	6.130	558	560	562	rBV	381	514	0.15%	0.023%
23	6.166	565	566	572	rVB	487	625	0.18%	0.028%
24	6.224	572	576	579	rBV	611	853	0.24%	0.039%
25	6.412	604	608	610	rBV	556	814	0.23%	0.037%
26	6.477	614	619	621	rBB	615	691	0.20%	0.031%
27	6.659	647	650	653	rVB	382	580	0.16%	0.026%
28	6.706	657	658	661	rBV	515	589	0.17%	0.027%
29	6.859	681	684	688	rBB	366	560	0.16%	0.025%
30	6.976	702	704	707	rBV	478	510	0.14%	0.023%
31	7.059	714	718	720	rBV	395	635	0.18%	0.029%
32	7.253	748	751	753	rBV2	1341	1848	0.53%	0.084%
33	7.411	772	778	784	rBV	7239	12056	3.43%	0.547%
34	7.629	810	815	820	rBB2	6415	10801	3.07%	0.490%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122115\
 Data File : BG020381.D
 Acq On : 21 Dec 2015 17:48
 Operator : UM/SJ
 Sample : G4768-01DL 5X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9N27DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

35	8.093	888	894	903	rBB	59726	100436	28.55%	4.559%
36	8.633	982	986	990	rBB2	1991	2949	0.84%	0.134%
37	8.804	1009	1015	1023	rBB3	4972	8598	2.44%	0.390%
38	9.262	1087	1093	1100	rBV	9255	16100	4.58%	0.731%
39	9.985	1212	1216	1223	rVB3	5962	9817	2.79%	0.446%
40	10.232	1255	1258	1262	rBB3	372	519	0.15%	0.024%
41	10.414	1286	1289	1293	rBB	388	518	0.15%	0.024%
42	10.531	1303	1309	1315	rBV2	9756	16169	4.60%	0.734%
43	10.907	1367	1373	1378	rBV	84532	161580	45.93%	7.334%
44	10.960	1378	1382	1394	rVV	133471	234608	66.69%	10.649%
45	11.083	1397	1403	1409	rVB	5204	8560	2.43%	0.389%
46	12.558	1647	1654	1660	rBV	14853	24365	6.93%	1.106%
47	12.781	1686	1692	1698	rVB	7122	11359	3.23%	0.516%
48	13.557	1820	1824	1829	rBV	3500	4645	1.32%	0.211%
49	13.880	1875	1879	1880	rBV	524	643	0.18%	0.029%
50	14.045	1900	1907	1911	rBB	1401	2003	0.57%	0.091%
51	14.121	1914	1920	1925	rBV	21094	30937	8.79%	1.404%
52	14.168	1925	1928	1932	rVB	3568	4243	1.21%	0.193%
53	14.286	1944	1948	1951	rBB2	604	735	0.21%	0.033%
54	14.421	1965	1971	1981	rBB	23431	39330	11.18%	1.785%
55	14.509	1983	1986	1990	rBB2	350	551	0.16%	0.025%
56	14.726	2017	2023	2029	rBV2	138236	220701	62.74%	10.018%
57	14.791	2029	2034	2042	rVB	21144	32706	9.30%	1.485%
58	14.856	2042	2045	2049	rBB	459	598	0.17%	0.027%
59	15.120	2085	2090	2097	rBB	10264	15201	4.32%	0.690%
60	15.525	2156	2159	2162	rVB2	545	797	0.23%	0.036%
61	15.713	2185	2191	2196	rBV	36614	54780	15.57%	2.486%
62	15.772	2196	2201	2209	rVB2	11889	18397	5.23%	0.835%
63	15.831	2209	2211	2212	rBV2	996	735	0.21%	0.033%
64	16.066	2246	2251	2253	rBV2	508	876	0.25%	0.040%
65	16.213	2272	2276	2280	rVB2	847	873	0.25%	0.040%
66	16.342	2297	2298	2301	rBV2	567	540	0.15%	0.025%
67	16.407	2306	2309	2312	rBV2	799	1094	0.31%	0.050%
68	16.589	2337	2340	2342	rBV2	416	485	0.14%	0.022%
69	17.200	2442	2444	2446	rVV	1085	740	0.21%	0.034%
70	17.253	2450	2453	2456	rBV2	968	1429	0.41%	0.065%
71	17.288	2456	2459	2463	rVB	1027	1420	0.40%	0.064%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122115\
 Data File : BG020381.D
 Acq On : 21 Dec 2015 17:48
 Operator : UM/SJ
 Sample : G4768-01DL 5X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9N27DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

72	17.353	2466	2470	2471	rBV	585	513	0.15%	0.023%
73	17.470	2483	2490	2495	rBV2	185564	275229	78.24%	12.493%
74	17.511	2495	2497	2502	rVV	24992	31873	9.06%	1.447%
75	17.570	2502	2507	2522	rVB2	39311	62865	17.87%	2.853%
76	17.793	2544	2545	2549	rVB	545	659	0.19%	0.030%
77	17.846	2549	2554	2555	rVB	812	825	0.23%	0.037%
78	17.875	2555	2559	2567	rBV2	2257	3364	0.96%	0.153%
79	17.940	2569	2570	2574	rBV	649	623	0.18%	0.028%
80	18.351	2636	2640	2641	rVB	715	803	0.23%	0.036%
81	18.398	2643	2648	2650	rBV2	1145	1746	0.50%	0.079%
82	18.422	2650	2652	2655	rVB2	638	658	0.19%	0.030%
83	18.551	2669	2674	2677	rVV2	1492	2353	0.67%	0.107%
84	18.616	2682	2685	2687	rBV	515	559	0.16%	0.025%
85	18.769	2709	2711	2715	rVB2	701	768	0.22%	0.035%
86	18.804	2715	2717	2719	rBV	626	590	0.17%	0.027%
87	19.062	2759	2761	2764	rVB2	669	710	0.20%	0.032%
88	19.092	2764	2766	2772	rBV2	1010	1265	0.36%	0.057%
89	19.180	2778	2781	2783	rBV	540	514	0.15%	0.023%
90	19.244	2791	2792	2794	rBV	964	748	0.21%	0.034%
91	19.474	2829	2831	2832	rBV	1126	956	0.27%	0.043%
92	19.491	2832	2834	2835	rVV	1818	1537	0.44%	0.070%
93	19.515	2835	2838	2842	rVV	5611	7372	2.10%	0.335%
94	19.550	2842	2844	2846	rVB2	744	643	0.18%	0.029%
95	19.850	2888	2895	2906	rBV	48760	80873	22.99%	3.671%
96	19.926	2906	2908	2909	rBV2	820	585	0.17%	0.027%
97	20.061	2929	2931	2932	rBV	1729	1411	0.40%	0.064%
98	20.143	2940	2945	2946	rBV4	4932	6792	1.93%	0.308%
99	21.747	3212	3218	3230	rBV	203234	351779	100.00%	15.967%
100	25.020	3767	3775	3790	rBV2	85038	262970	74.75%	11.936%


Sum of corrected areas: 2203146

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122115\
Data File : BG020381.D
Acq On : 21 Dec 2015 17:48
Operator : UM/SJ
Sample : G4768-01DL 5X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9N27DL

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

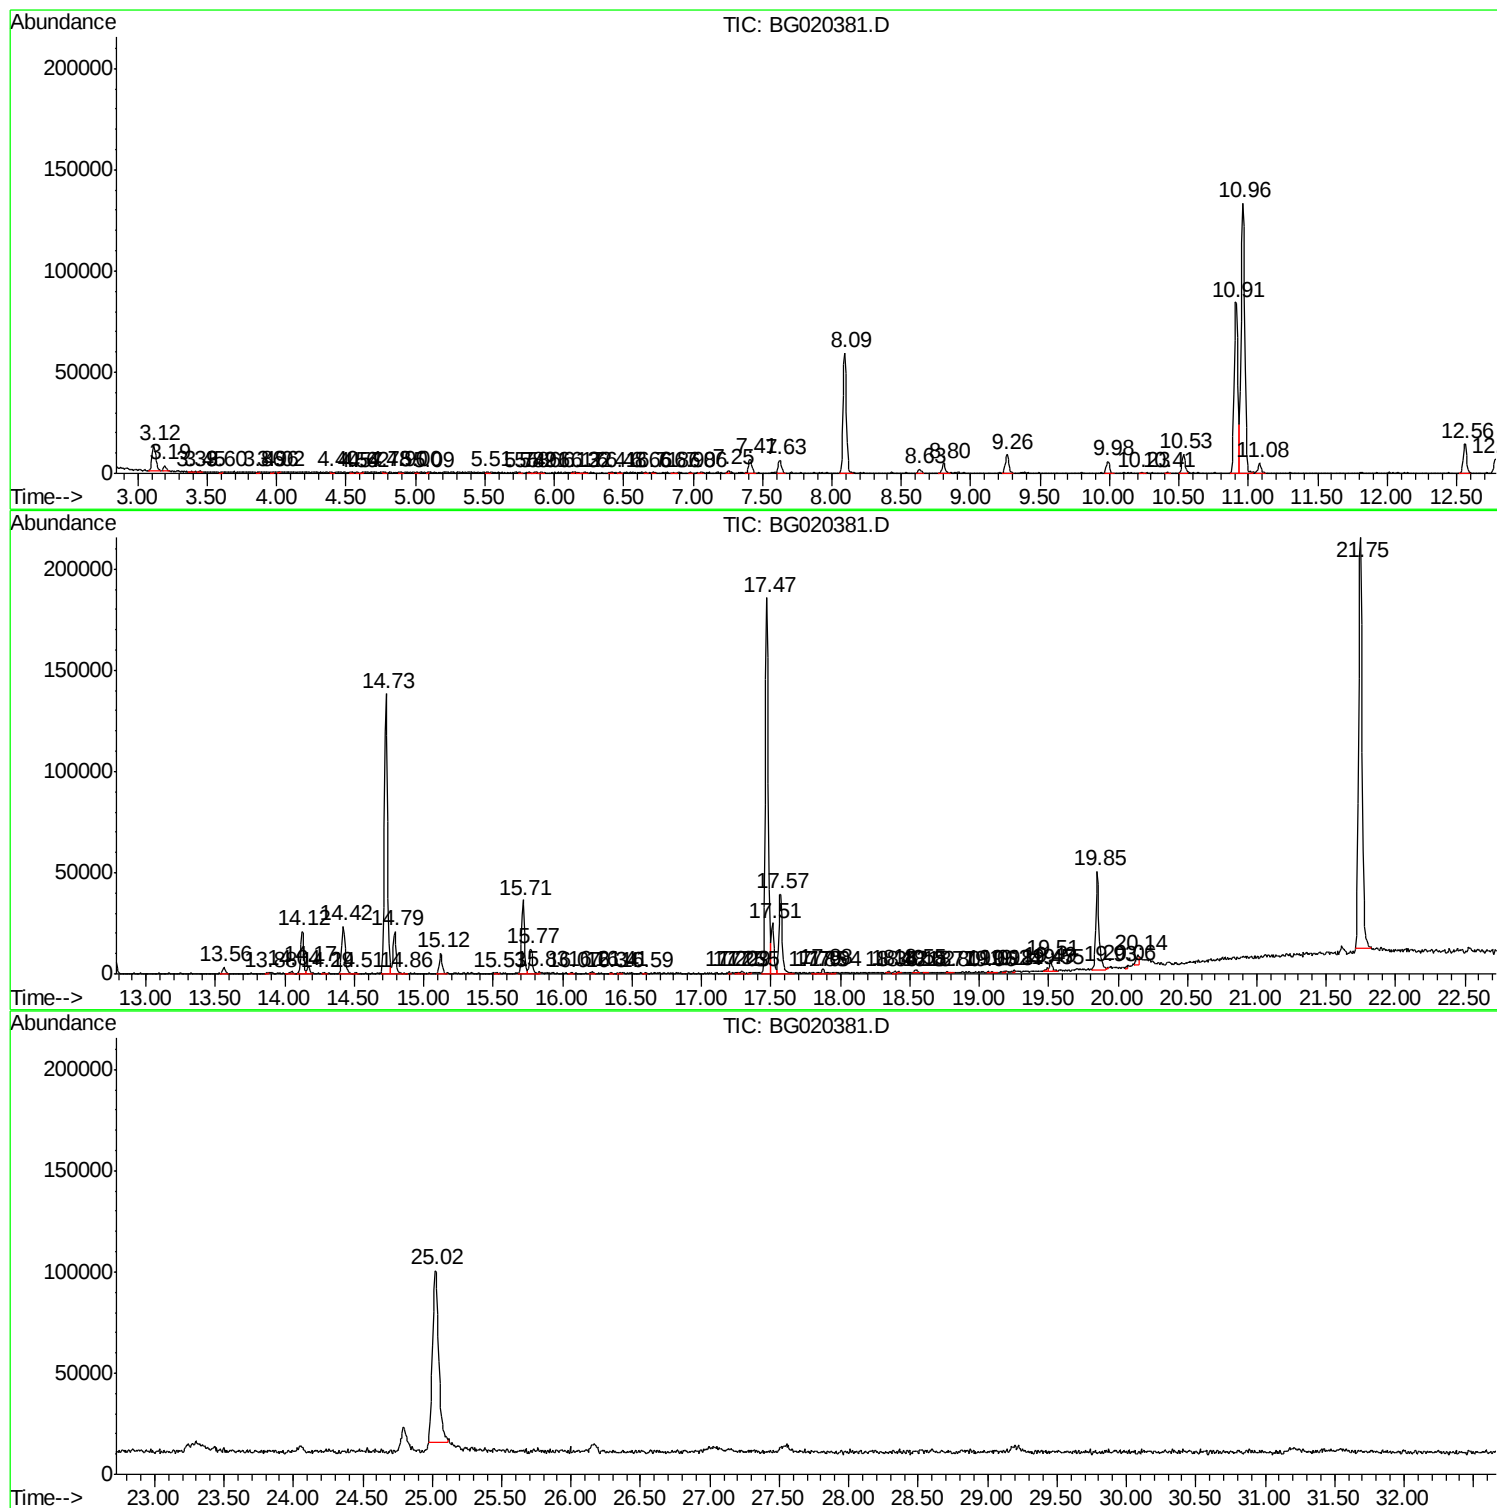

Data_Path : Z:\HPCHEM1\BNA_G\DATA\BG122115\
Data_File : BG020381.D
Acq_On : 21-Dec-2015 17:488
Operator : UM/SJJ
Sample : G4768-01DL_5XX
Misc :
ALS_Vial : 3 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
D9N27DL

Quant_Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
