

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122115\
 Data File : BG020386.D
 Acq On : 21 Dec 2015 21:03
 Operator : UM/SJ
 Sample : G4768-11DL 100X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9N35DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	41	47	55	rBV	8289	15223	3.55%	0.614%
2	4.022	199	201	203	rBV	501	503	0.12%	0.020%
3	4.786	328	331	332	rBV2	631	640	0.15%	0.026%
4	4.938	356	357	360	rBV	597	542	0.13%	0.022%
5	5.068	377	379	381	rBV	571	589	0.14%	0.024%
6	5.121	385	388	390	rVB	643	593	0.14%	0.024%
7	5.344	423	426	429	rBV2	406	634	0.15%	0.026%
8	5.579	460	466	470	rVB	1043	1312	0.31%	0.053%
9	5.702	484	487	488	rBV	719	535	0.12%	0.022%
10	5.779	496	500	503	rVB2	576	733	0.17%	0.030%
11	5.820	503	507	509	rBV	573	658	0.15%	0.027%
12	6.719	655	660	663	rBV2	511	1055	0.25%	0.043%
13	6.819	675	677	681	rVB	578	605	0.14%	0.024%
14	7.418	776	779	782	rBV3	735	802	0.19%	0.032%
15	7.882	856	858	862	rVB3	575	662	0.15%	0.027%
16	8.094	888	894	907	rVB	63285	105787	24.67%	4.267%
17	8.470	952	958	965	rBV2	4155	6842	1.60%	0.276%
18	8.587	975	978	979	rBV2	576	537	0.13%	0.022%
19	8.634	979	986	993	rVB2	5733	10392	2.42%	0.419%
20	8.740	999	1004	1006	rBB2	515	699	0.16%	0.028%
21	9.568	1142	1145	1146	rBV2	690	546	0.13%	0.022%
22	9.586	1146	1148	1150	rVB	775	673	0.16%	0.027%
23	9.815	1183	1187	1189	rBB	546	658	0.15%	0.027%
24	10.150	1241	1244	1246	rBV	360	512	0.12%	0.021%
25	10.297	1265	1269	1273	rBV	848	1516	0.35%	0.061%
26	10.332	1273	1275	1279	rVB	1122	1206	0.28%	0.049%
27	10.409	1284	1288	1291	rVB	993	1043	0.24%	0.042%
28	10.532	1307	1309	1312	rBV	505	554	0.13%	0.022%
29	10.626	1322	1325	1328	rBB	530	515	0.12%	0.021%
30	10.755	1346	1347	1352	rBV	417	553	0.13%	0.022%
31	10.908	1364	1373	1377	rBV	95704	170499	39.76%	6.876%
32	10.961	1377	1382	1392	rVV	239699	428813	100.00%	17.295%
33	11.078	1396	1402	1407	rBV	9038	15041	3.51%	0.607%
34	12.447	1631	1635	1636	rBV	806	967	0.23%	0.039%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122115\
 Data File : BG020386.D
 Acq On : 21 Dec 2015 21:03
 Operator : UM/SJ
 Sample : G4768-11DL 100X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9N35DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

35	12.559	1646	1654	1661	rBV	46980	73307	17.10%	2.957%
36	12.671	1670	1673	1677	rVB	1151	1563	0.36%	0.063%
37	12.776	1684	1691	1698	rVB	26515	42726	9.96%	1.723%
38	13.558	1818	1824	1831	rBV	9227	13593	3.17%	0.548%
39	13.752	1854	1857	1860	rBV	1307	1811	0.42%	0.073%
40	13.893	1876	1881	1888	rVB3	2050	4311	1.01%	0.174%
41	14.040	1902	1906	1911	rBV2	3587	5214	1.22%	0.210%
42	14.098	1911	1916	1918	rBV	2048	2727	0.64%	0.110%
43	14.163	1925	1927	1931	rBB	580	574	0.13%	0.023%
44	14.275	1941	1946	1950	rBV	1164	1980	0.46%	0.080%
45	14.416	1966	1970	1973	rBV	2098	3405	0.79%	0.137%
46	14.445	1973	1975	1979	rVB2	2387	2675	0.62%	0.108%
47	14.727	2012	2023	2028	rBV2	144373	239849	55.93%	9.673%
48	14.786	2028	2033	2040	rVV	55054	86248	20.11%	3.479%
49	14.856	2040	2045	2051	rVB	7024	10098	2.35%	0.407%
50	14.991	2063	2068	2071	rBV	382	707	0.16%	0.029%
51	15.027	2071	2074	2078	rVB	917	1182	0.28%	0.048%
52	15.121	2084	2090	2097	rBV	28991	45688	10.65%	1.843%
53	15.456	2145	2147	2150	rVB	483	530	0.12%	0.021%
54	15.550	2160	2163	2165	rBV2	505	621	0.14%	0.025%
55	15.714	2187	2191	2195	rBV	3598	4653	1.09%	0.188%
56	15.767	2195	2200	2209	rVV	35658	50505	11.78%	2.037%
57	15.826	2209	2210	2215	rVB	468	537	0.13%	0.022%
58	15.867	2215	2217	2218	rBV	750	647	0.15%	0.026%
59	15.890	2218	2221	2224	rVV	1249	1714	0.40%	0.069%
60	15.931	2224	2228	2231	rVV3	1800	2425	0.57%	0.098%
61	15.967	2231	2234	2237	rVB	520	745	0.17%	0.030%
62	16.020	2241	2243	2246	rVV	1003	906	0.21%	0.037%
63	16.061	2246	2250	2254	rVB2	1521	2242	0.52%	0.090%
64	16.137	2260	2263	2265	rBV2	484	635	0.15%	0.026%
65	16.155	2265	2266	2270	rVB	546	505	0.12%	0.020%
66	16.202	2270	2274	2282	rBV2	1912	4204	0.98%	0.170%
67	16.560	2330	2335	2340	rBV2	1756	2643	0.62%	0.107%
68	16.742	2361	2366	2369	rBV2	550	862	0.20%	0.035%
69	16.766	2369	2370	2373	rVV	776	556	0.13%	0.022%
70	16.825	2375	2380	2381	rBV	496	628	0.15%	0.025%
71	17.054	2413	2419	2420	rBV	455	671	0.16%	0.027%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122115\
 Data File : BG020386.D
 Acq On : 21 Dec 2015 21:03
 Operator : UM/SJ
 Sample : G4768-11DL 100X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9N35DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

72	17.253	2448	2453	2454	rBV	849	890	0.21%	0.036%
73	17.289	2454	2459	2465	rVB	2853	3919	0.91%	0.158%
74	17.465	2483	2489	2494	rBV2	190613	296020	69.03%	11.939%
75	17.506	2494	2496	2502	rVB	43572	59352	13.84%	2.394%
76	17.565	2502	2506	2509	rBV2	4230	5892	1.37%	0.238%
77	17.835	2550	2552	2553	rBV2	556	522	0.12%	0.021%
78	17.870	2553	2558	2567	rVV	22670	34996	8.16%	1.411%
79	17.929	2567	2568	2572	rVV	703	925	0.22%	0.037%
80	17.988	2575	2578	2584	rVV	705	1534	0.36%	0.062%
81	18.064	2588	2591	2594	rVV	421	584	0.14%	0.024%
82	18.164	2606	2608	2610	rVB2	698	587	0.14%	0.024%
83	18.241	2616	2621	2622	rVB	527	721	0.17%	0.029%
84	18.305	2626	2632	2635	rBV3	513	1223	0.29%	0.049%
85	18.340	2635	2638	2642	rBV	1423	1753	0.41%	0.071%
86	18.393	2642	2647	2650	rVB3	2953	4706	1.10%	0.190%
87	18.540	2668	2672	2676	rBV	2485	3584	0.84%	0.145%
88	18.640	2684	2689	2692	rVB2	1589	2017	0.47%	0.081%
89	18.687	2692	2697	2704	rBV4	1741	2672	0.62%	0.108%
90	18.775	2707	2712	2718	rBV3	1588	2343	0.55%	0.094%
91	18.834	2720	2722	2724	rBV2	819	669	0.16%	0.027%
92	18.881	2726	2730	2732	rBV2	485	549	0.13%	0.022%
93	19.075	2762	2763	2768	rBV3	584	665	0.16%	0.027%
94	19.410	2818	2820	2821	rVB	868	579	0.14%	0.023%
95	19.433	2821	2824	2825	rBV2	772	730	0.17%	0.029%
96	19.516	2834	2838	2842	rBV	5439	7488	1.75%	0.302%
97	19.845	2891	2894	2897	rBV3	3834	5541	1.29%	0.223%
98	19.915	2904	2906	2909	rBV3	763	758	0.18%	0.031%
99	21.742	3210	3217	3229	rBV	203204	369907	86.26%	14.919%
100	25.015	3765	3774	3792	rBV3	80213	282002	65.76%	11.374%


Sum of corrected areas: 2479454

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122115\
Data File : BG020386.D
Acq On : 21 Dec 2015 21:03
Operator : UM/SJ
Sample : G4768-11DL 100X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9N35DL

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

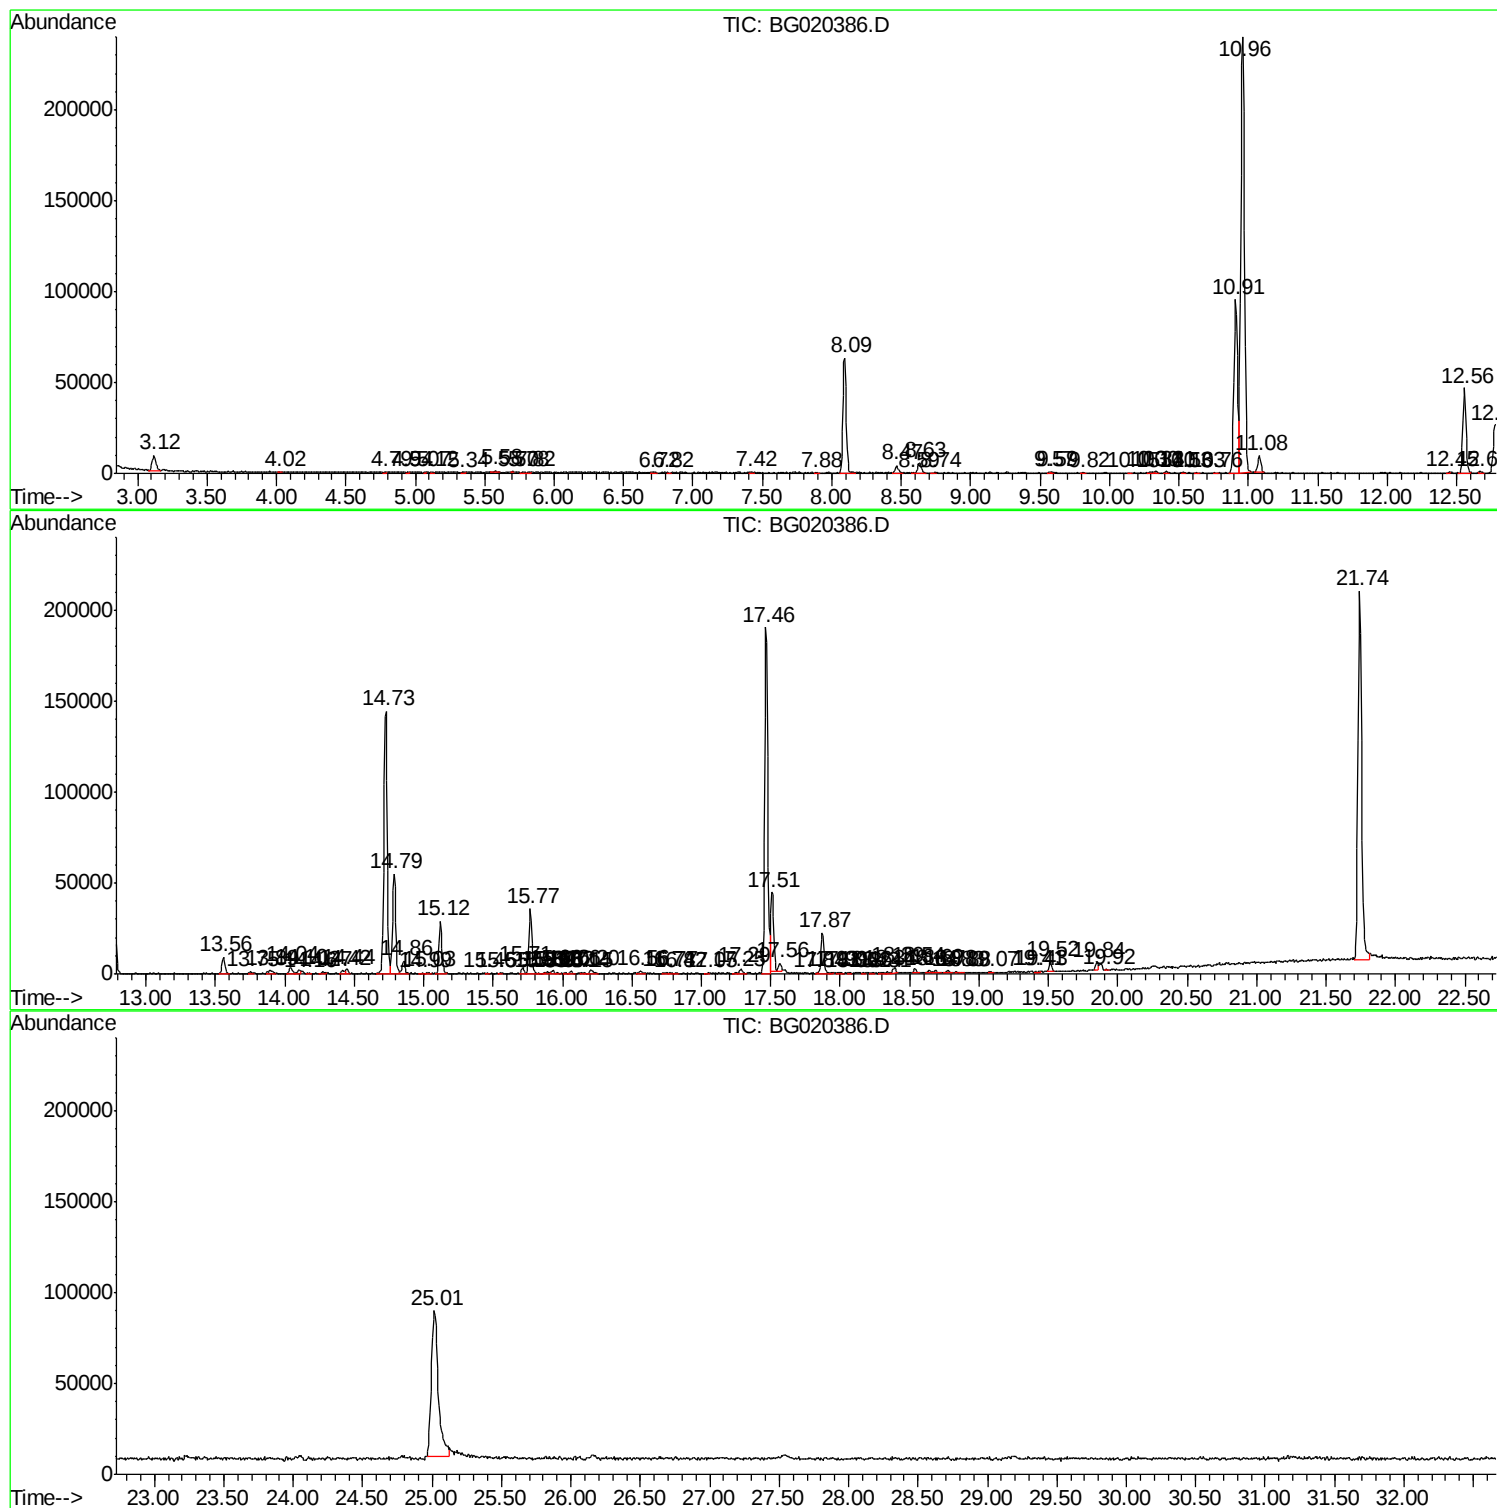

Data_Path : Z:\HPCHEM1\BNA_G\DATA\BG122115\
Data_File : BG020386.D
Acq_On : 21-Dec-2015 21:033
Operator : UM/SJJ
Sample : G4768-11DL_100XX
Misc :
ALS_Vial : 8 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
D9N35DL

Quant_Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
