


Data Path : Z:\HPCHEM1\BNA G\Data\BG122115\
 Data File : BG020379.D
 Acq On : 21 Dec 2015 16:14
 Operator : UM/SJ
 Sample : DFTPP12
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP12

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION
 Last Update : Tue Dec 22 05:02:37 2015

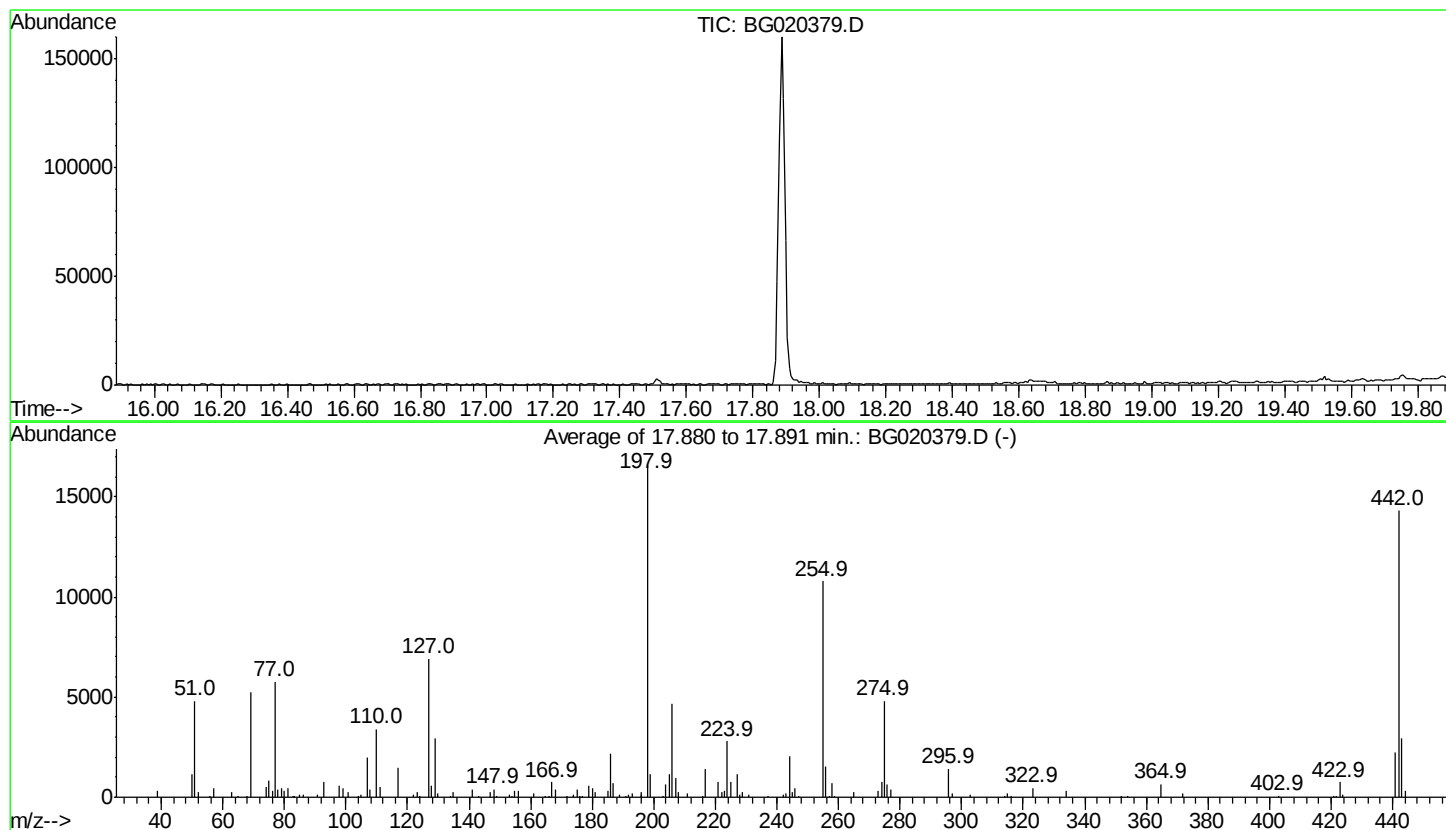

AutoFind: Scans 2560, 2561, 2562; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.0	4795	PASS
68	69	0.00	2	1.0	52	PASS
69	198	0.00	100	31.8	5271	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.8	6921	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16554	PASS
199	198	5	9	7.1	1179	PASS
275	198	10	60	29.1	4814	PASS
365	198	1	100	3.9	643	PASS
441	442	0.01	24	15.6	2232	PASS
442	198	50	100	86.4	14300	PASS
443	442	15	24	20.7	2963	PASS

Scan 2555 (17.850 min): BG020379.D
DFTPP12

m/z	Abundance
39.90	176.0
43.90	218.0

Instrument :
BNA_G
ClientSampleId :
DFTPP12

m/z	Abundance
39.00	330.0
40.00	158.0
44.00	185.0
50.00	1190.0
51.00	4716.0
52.00	274.0
55.90	276.0
56.90	432.0
63.00	219.0
68.90	5046.0
73.90	484.0
74.90	965.0
76.00	250.0
77.00	5577.0
78.00	346.0
78.90	347.0
79.90	311.0
81.00	425.0
82.90	151.0
90.90	212.0
92.90	789.0
97.90	574.0
99.00	510.0
100.90	290.0
104.90	163.0
106.90	1859.0
107.90	372.0
109.90	3100.0
110.90	453.0
116.90	1439.0
121.90	171.0
123.00	217.0
127.00	6612.0
127.90	513.0
128.90	2885.0
129.90	214.0
134.90	269.0
140.90	445.0
146.90	282.0
147.90	384.0
154.90	297.0
155.90	250.0
160.90	176.0
164.90	195.0
165.90	154.0
166.90	647.0
167.90	284.0
173.80	154.0
175.00	298.0
178.90	530.0
180.00	507.0
180.80	193.0
185.00	241.0
185.90	1879.0
187.00	607.0
191.90	194.0
193.00	161.0
195.90	361.0
197.90	14413.0
198.90	1025.0
203.90	526.0
205.00	992.0
206.00	4233.0
207.00	894.0
207.90	154.0
216.80	1242.0
220.90	608.0
222.00	175.0
222.80	188.0
224.00	2475.0
224.90	820.0
226.90	908.0
228.90	212.0
243.90	1514.0
244.90	156.0
245.90	405.0
254.90	8785.0
255.90	1082.0
257.90	476.0
264.90	237.0
272.90	237.0
273.90	670.0
274.90	3822.0
275.90	514.0
277.00	328.0
295.90	1116.0
322.90	225.0
334.00	197.0
364.90	399.0
422.90	503.0
440.90	1743.0
442.00	9586.0

Instrument :
BNA_G
ClientSampleId :
DFTPP12

442.902083.0

444.00291.0

Instrument :
BNA_G
ClientSampleId :
DFTPP12

m/z	Abundance
39.00	377.0
44.00	155.0
50.00	1263.0
51.00	5871.0
52.00	310.0
56.90	429.0
63.00	262.0
65.00	178.0
68.00	157.0
68.90	6336.0
74.00	603.0
74.90	1043.0
76.00	306.0
77.00	6742.0
78.00	538.0
79.00	597.0
79.90	393.0
80.90	582.0
83.10	177.0
85.00	167.0
85.90	166.0
90.90	190.0
92.90	839.0
97.90	617.0
98.90	521.0
100.90	292.0
103.90	213.0
105.00	205.0
107.00	2325.0
107.90	382.0
110.00	4143.0
110.90	624.0
117.00	1712.0
121.90	205.0
122.90	276.0
127.00	8031.0
127.90	748.0
128.90	3206.0
130.00	231.0
134.00	161.0
134.90	368.0
140.90	458.0
143.00	174.0
146.90	261.0
147.90	391.0
148.90	199.0
152.90	173.0
153.90	222.0
154.90	349.0
155.90	404.0
160.90	217.0
167.00	969.0
167.90	435.0
171.90	179.0
174.00	237.0
174.90	455.0
178.90	621.0
179.90	471.0
180.80	364.0
184.90	419.0
186.00	2451.0
187.00	925.0
188.90	242.0
192.00	232.0
192.80	211.0
195.90	449.0
197.90	19280.0
198.90	1525.0
203.00	203.0
203.90	719.0
205.00	1380.0
205.90	5340.0
206.90	981.0
207.90	286.0
210.90	252.0
215.90	188.0
216.90	1726.0
221.00	1042.0
221.80	261.0
222.90	493.0
223.90	3063.0
224.90	792.0
226.90	1537.0
227.90	195.0
228.90	345.0
230.90	217.0
241.90	155.0
242.90	274.0
244.00	2445.0
244.90	355.0
245.90	485.0
246.90	157.0

Instrument :
BNA_G
ClientSampleId :
DFTPP12

254.90	12719.0
255.90	1963.0
256.90	231.0
257.90	802.0
265.00	251.0
272.80	437.0
273.90	912.0
274.90	5567.0
275.90	803.0
276.90	548.0
295.90	1451.0
296.90	323.0
302.90	225.0
313.90	150.0
314.80	337.0
316.00	156.0
323.00	607.0
333.90	327.0
351.90	198.0
354.00	169.0
364.90	858.0
371.90	287.0
402.90	285.0
421.80	242.0
422.90	775.0
424.00	204.0
440.90	2387.0
442.00	16156.0
443.00	3443.0
444.00	269.0

Instrument :
BNA_G
ClientSampleId :
DFTPP12

m/z	Abundance
38.90	246.0
43.90	214.0
50.00	1041.0
51.00	3798.0
51.90	180.0
56.90	394.0
62.90	219.0
68.90	4431.0
74.00	374.0
74.90	574.0
76.00	393.0
77.00	4951.0
78.00	366.0
78.90	345.0
79.90	317.0
81.00	428.0
84.90	206.0
86.00	175.0
92.90	718.0
98.00	507.0
99.00	401.0
100.90	228.0
106.90	1820.0
108.00	325.0
109.90	2919.0
110.90	444.0
116.90	1294.0
122.90	203.0
123.80	168.0
127.00	6120.0
127.90	383.0
128.90	2787.0
129.90	176.0
134.90	209.0
141.00	336.0
147.00	251.0
147.90	468.0
152.90	206.0
154.80	350.0
156.00	367.0
160.90	164.0
167.00	627.0
168.00	403.0
173.90	192.0
174.90	372.0
176.00	198.0
176.90	243.0
178.90	601.0
180.00	461.0
180.90	208.0
185.00	357.0
185.90	2105.0
186.90	596.0
189.00	154.0
190.90	156.0
193.00	233.0
196.10	344.0
197.90	15969.0
198.90	989.0
203.90	700.0
205.00	1013.0
206.00	4435.0
207.00	926.0
208.00	270.0
210.90	268.0
216.90	1195.0
220.90	563.0
221.90	259.0
222.90	303.0
224.00	2827.0
225.00	717.0
227.00	1108.0
227.90	199.0
228.90	239.0
230.90	188.0
236.90	178.0
241.90	179.0
243.00	220.0
243.90	2229.0
245.00	232.0
245.90	374.0
254.90	10808.0
255.90	1564.0
257.90	768.0
258.80	152.0
264.90	227.0
272.90	376.0
273.90	751.0
274.90	5055.0
275.90	675.0
277.00	301.0
295.90	1660.0

Instrument :
BNA_G
ClientSampleId :
DFTPP12

296.80	203.0
302.90	214.0
314.90	172.0
323.00	609.0
334.00	347.0
364.90	674.0
372.00	247.0
420.90	154.0
422.90	1020.0
423.90	170.0
440.90	2567.0
442.00	17160.0
443.00	3364.0
443.90	338.0

Instrument :
BNA_G
ClientSampleId :
DFTPP12