



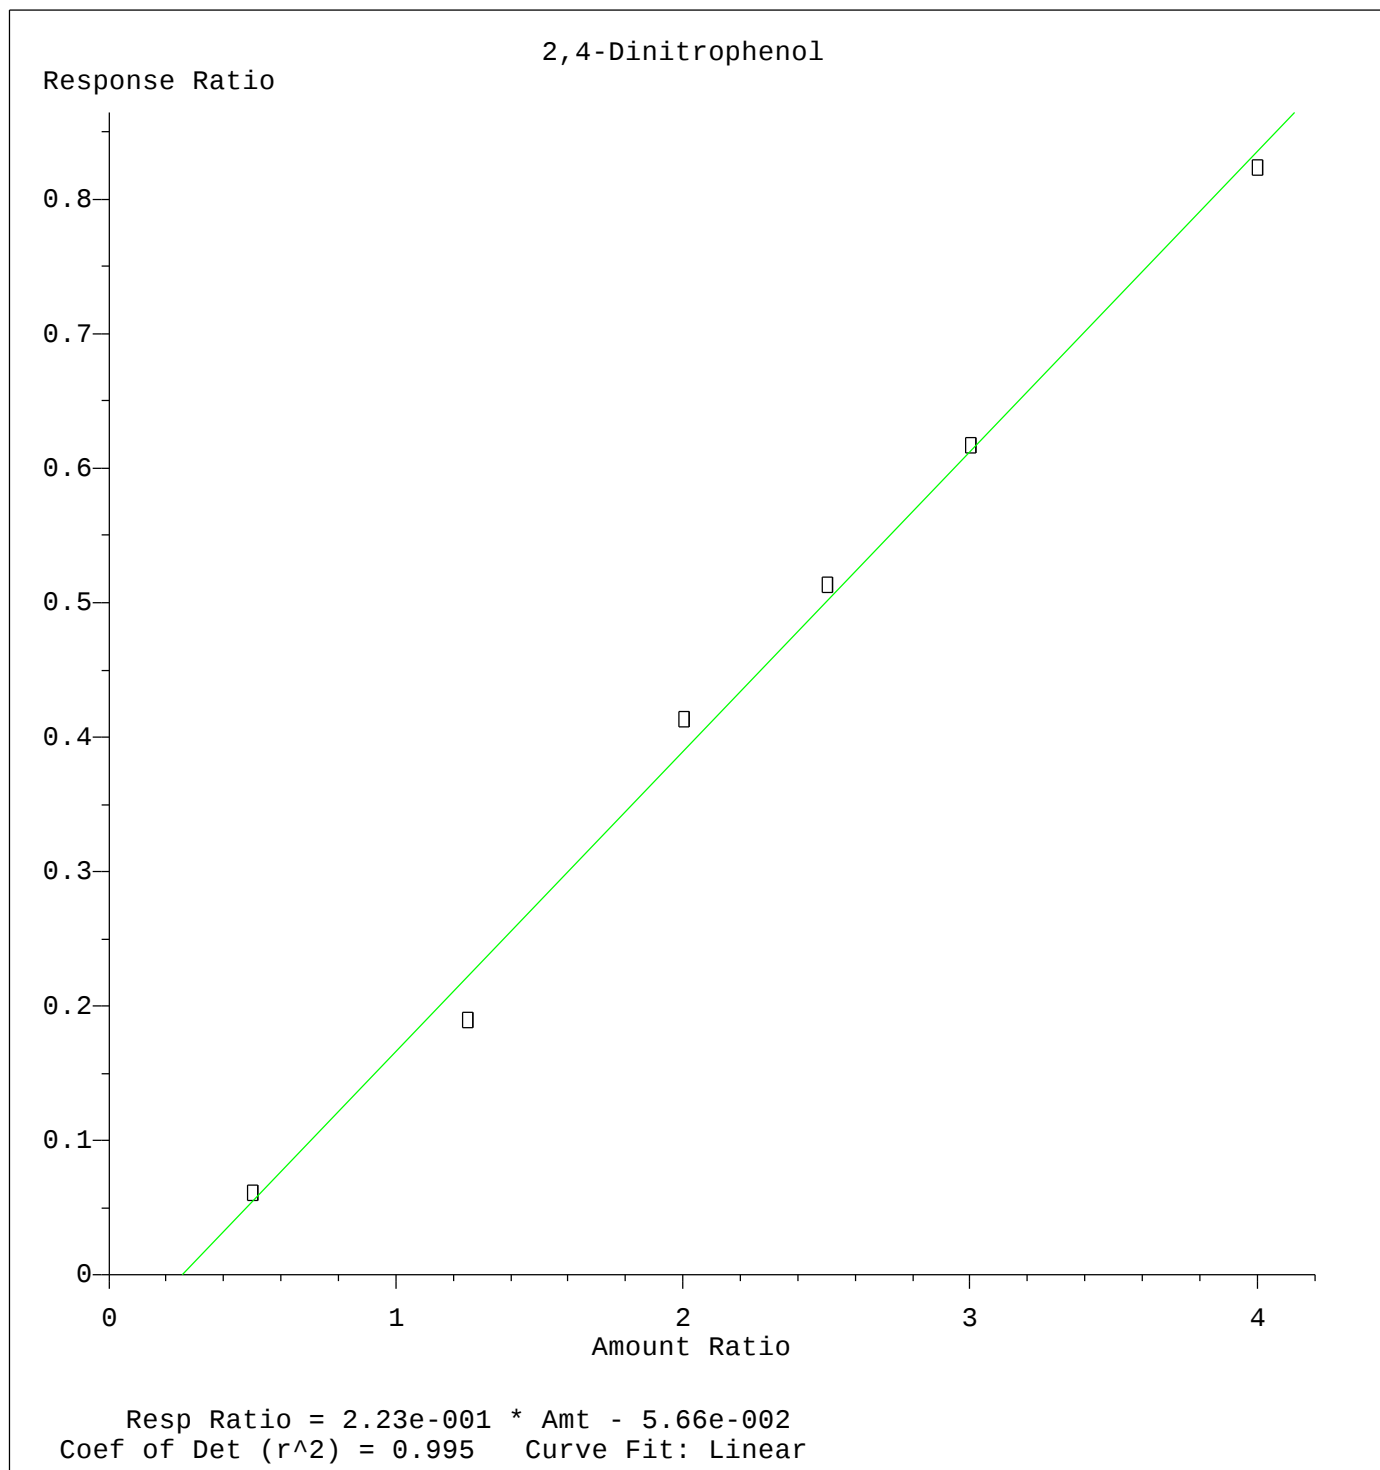

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
Calibration Table Last Updated: Wed Dec 21 18:42:01 2016

Hexachlorocyclopentadiene

Response Ratio

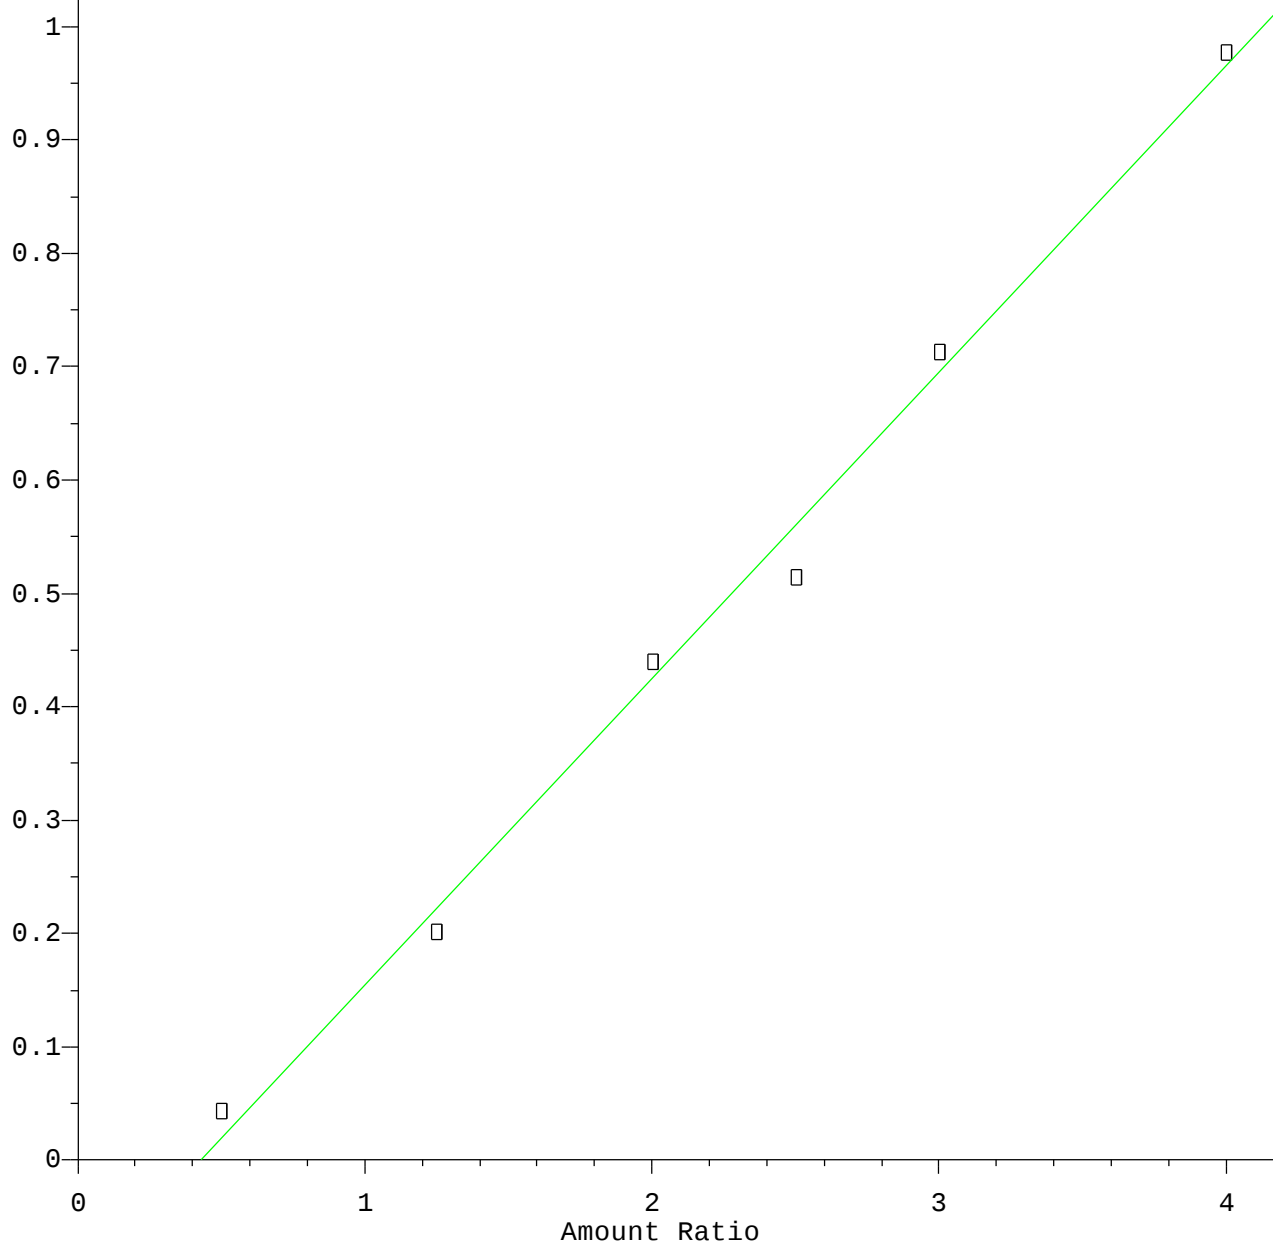

Resp Ratio = $2.70 \times 10^{-1} \times \text{Amt} - 1.15 \times 10^{-1}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
Calibration Table Last Updated: Wed Dec 21 18:42:01 2016