


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122116\
 Data File : BG025354.D
 Acq On : 21 Dec 2016 12:13
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 21 18:42:01 2016

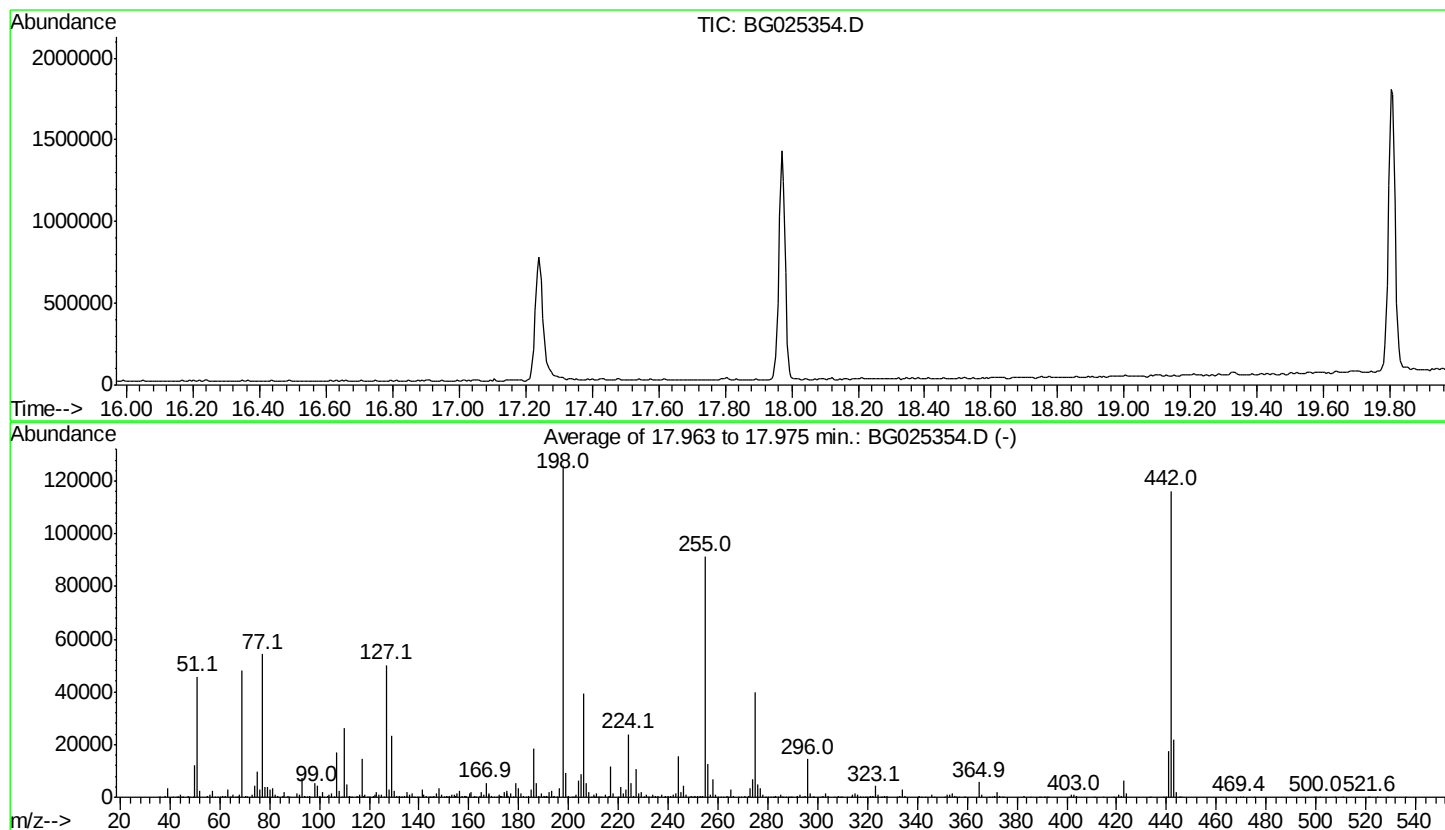

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	45868	PASS
68	69	0.00	2	1.8	866	PASS
69	198	0.00	100	38.2	48036	PASS
70	69	0.00	2	0.6	311	PASS
127	198	10	80	39.9	50248	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	125869	PASS
199	198	5	9	7.4	9299	PASS
275	198	10	60	31.5	39664	PASS
365	198	1	100	4.6	5807	PASS
441	442	0.01	24	15.1	17578	PASS
442	198	50	100	92.3	116208	PASS
443	442	15	24	18.8	21823	PASS