


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122116\
 Data File : BG025363.D
 Acq On : 21 Dec 2016 18:46
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 21 18:42:01 2016

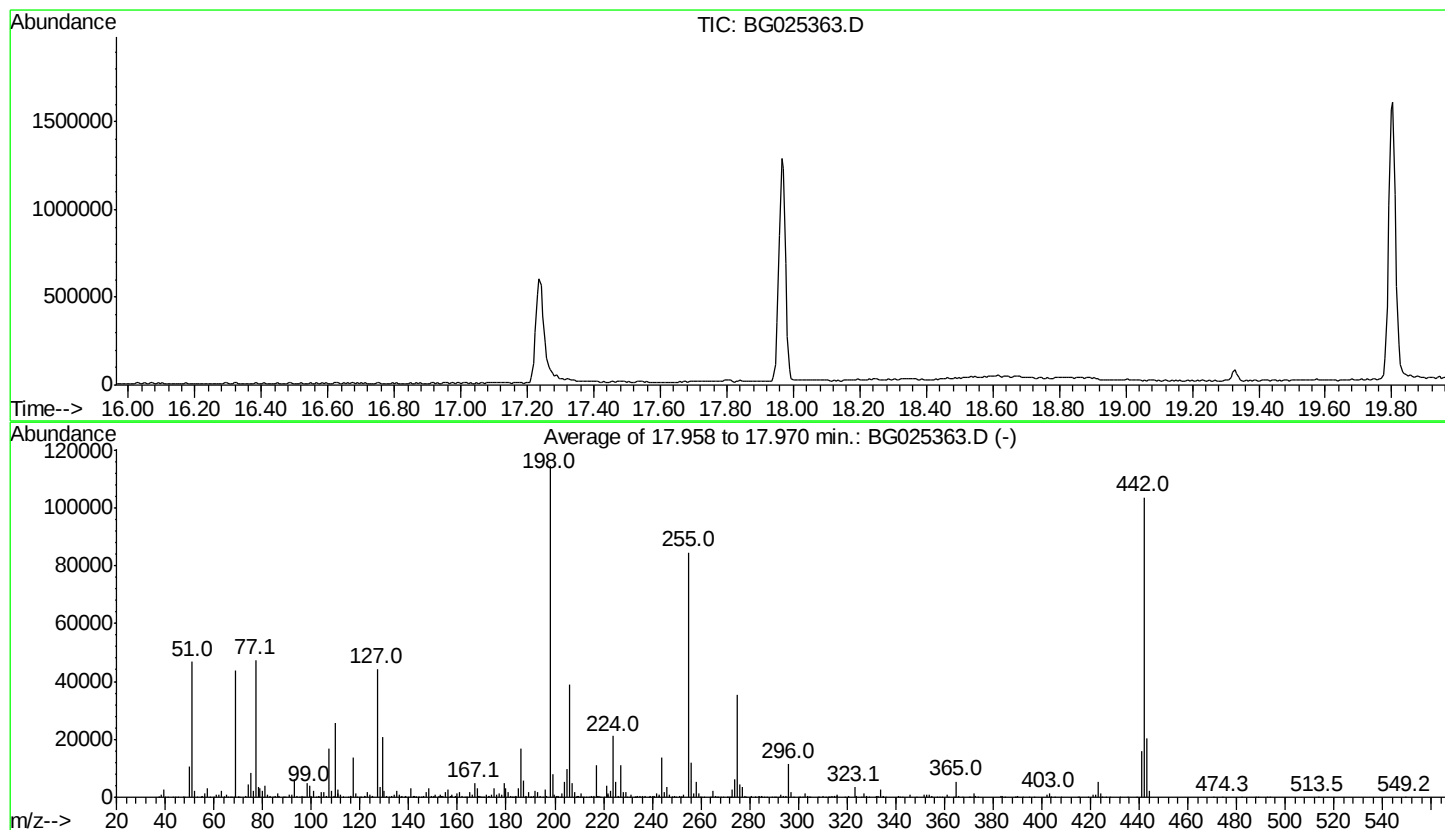

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2565

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.9	46840	PASS
68	69	0.00	2	0.4	163	PASS
69	198	0.00	100	38.1	43573	PASS
70	69	0.00	2	0.3	113	PASS
127	198	10	80	38.7	44350	PASS
197	198	0.00	2	0.5	539	PASS
198	198	100	100	100.0	114512	PASS
199	198	5	9	6.9	7923	PASS
275	198	10	60	31.0	35533	PASS
365	198	1	100	4.8	5509	PASS
441	442	0.01	24	15.6	16108	PASS
442	198	50	100	90.4	103506	PASS
443	442	15	24	19.7	20381	PASS