

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122117\
 Data File : BG031690.D
 Acq On : 22 Dec 2017 1:37
 Operator : SJ/JU
 Sample : I7002-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Dec 22 03:19:16 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 14:09:19 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.83	152	48931	20.00	ng	-0.01
21) Naphthalene-d8	11.72	136	205437	20.00	ng	0.00
38) Acenaphthene-d10	15.46	164	146139	20.00	ng	0.00
63) Phenanthrene-d10	18.20	188	391076	20.00	ng	0.00
75) Chrysene-d12	22.56	240	444739	20.00	ng	-0.01
86) Perylene-d12	26.34	264	472975	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	6.24	112	390912	145.51	ng	0.00
7) Phenol-d6	7.92	99	505463	144.92	ng	0.00
23) Nitrobenzene-d5	10.03	82	253259	93.09	ng	-0.01
41) 2,4,6-Tribromophenol	16.94	330	339745	152.36	ng	0.00
44) 2-Fluorobiphenyl	14.09	172	955569	82.07	ng	0.00
78) Terphenyl-d14	20.73	244	1667760	85.67	ng	0.00
Target Compounds						
9) Benzaldehyde	8.33	77	8869	4.223	ng	94
10) Phenol	7.95	94	19913	5.655	ng	89
19) n-Nitroso-di-n-propylamine	10.03	70	32932	13.825	ng	# 72
49) Dimethylphthalate	14.89	163	91147	7.080	ng	99
56) 2,4-Dinitrotoluene	15.46	165	19482	6.397	ng	# 17
64) 4,6-Dinitro-2-methylphenol	16.93	198	791	8.650	ng	# 17
66) 4-Bromophenyl-phenylether	16.94	248	27295	4.827	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122117\
Data File : BG031690.D
Acq On : 22 Dec 2017 1:37
Operator : SJ/JU
Sample : I7002-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Dec 22 03:19:16 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 14:09:19 2017
Response via : Initial Calibration

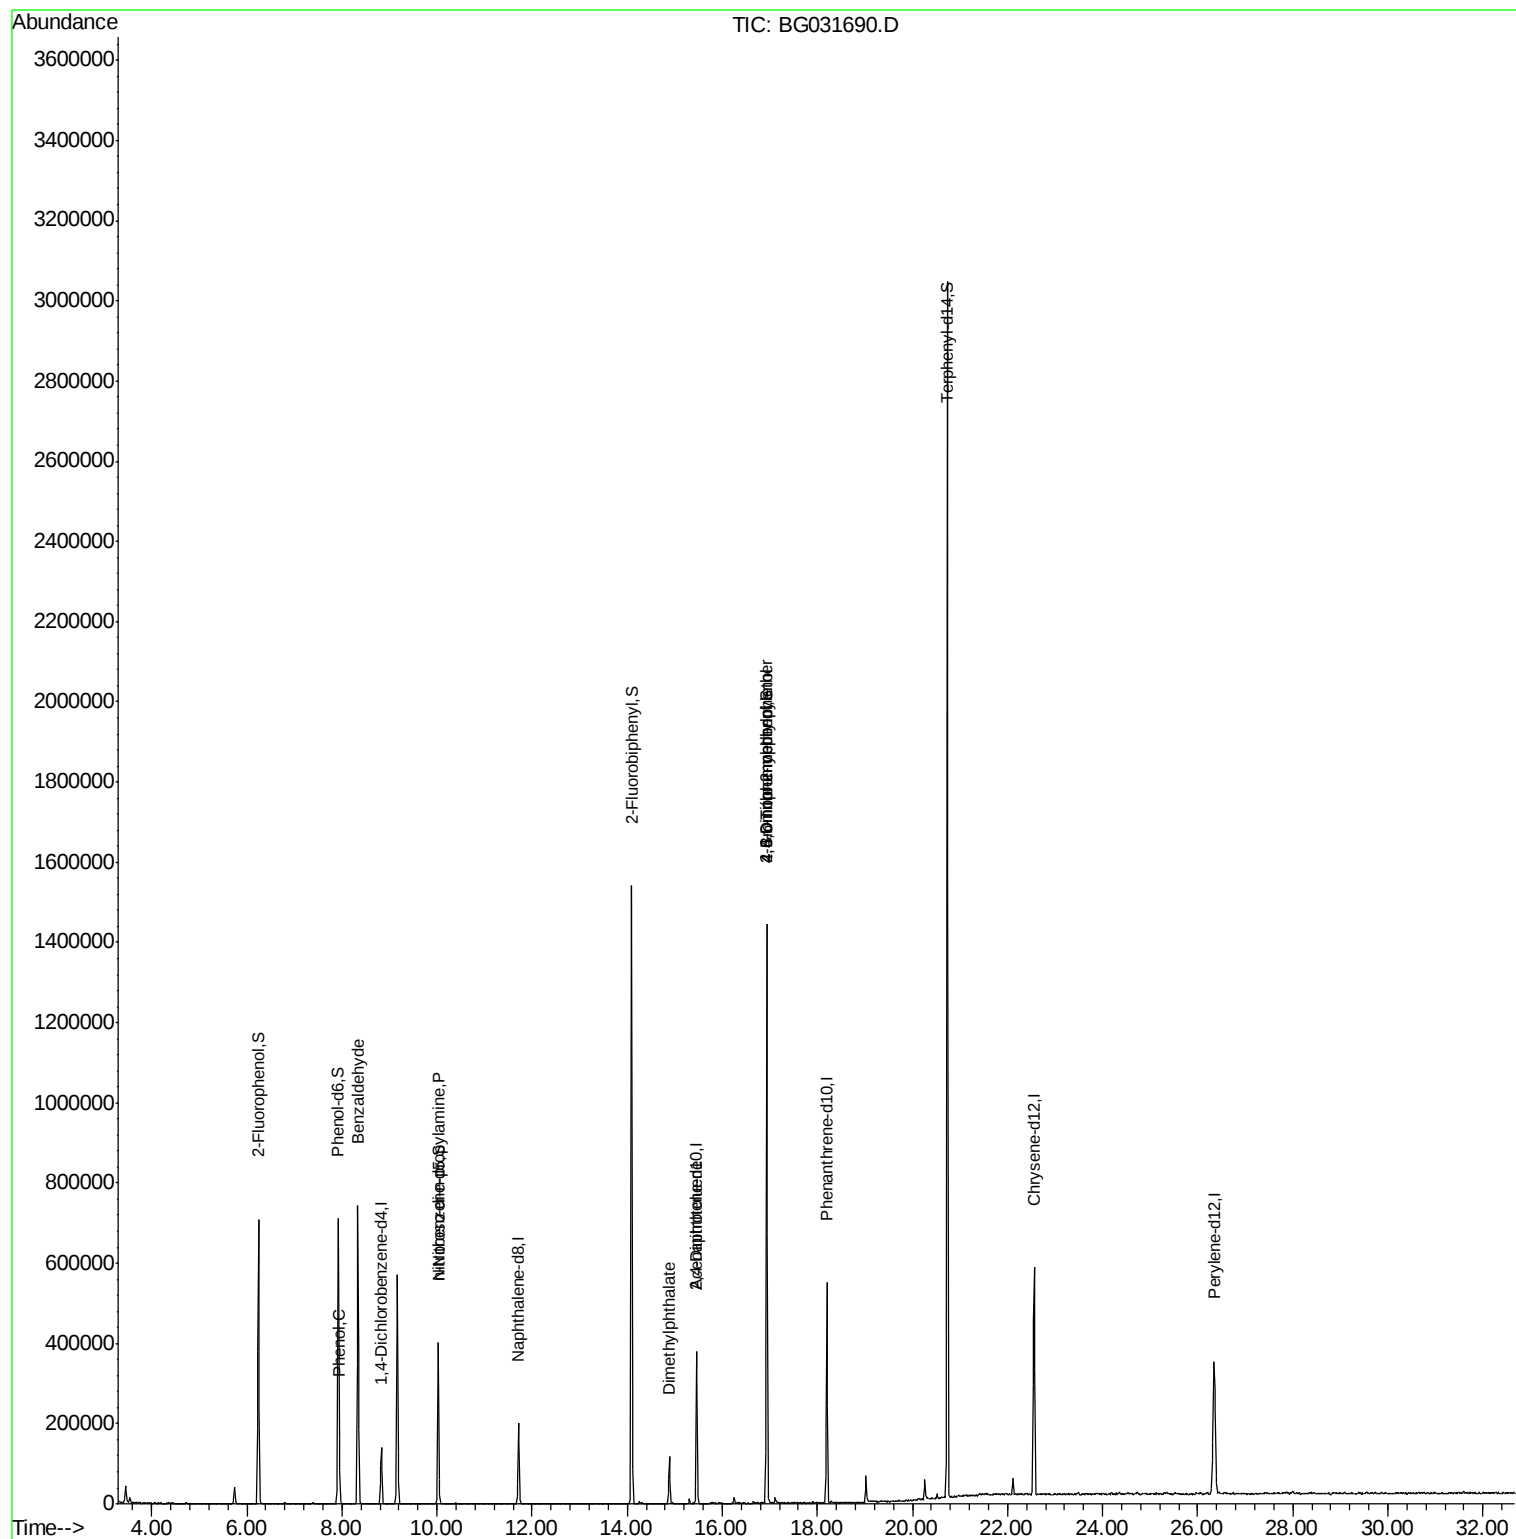







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.83 min Scan# 943
Delta R.T. -0.01 min
Lab File: BG031690.D
Acq: 22 Dec 2017 1:37

Instrument :
BNA_G
ClientSampleId :




Tot Ion:152 Resp: 48931
Ion Ratio Lower Upper
152 100
150 149.0 126.6 189.8
115 56.0 53.0 79.4

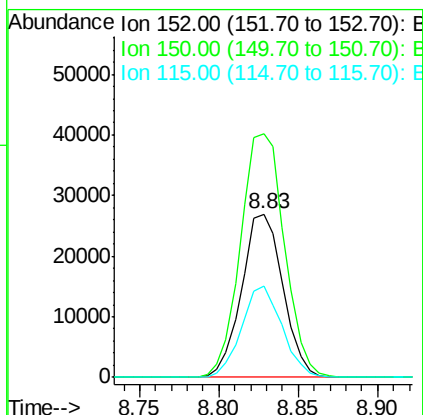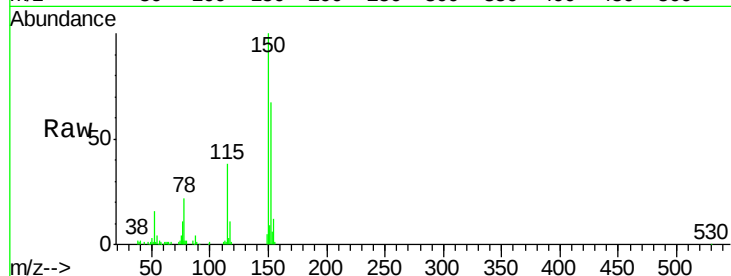


#5

2-Fluorophenol
Concen: 145.511 ng
RT: 6.24 min Scan# 503
Delta R.T. -0.01 min
Lab File: BG031690.D
Acq: 22 Dec 2017 1:37

Tgt Ion:112 Resp: 390912
Ion Ratio Lower Upper
112 100
64 48.1 56.3 84.5#
63 26.0 30.1 45.1#

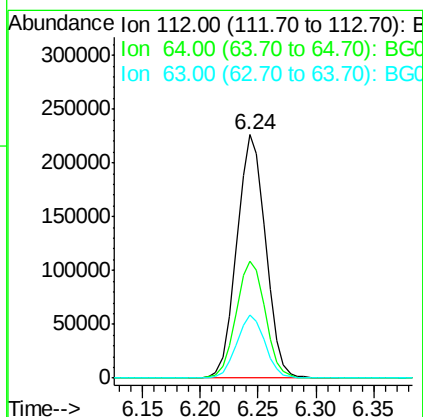

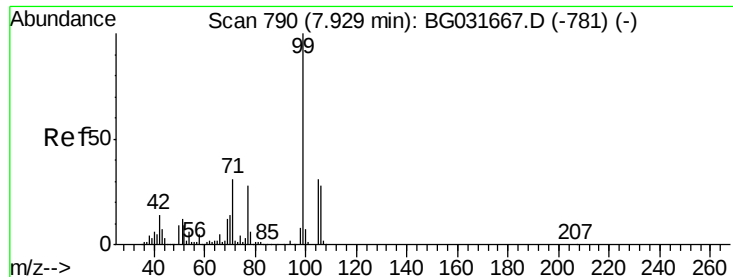

#7

Phenol-d6

Concen: 144.918 ng

RT: 7.92 min Scan# 789

Delta R.T. -0.01 min

Lab File: BG031690.D

Acq: 22 Dec 2017 1:37

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 505463

Ion Ratio Lower Upper




99 100

42 14.7 14.1 21.1

71 34.7 26.1 39.1

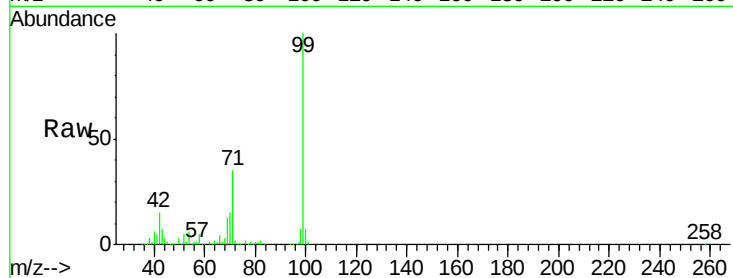

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

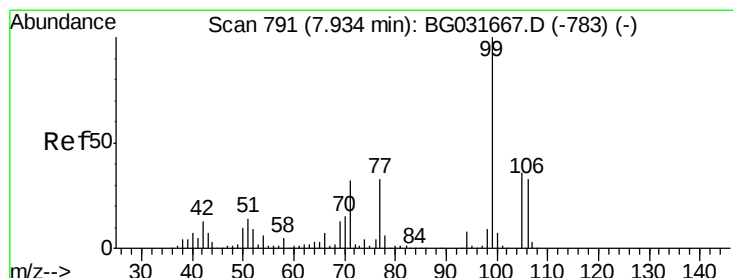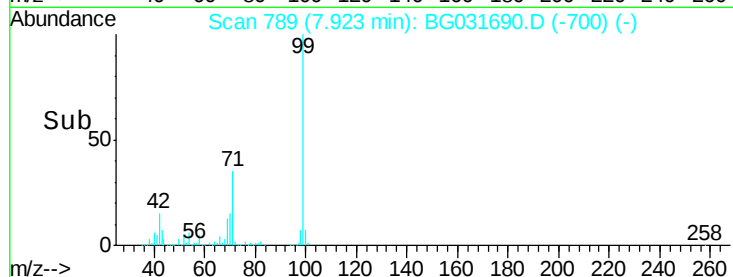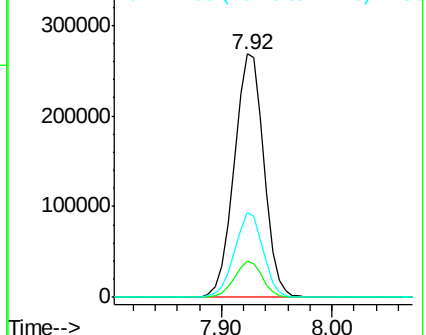

#9

Benzaldehyde

Concen: 4.223 ng

RT: 8.33 min Scan# 859

Delta R.T. 0.40 min

Lab File: BG031690.D

Acq: 22 Dec 2017 1:37


Tgt Ion: 77 Resp: 8869

Ion Ratio Lower Upper



77 100


105 98.8 71.3 111.3

106 80.6 64.2 104.2

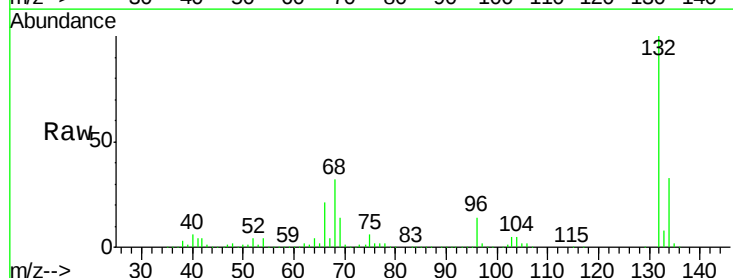

Abundance Ion 77.00 (76.70 to 77.70): BGC
Ion 105.00 (104.70 to 105.70): BGC
Ion 106.00 (105.70 to 106.70): BGC

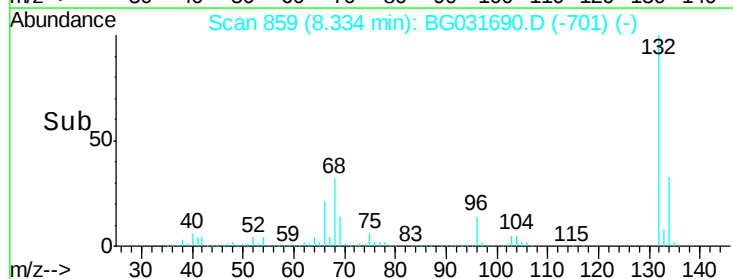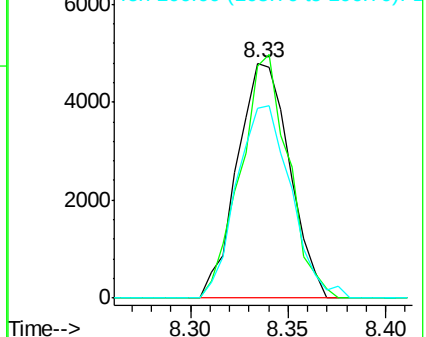

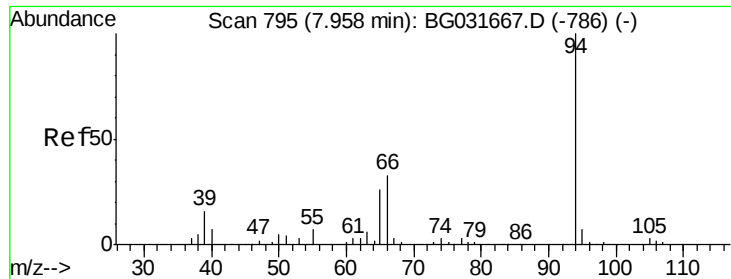

#10

Phenol

Concen: 5.655 ng

RT: 7.95 min Scan# 794

Delta R.T. -0.01 min

Lab File: BG031690.D

Acq: 22 Dec 2017 1:37

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 94 Resp: 19913

Ion Ratio Lower Upper




94 100

65 24.6 11.9 51.9

66 36.5 22.2 62.2



Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

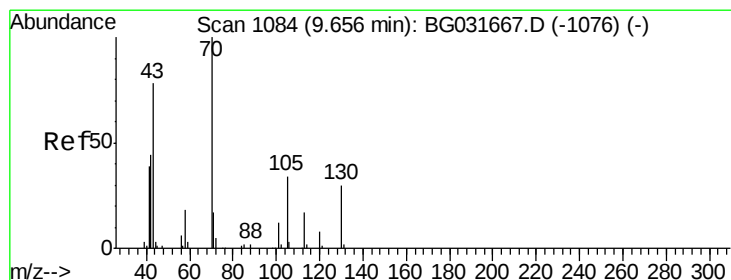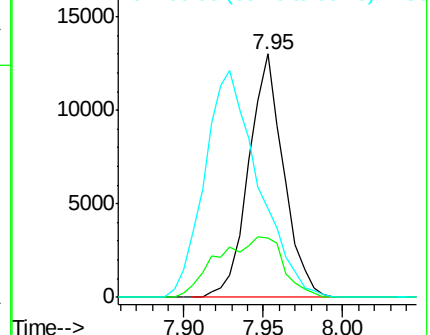

#19

n-Nitroso-di-n-propylamine

Concen: 13.825 ng

RT: 10.03 min Scan# 1147

Delta R.T. 0.37 min

Lab File: BG031690.D

Acq: 22 Dec 2017 1:37

Tgt Ion: 70 Resp: 32932


Ion Ratio Lower Upper

70 100



42 40.8 49.1 73.7#


101 0.0 8.5 12.7#

130 3.3 13.4 20.0#

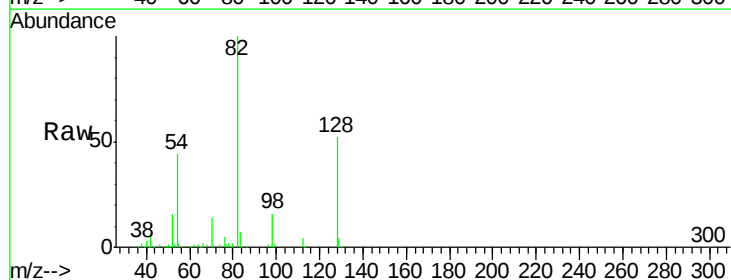

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC



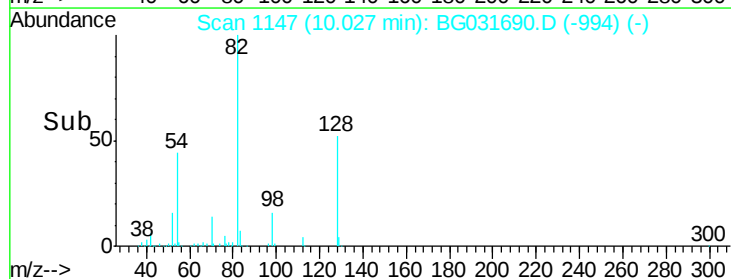
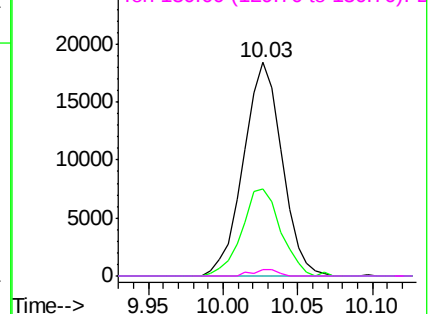


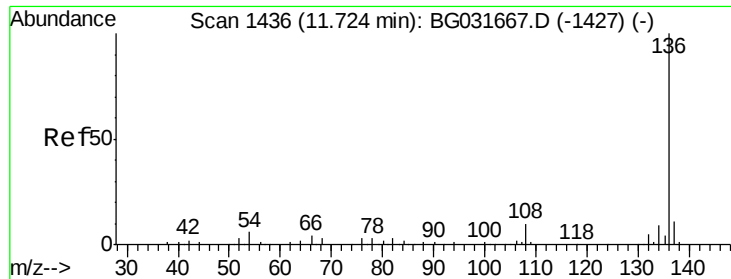

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.72 min Scan# 1435
Delta R.T. -0.01 min
Lab File: BG031690.D
Acq: 22 Dec 2017 1:37




Instrument :
BNA_G
ClientSampleId :


Tot Ion:136	Resp:	205437
Ion Ratio	Lower	Upper
136	100	
137	11.5	9.2 13.8
54	5.7	10.3 15.5#
68	3.0	4.5 6.7#

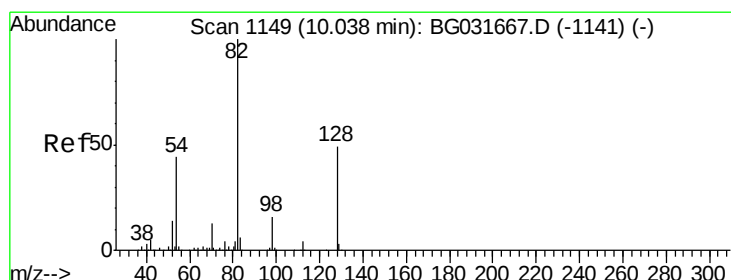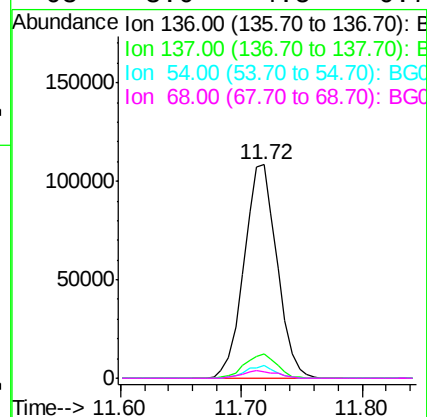

#23
Nitrobenzene-d5
Concen: 93.090 ng
RT: 10.03 min Scan# 1147
Delta R.T. -0.01 min
Lab File: BG031690.D
Acq: 22 Dec 2017 1:37

Tgt Ion: 82	Resp:	253259
Ion Ratio	Lower	Upper
82	100	
128	52.1	29.7 44.5#
54	43.9	43.1 64.7



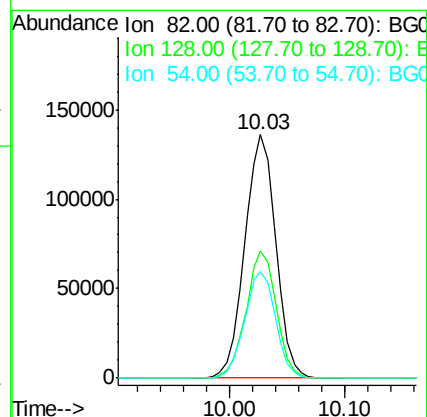



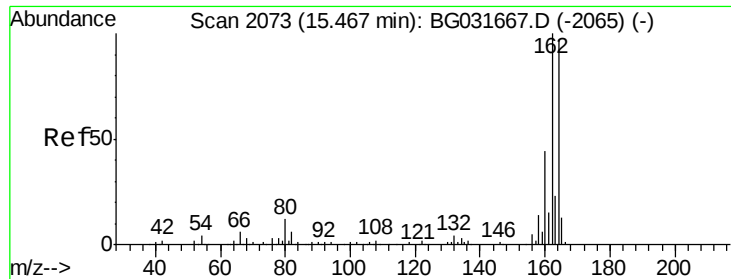

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.46 min Scan# 2072
 Delta R.T. -0.01 min
 Lab File: BG031690.D
 Acq: 22 Dec 2017 1:37




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
164	100		
162	103.8	78.8	118.2
160	45.5	35.4	53.0

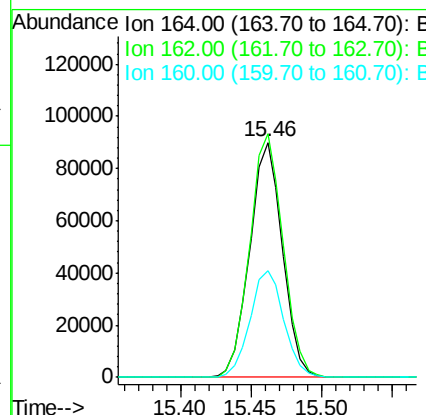

#41
 2,4,6-Tribromophenol
 Concen: 152.360 ng
 RT: 16.94 min Scan# 2323
 Delta R.T. -0.01 min
 Lab File: BG031690.D
 Acq: 22 Dec 2017 1:37

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.9	77.0	115.6
141	26.6	25.2	37.8

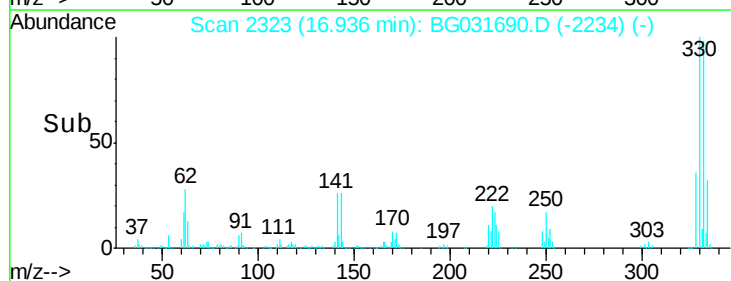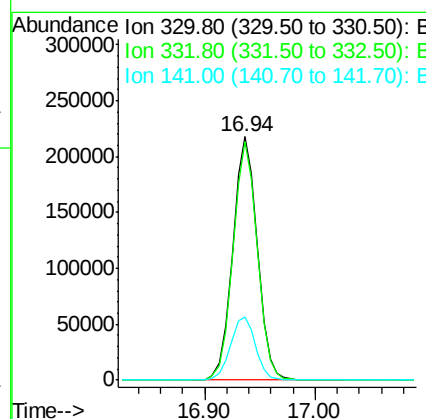







#44
2-Fluorobiphenyl
Concen: 82.070 ng
RT: 14.09 min Scan# 1839
Delta R.T. -0.01 min
Lab File: BG031690.D
Acq: 22 Dec 2017 1:37

Instrument :
BNA_G
ClientSampleId :

Tot Ion:172 Resp: 955569
Ion Ratio Lower Upper
172 100
171 37.6 30.0 45.0
170 23.8 19.5 29.3

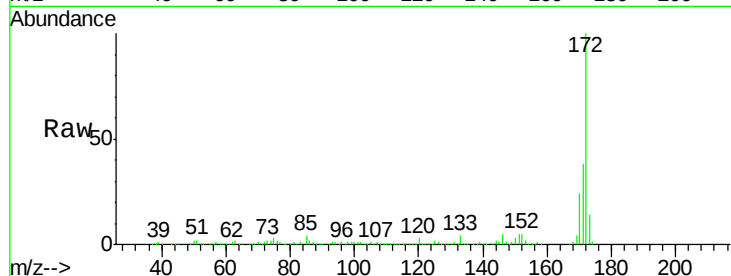


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E


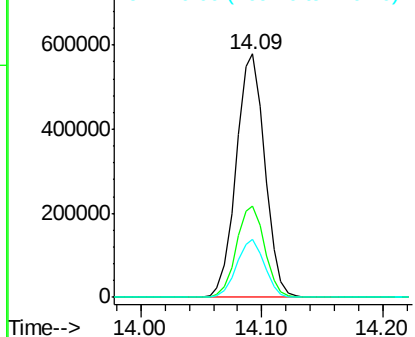



#49
Dimethylphthalate
Concen: 7.080 ng
RT: 14.89 min Scan# 1974
Delta R.T. -0.02 min
Lab File: BG031690.D
Acq: 22 Dec 2017 1:37

Tgt Ion:163 Resp: 91147
Ion Ratio Lower Upper
163 100
194 4.5 3.4 5.2
164 10.0 8.2 12.4



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

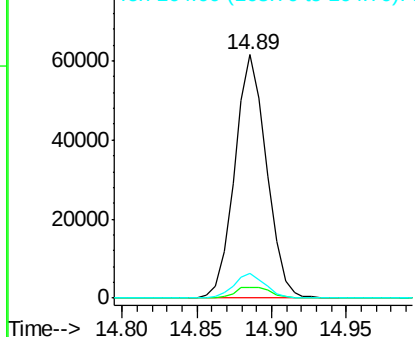


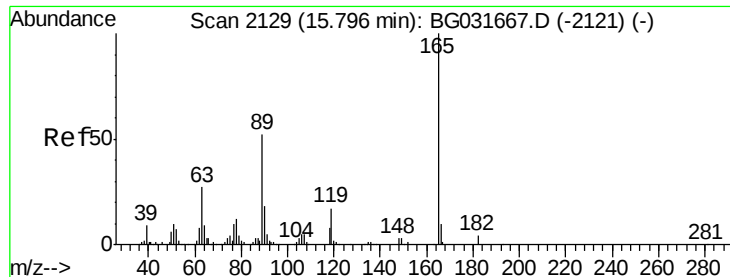

#56
2,4-Dinitrotoluene
Concen: 6.397 ng
RT: 15.46 min Scan# 2072
Delta R.T. -0.33 min
Lab File: BG031690.D
Acq: 22 Dec 2017 1:37

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	0.0	42.0	63.0#
89	1.3	66.9	100.3#
182	0.0	2.6	3.8#



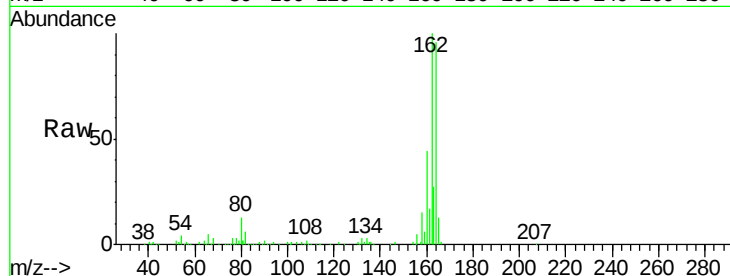


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC


Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

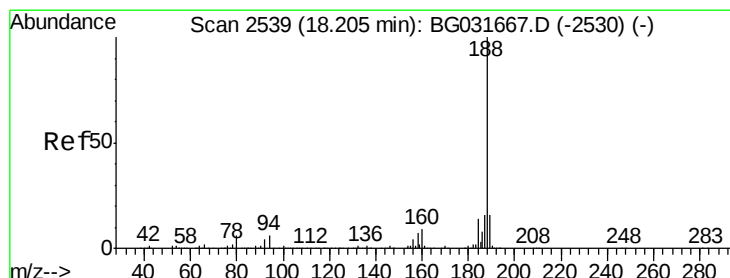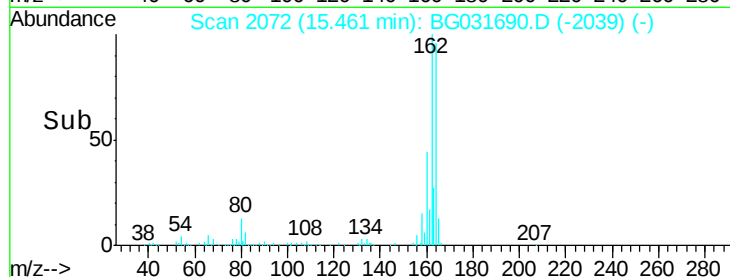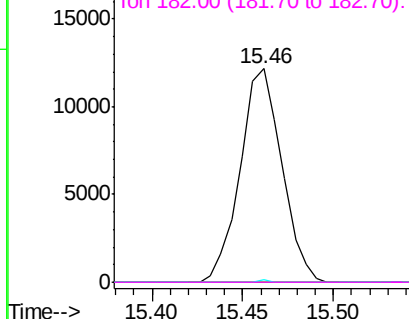

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 18.20 min Scan# 2538
Delta R.T. -0.01 min
Lab File: BG031690.D
Acq: 22 Dec 2017 1:37



Tgt Ion	Ratio	Lower	Upper
188	100		
94	5.1	6.9	10.3#
80	5.7	7.7	11.5#

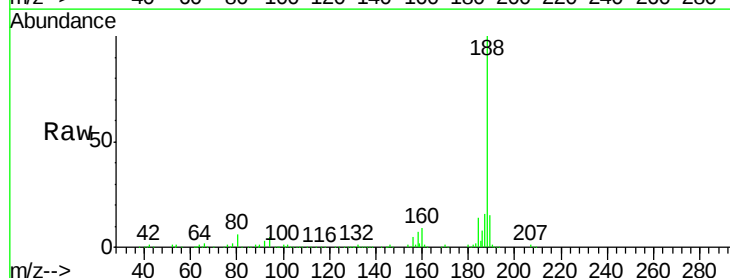


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

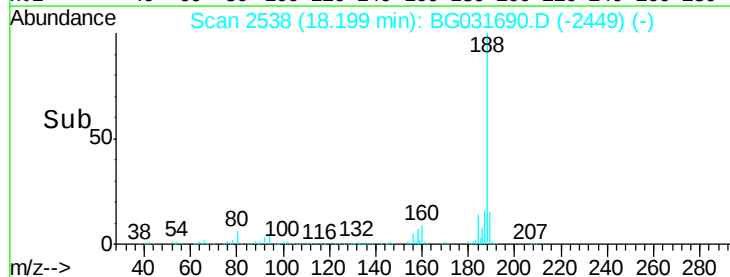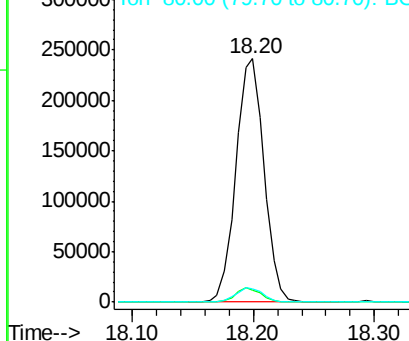


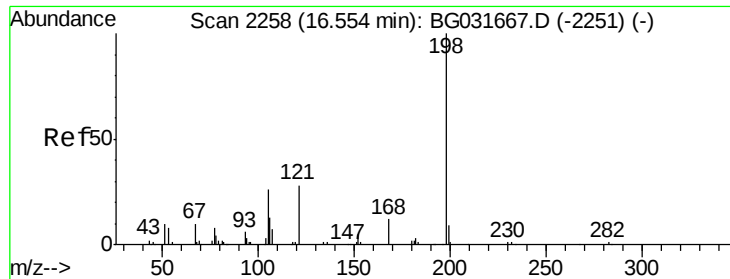




#64
4,6-Dinitro-2-methylphenol
Concen: 8.650 ng
RT: 16.93 min Scan# 2322
Delta R.T. 0.38 min
Lab File: BG031690.D
Acq: 22 Dec 2017 1:37

Instrument :
BNA_G
ClientSampled :

Tot Ion:198 Resp: 791
Ion Ratio Lower Upper
198 100
51 71.9 30.6 70.6#
105 136.2 23.8 63.8#

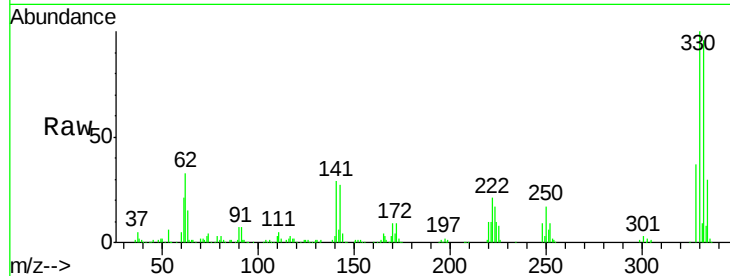


Abundance Ion 198.00 (197.70 to 198.70): E
Ion 51.00 (50.70 to 51.70): BGC
Ion 105.00 (104.70 to 105.70): E

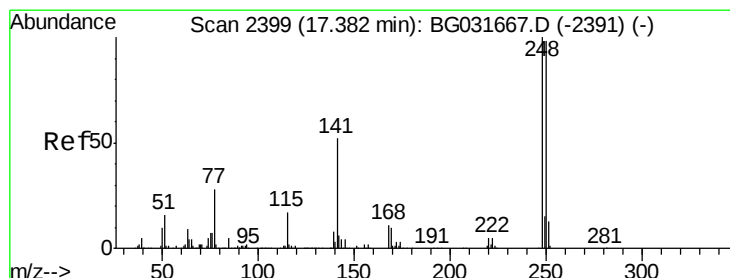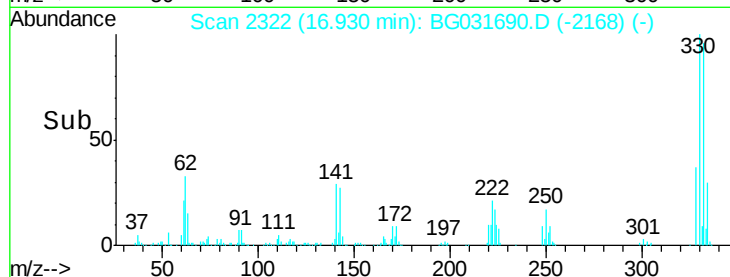
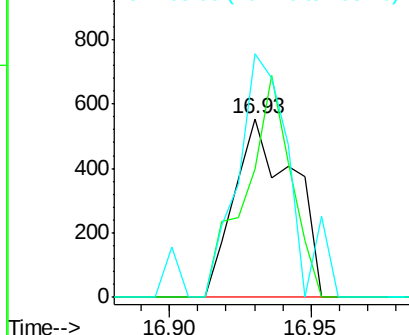



#66
4-Bromophenyl-phenylether
Concen: 4.827 ng
RT: 16.94 min Scan# 2323
Delta R.T. -0.45 min
Lab File: BG031690.D
Acq: 22 Dec 2017 1:37

Tgt Ion:248 Resp: 27295
Ion Ratio Lower Upper
248 100
250 206.5 77.1 115.7#
141 320.6 50.8 76.2#

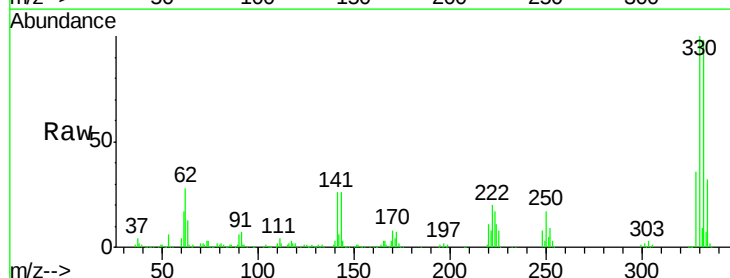

Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

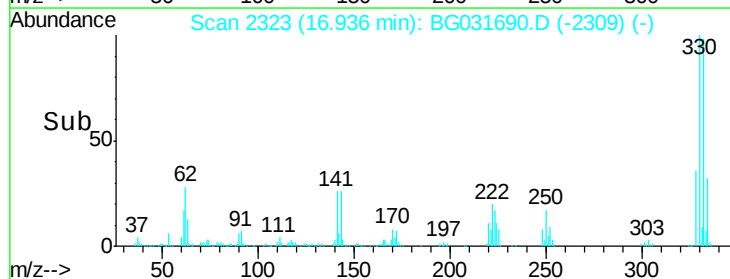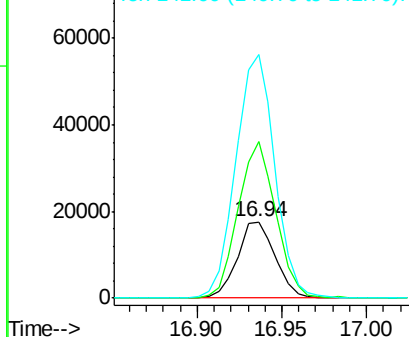

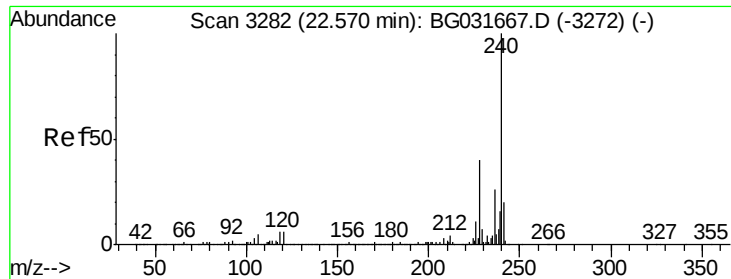

#75

Chrysene-d12

Concen: 20.000 ng

RT: 22.56 min Scan# 3280

Delta R.T. -0.01 min

Lab File: BG031690.D

Acq: 22 Dec 2017 1:37

Instrument :

BNA_G

ClientSampleId :


Tot Ion:240 Resp: 444739

Ion Ratio Lower Upper

240 100

120 5.5 6.8 10.2#




236 25.6 20.9 31.3

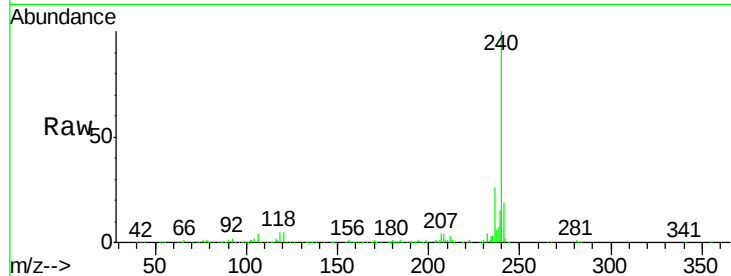

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

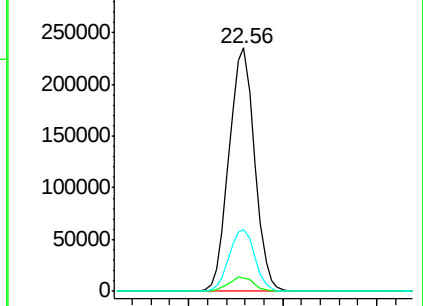

#78

Terphenyl-d14

Concen: 85.674 ng

RT: 20.73 min Scan# 2969

Delta R.T. -0.01 min

Lab File: BG031690.D

Acq: 22 Dec 2017 1:37


Tgt Ion:244 Resp: 1667760

Ion Ratio Lower Upper

244 100

212 7.3 5.8 8.8



122 7.0 7.0 10.4




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

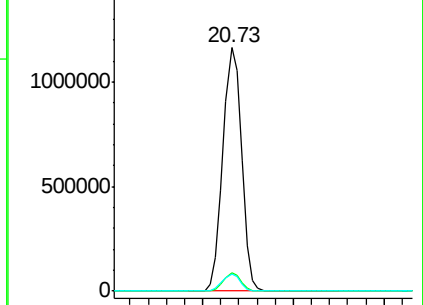


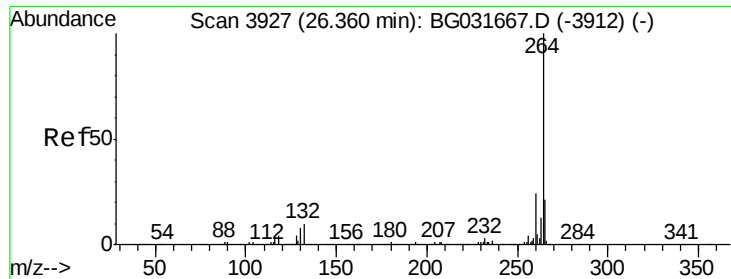

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 26.34 min Scan# 3924
 Delta R.T. -0.02 min
 Lab File: BG031690.D
 Acq: 22 Dec 2017 1:37

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.5	17.4	26.0
265	22.1	17.7	26.5



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

