
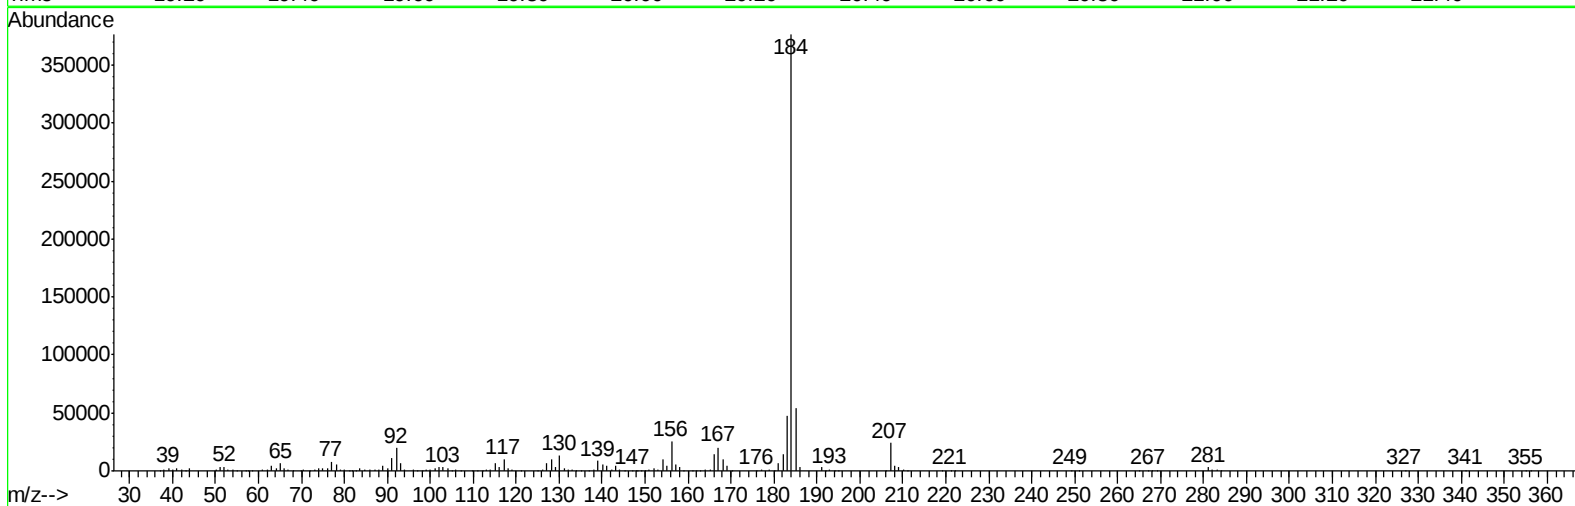


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122117\
Data File : BG031663.D
Acq On : 21 Dec 2017 8:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 06:41:04 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 03:38:35 2017
Response via : Initial Calibration

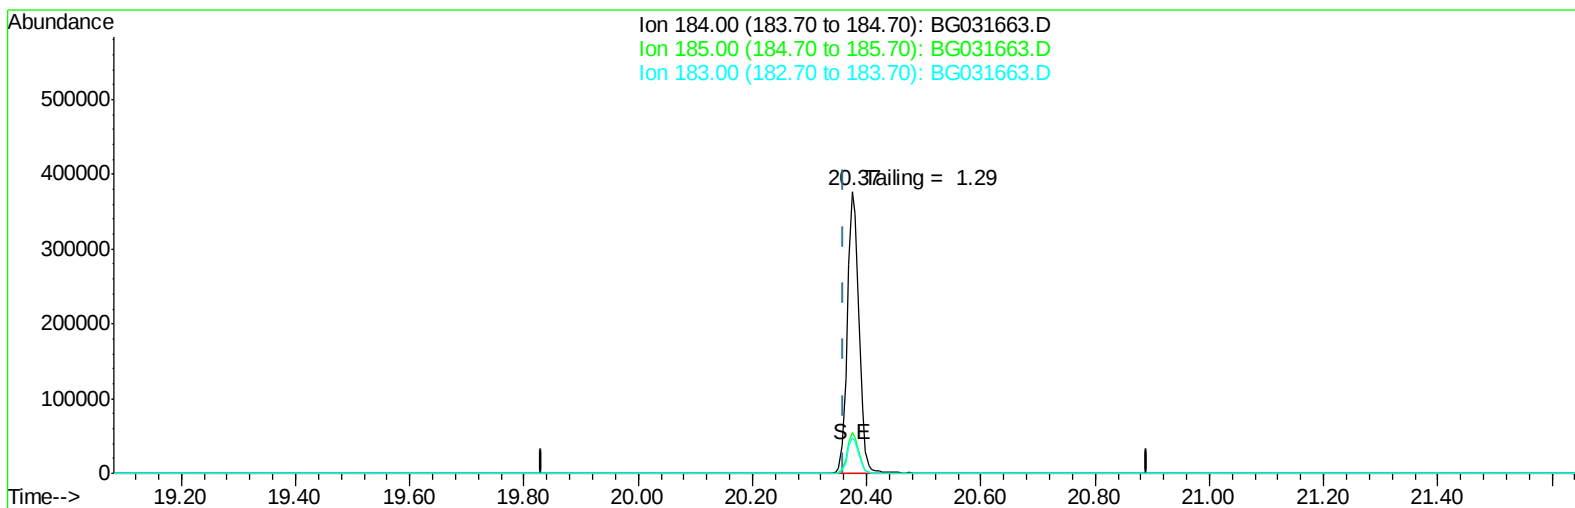

TIC: BG031663.D

(76) Benzidine



20.374min (+0.013) 19053.52ng

response 542223

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.48
183.00	13.30	12.77
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122117\
Data File : BG031663.D
Acq On : 21 Dec 2017 8:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 06:41:04 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 03:38:35 2017
Response via : Initial Calibration

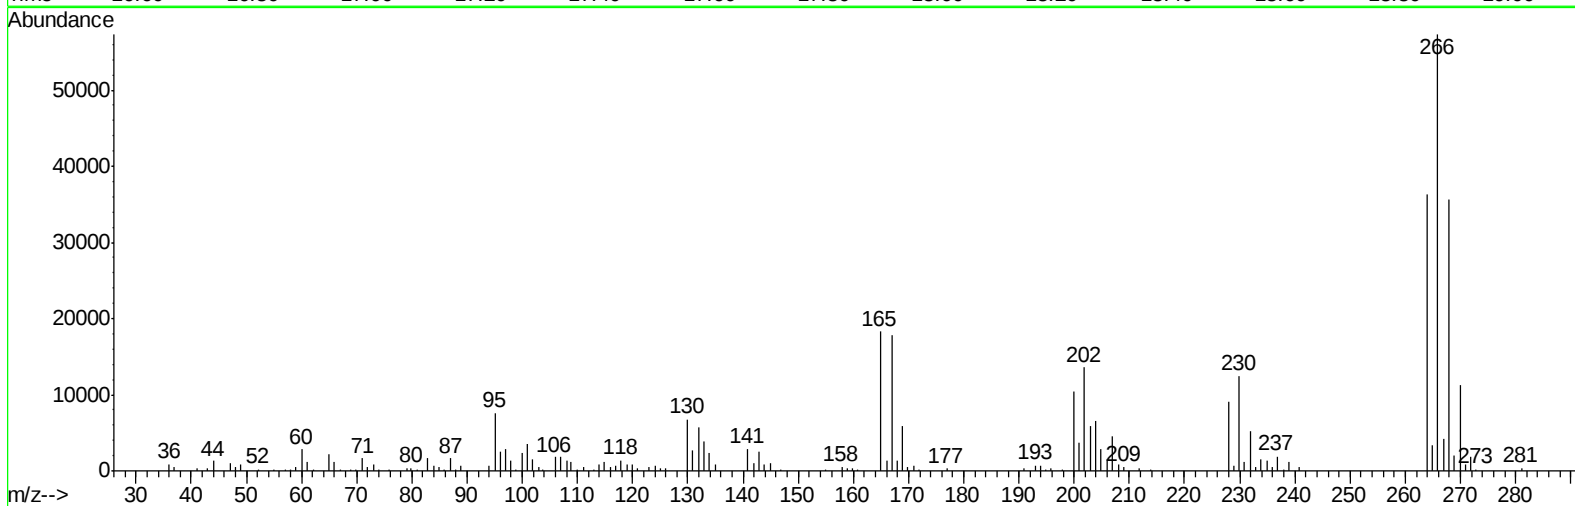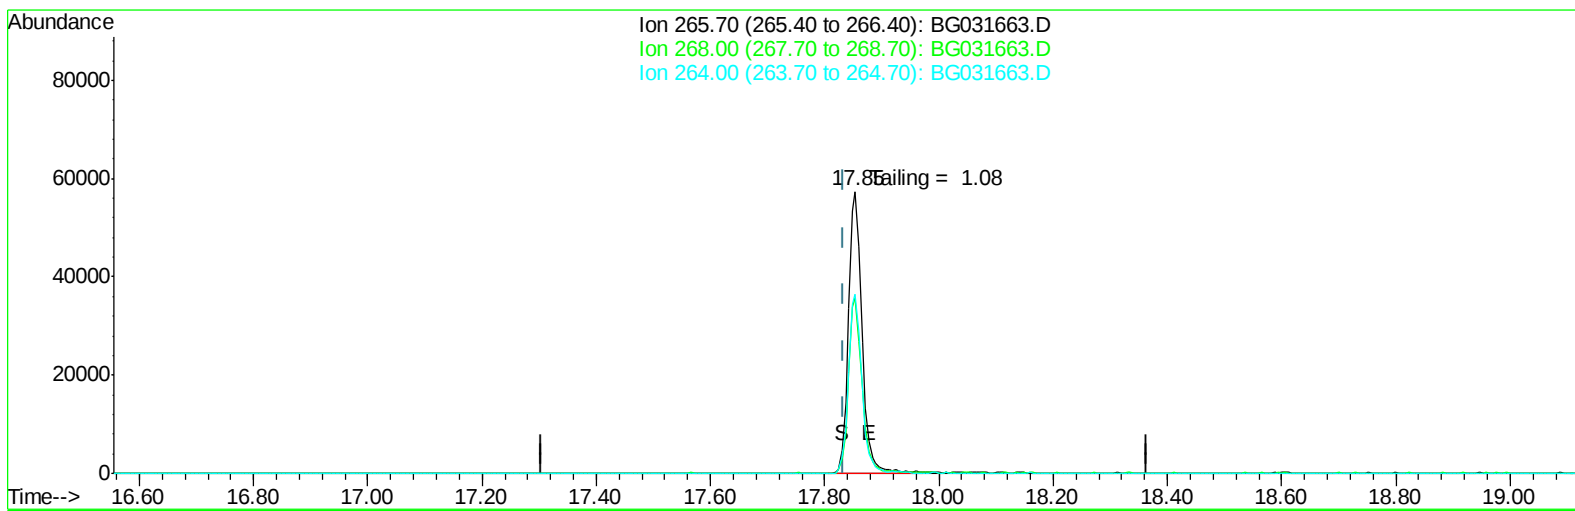

TIC: BG031663.D

(69) Pentachlorophenol (C)

17.854min (+0.019) 0.00ng

response 95378

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.33
264.00	62.00	63.50
0.00	0.00	0.00