
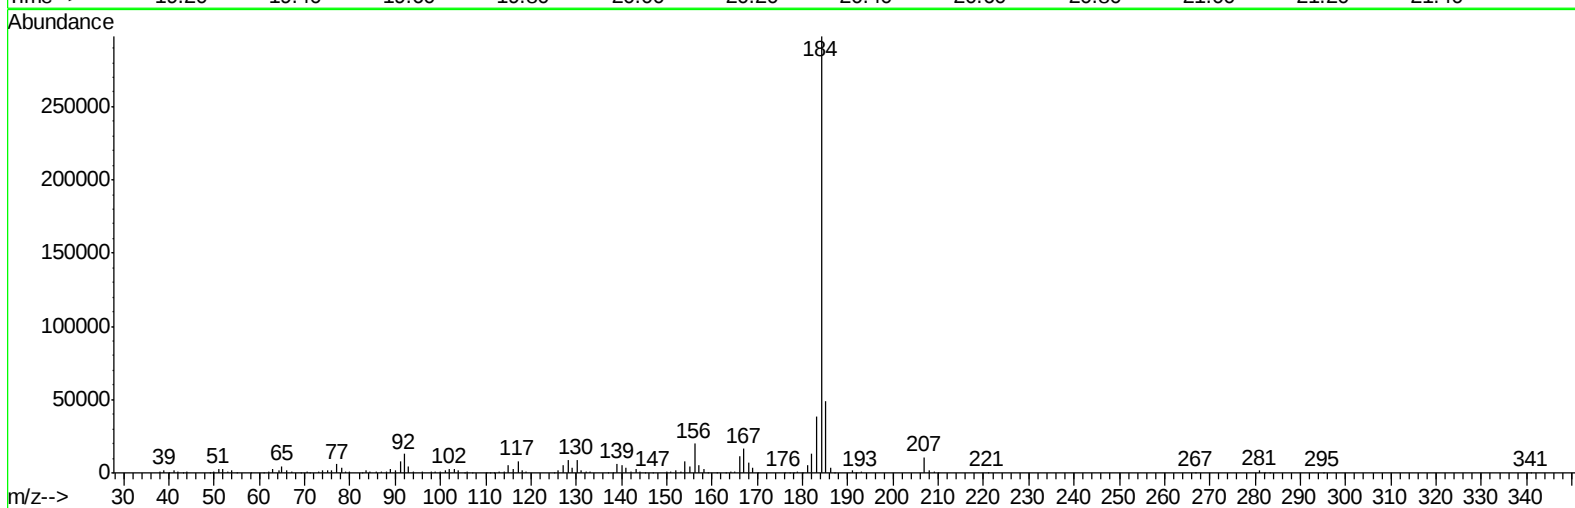


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122117\  
Data File : BG031674.D  
Acq On : 21 Dec 2017 15:35  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 06:44:08 2017  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 22 03:38:35 2017  
Response via : Initial Calibration

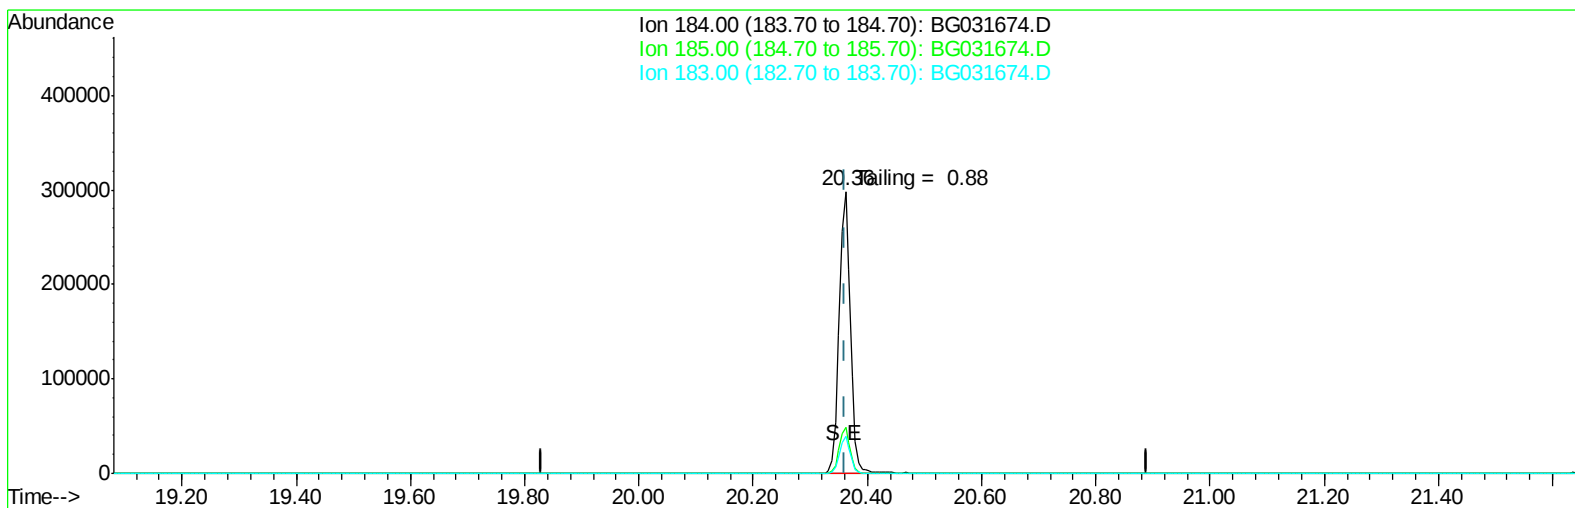

TIC: BG031674.D

(76) Benzidine



20.361min (+0.000) 0.00ng

response 407805

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 13.90 | 16.32 |
| 183.00 | 13.30 | 13.01 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122117\  
Data File : BG031674.D  
Acq On : 21 Dec 2017 15:35  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 06:44:08 2017  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 22 03:38:35 2017  
Response via : Initial Calibration

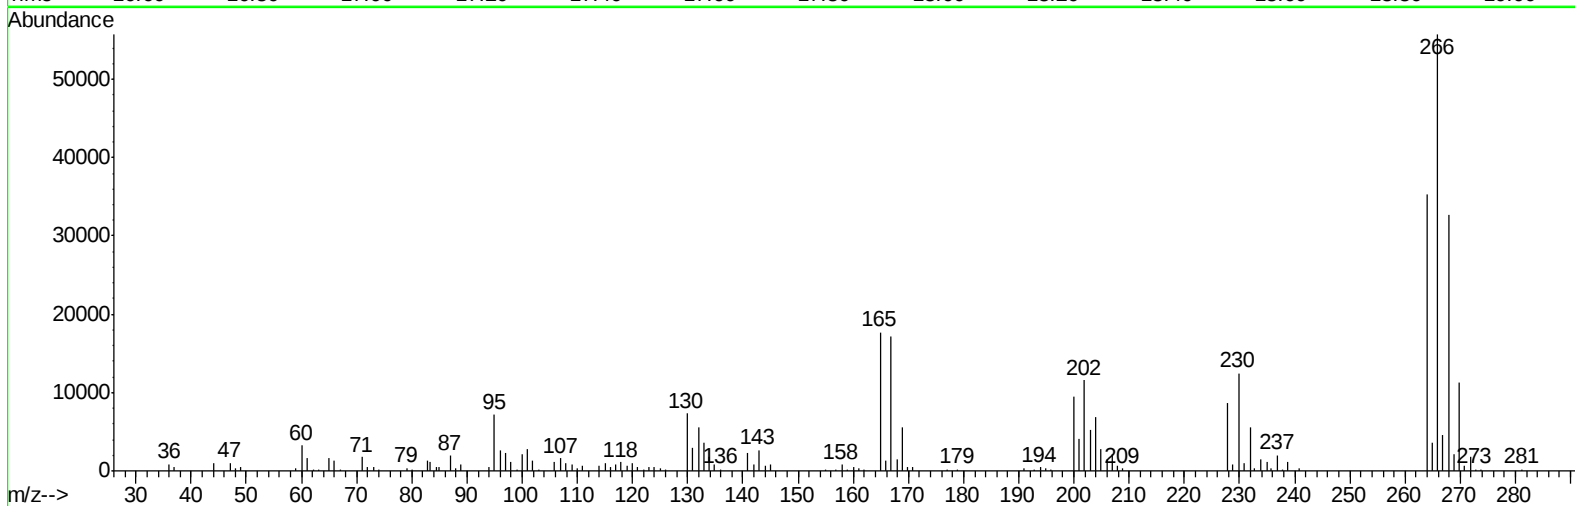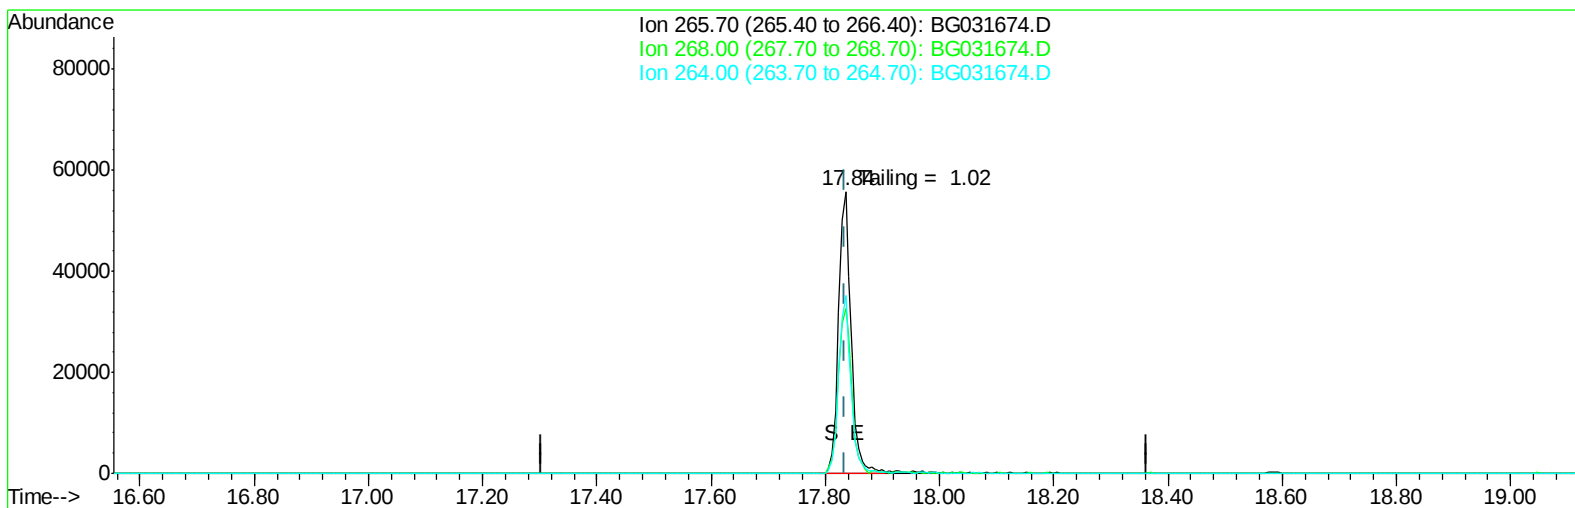

TIC: BG031674.D

(69) Pentachlorophenol (C)

17.835min (+0.000) 92614.34ng

response 84751

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 58.76 |
| 264.00 | 62.00 | 63.40 |
| 0.00   | 0.00  | 0.00  |