
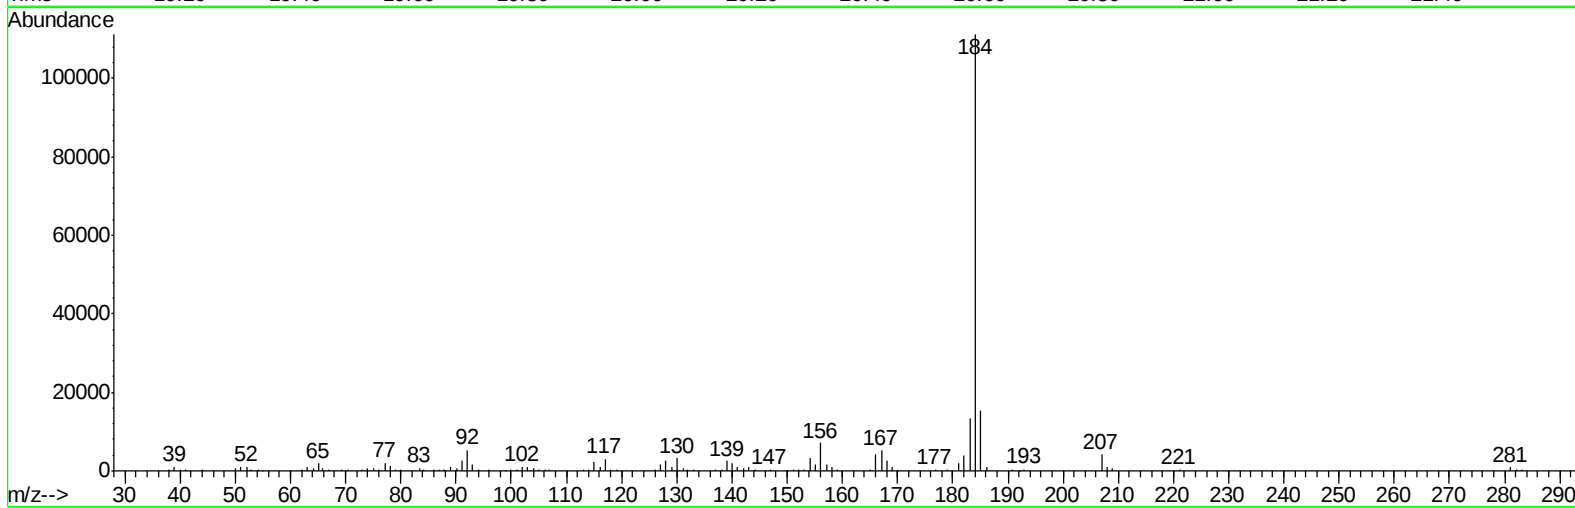


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122117\
Data File : BG031693.D
Acq On : 22 Dec 2017 3:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 06:47:12 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 03:38:35 2017
Response via : Initial Calibration

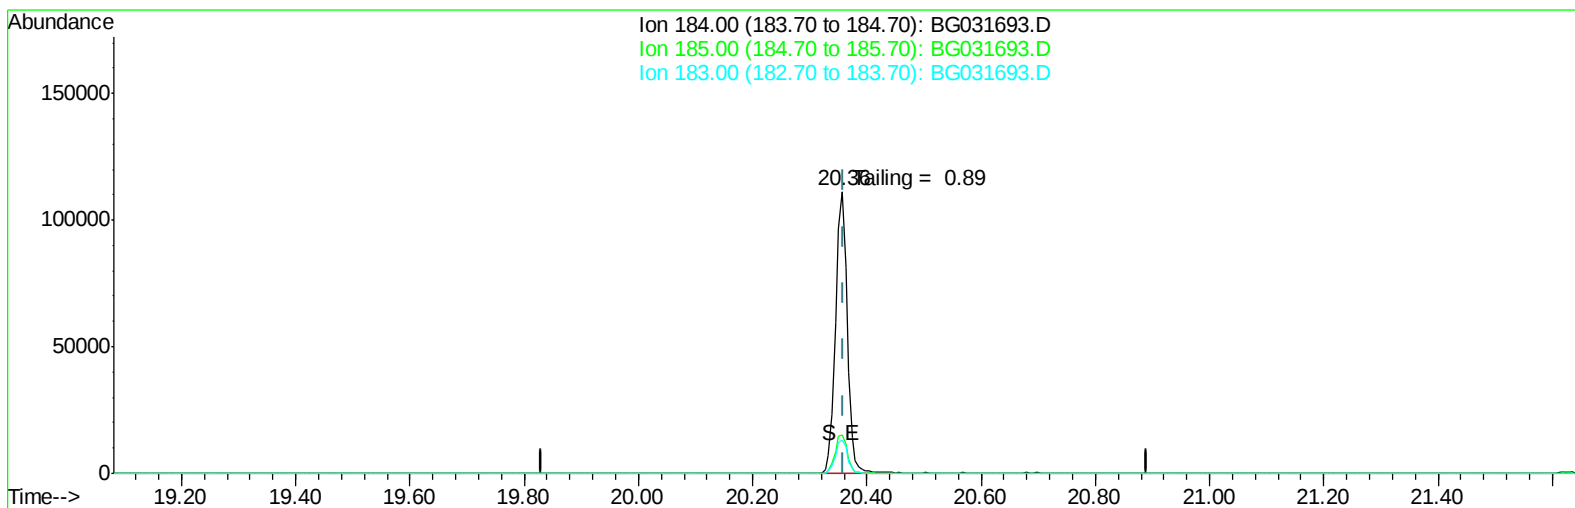

TIC: BG031693.D

(76) Benzidine



20.356min (-0.005) 0.00ng

response 159121

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.80
183.00	13.30	12.03
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122117\
Data File : BG031693.D
Acq On : 22 Dec 2017 3:29
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 06:47:12 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 03:38:35 2017
Response via : Initial Calibration

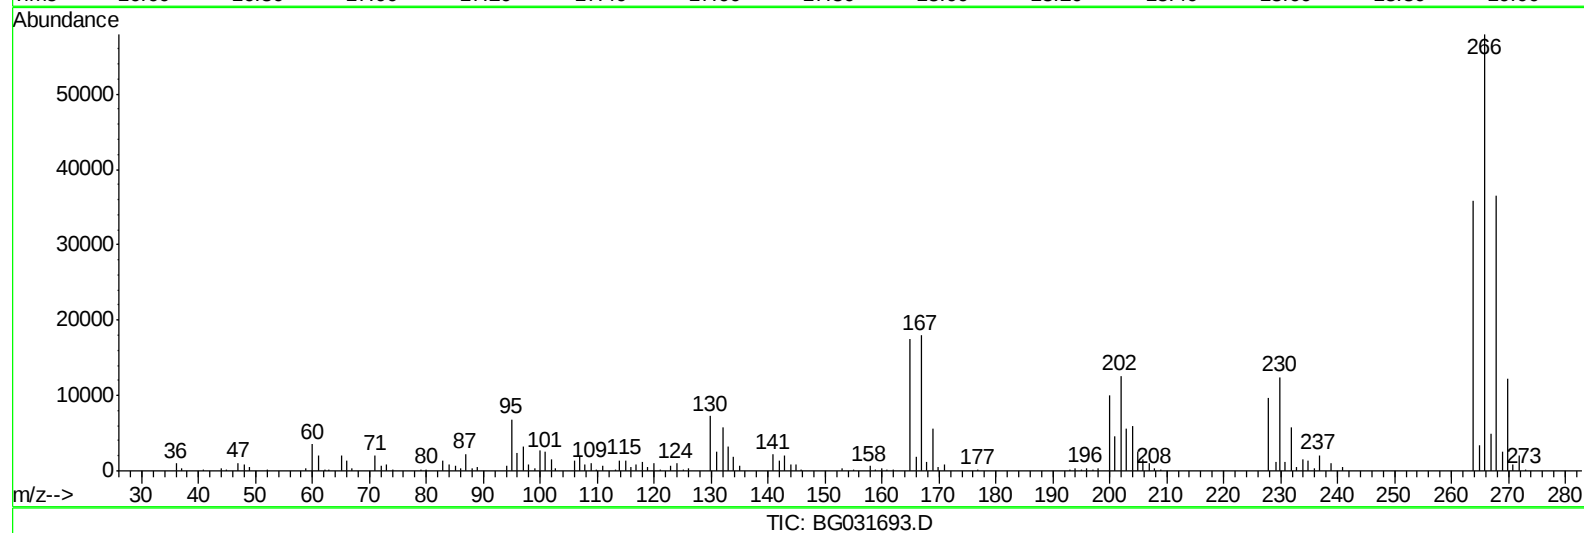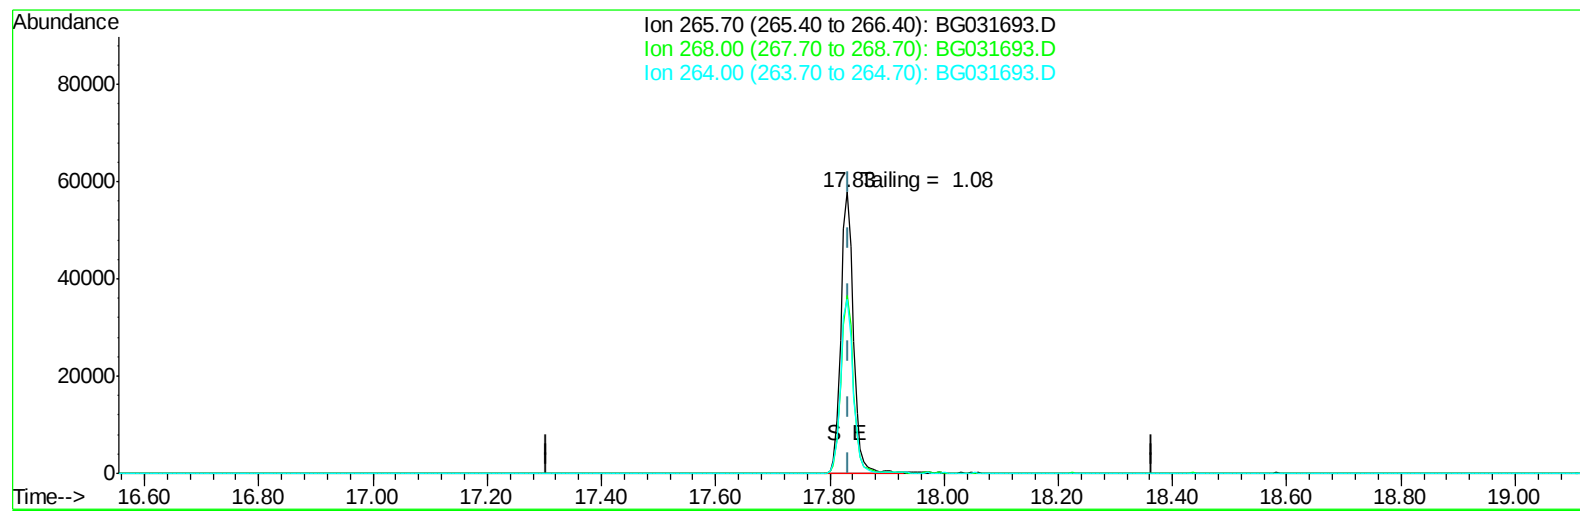

(69) Pentachlorophenol (C)

17.830min (-0.005) 25829.41ng

response 87192

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.02
264.00	62.00	61.80
0.00	0.00	0.00