


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122117\
 Data File : BG031663.D
 Acq On : 21 Dec 2017 8:32
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 22 11:08:55 2017

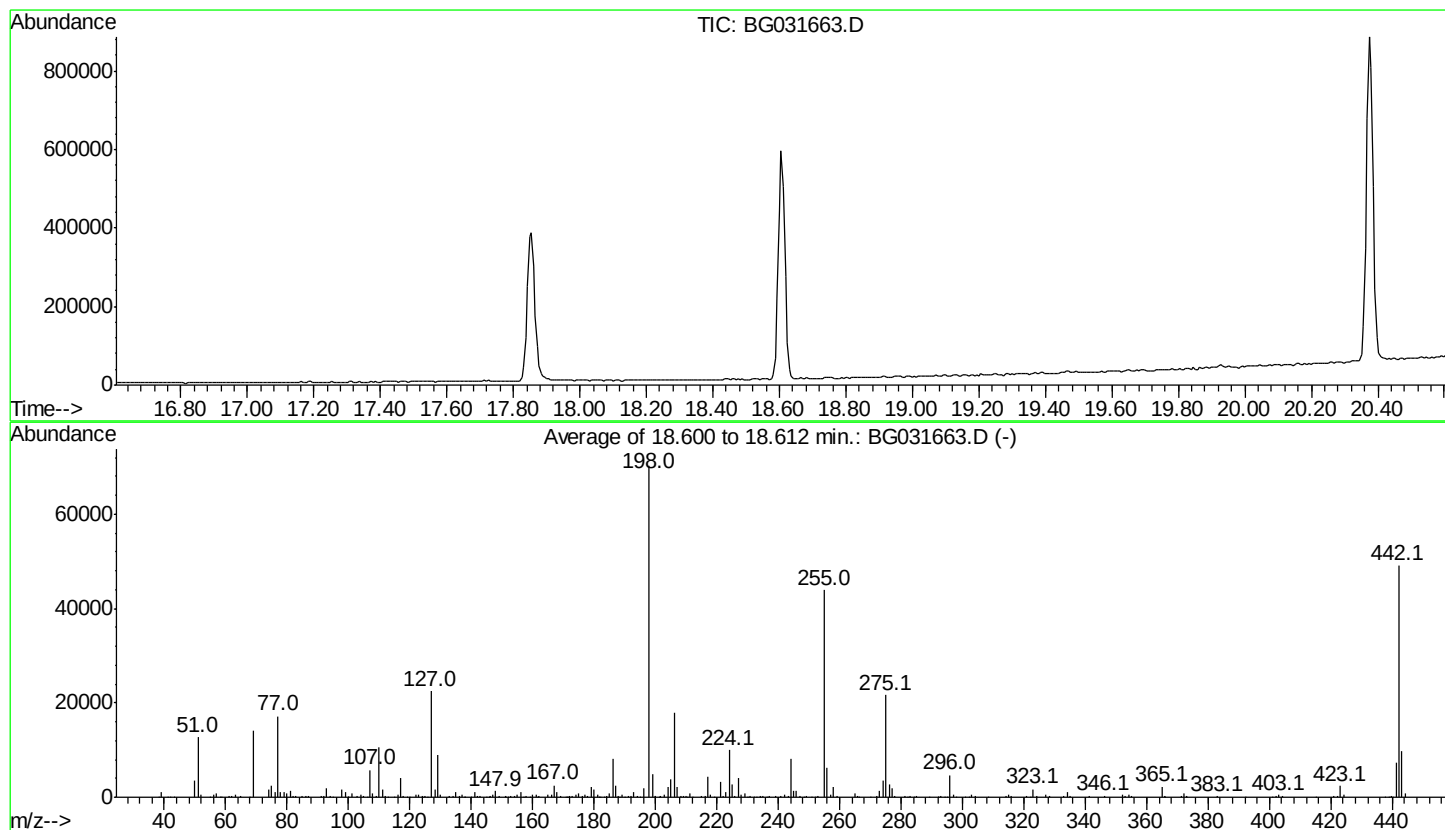

AutoFind: Scans 2606, 2607, 2608; Background Corrected with Scan 2600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.1	12750	PASS
68	69	0.00	2	0.8	108	PASS
69	198	0.00	100	20.2	14219	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.0	22477	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70309	PASS
199	198	5	9	6.9	4845	PASS
275	198	10	60	30.8	21648	PASS
365	198	1	100	3.2	2237	PASS
441	442	0.01	24	14.8	7268	PASS
442	198	50	100	69.8	49106	PASS
443	442	15	24	19.8	9733	PASS