


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122117\
 Data File : BG031674.D
 Acq On : 21 Dec 2017 15:35
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 22 11:08:55 2017

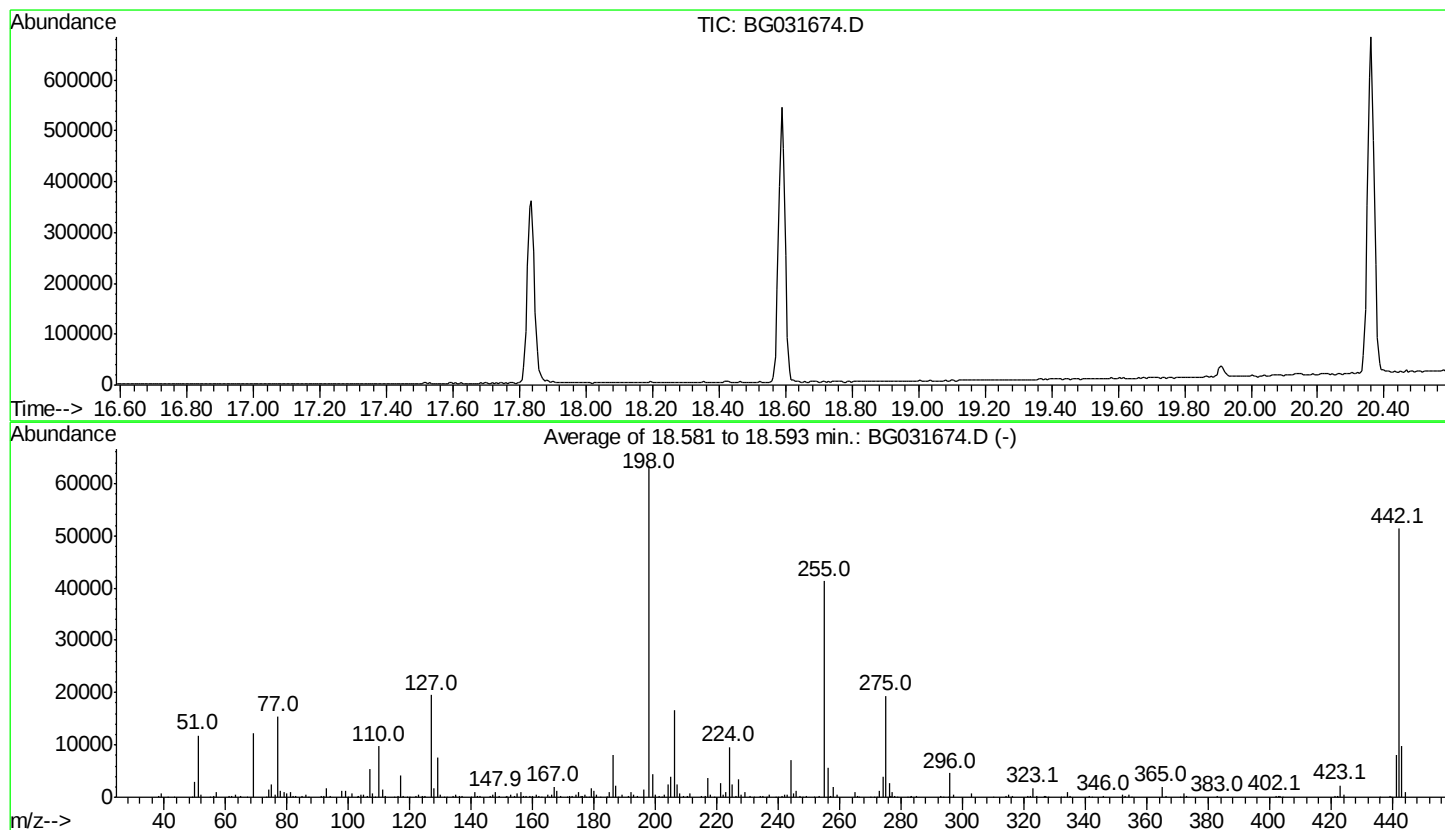

AutoFind: Scans 2603, 2604, 2605; Background Corrected with Scan 2596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.7	11853	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	19.4	12272	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	30.8	19552	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63394	PASS
199	198	5	9	7.0	4427	PASS
275	198	10	60	30.5	19354	PASS
365	198	1	100	3.2	2017	PASS
441	442	0.01	24	15.7	8059	PASS
442	198	50	100	81.0	51349	PASS
443	442	15	24	19.0	9769	PASS