


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122117\
 Data File : BG031693.D
 Acq On : 22 Dec 2017 3:29
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 22 11:08:55 2017

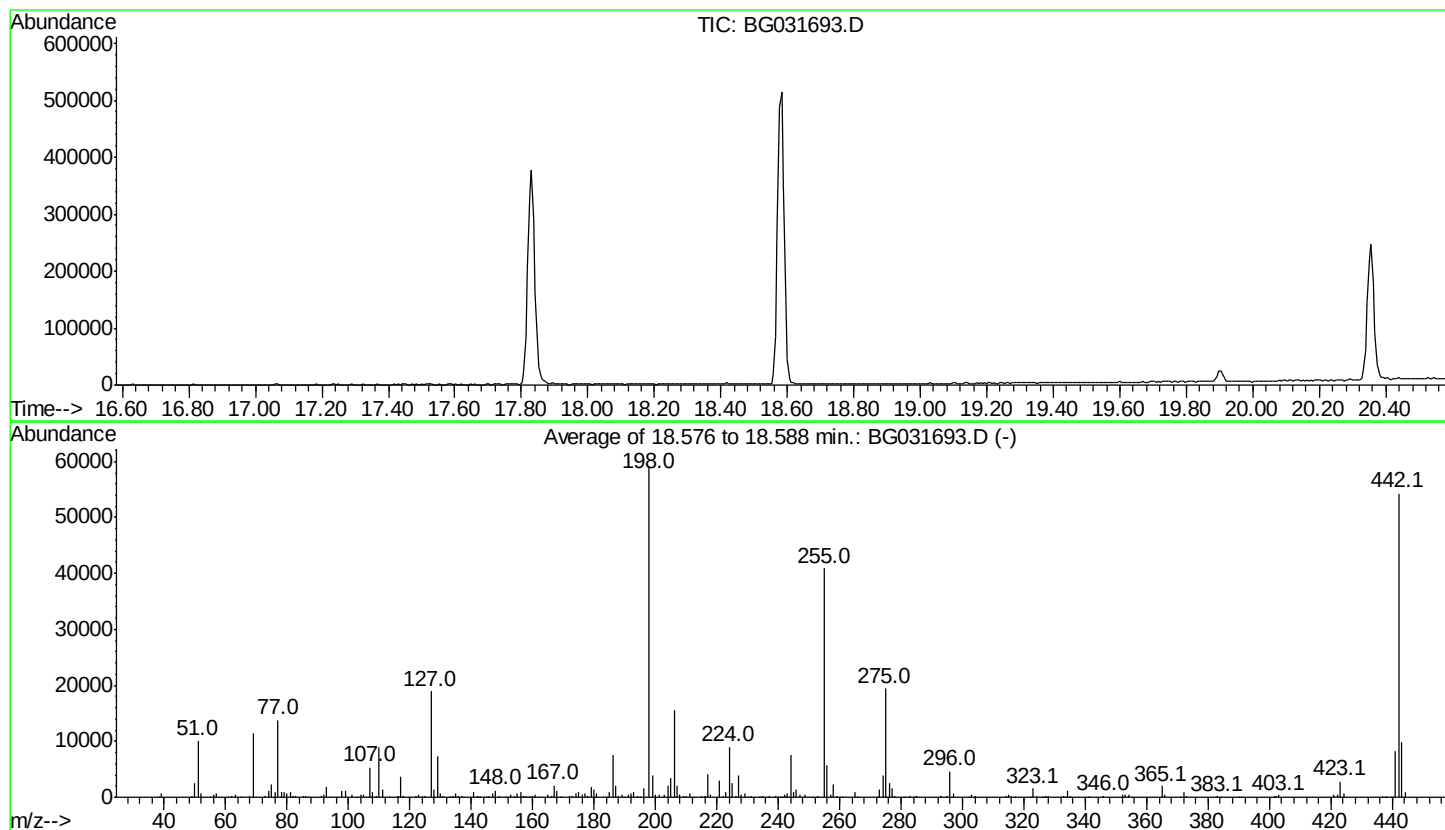

AutoFind: Scans 2602, 2603, 2604; Background Corrected with Scan 2595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	17.1	10108	PASS
68	69	0.00	2	1.5	168	PASS
69	198	0.00	100	19.3	11428	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.0	18951	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59264	PASS
199	198	5	9	6.7	3944	PASS
275	198	10	60	32.8	19426	PASS
365	198	1	100	3.4	2012	PASS
441	442	0.01	24	15.4	8346	PASS
442	198	50	100	91.5	54234	PASS
443	442	15	24	18.2	9894	PASS