
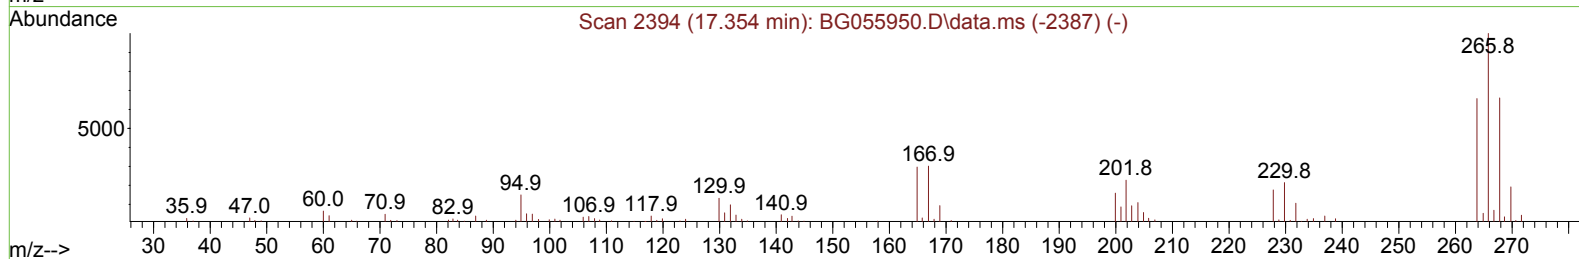
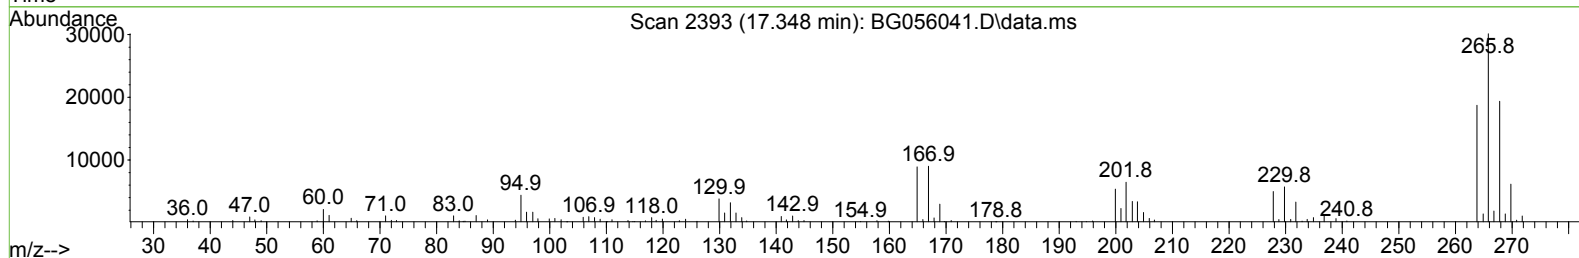


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122122\
Data File : BG056041.D
Acq On : 21 Dec 2022 9:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 04:13:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 01:11:10 2022
Response via : Initial Calibration

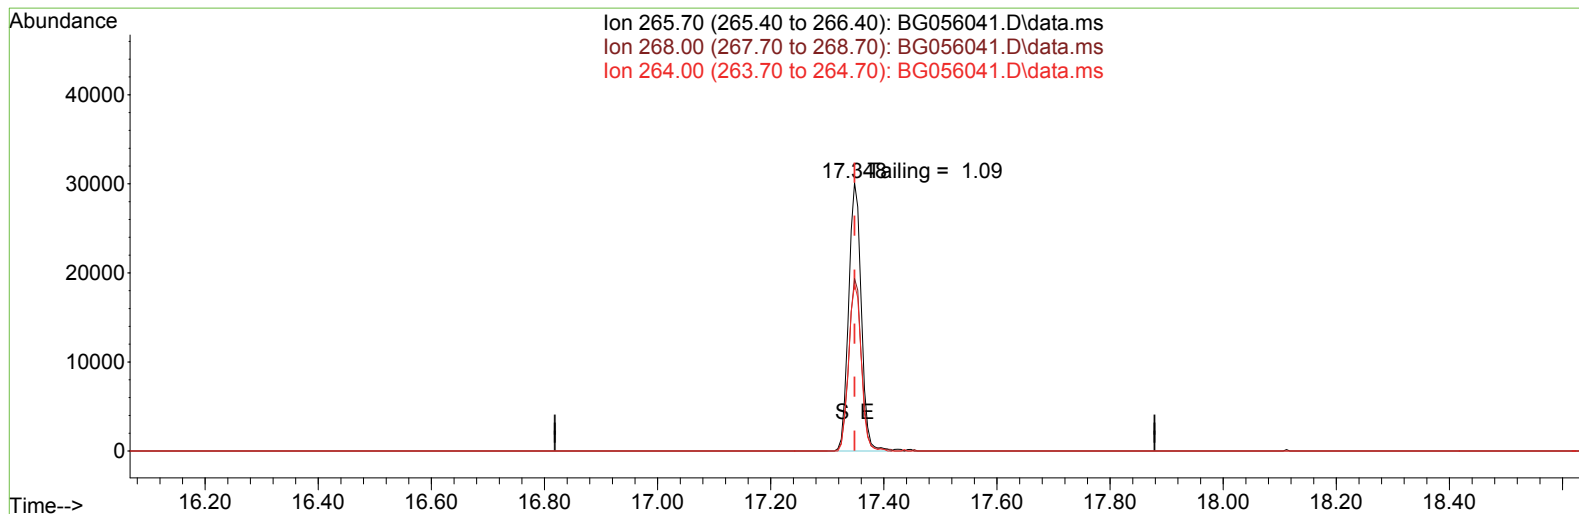

TIC: BG056041.D\data.ms

(70) Pentachlorophenol (C)




17.348min (-0.000) 73079.46 ng

response 46752

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.40	64.24
264.00	65.70	62.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122122\
Data File : BG056041.D
Acq On : 21 Dec 2022 9:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 04:13:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 01:11:10 2022
Response via : Initial Calibration

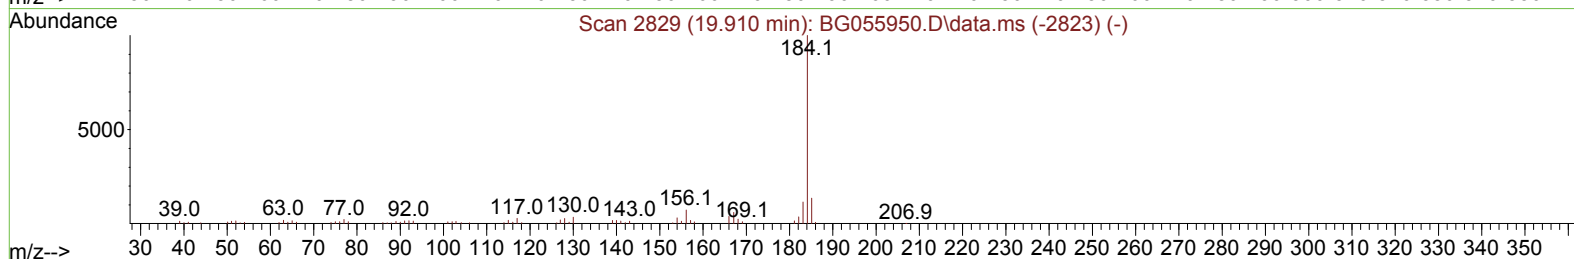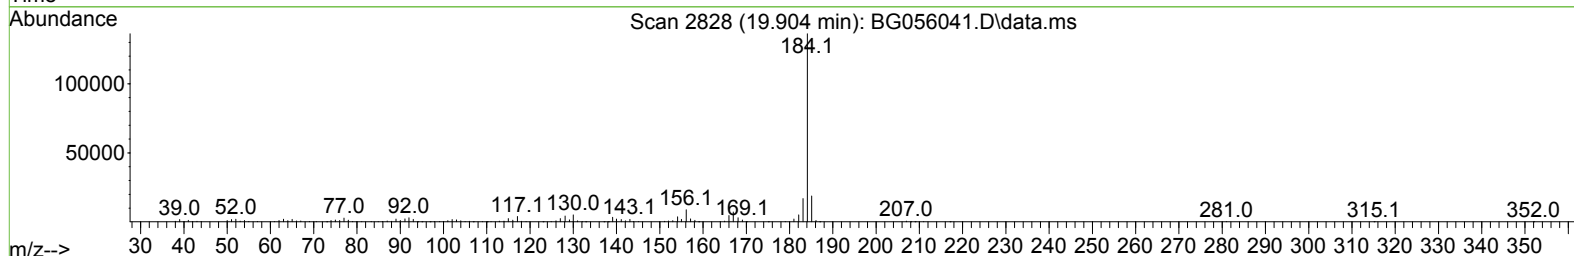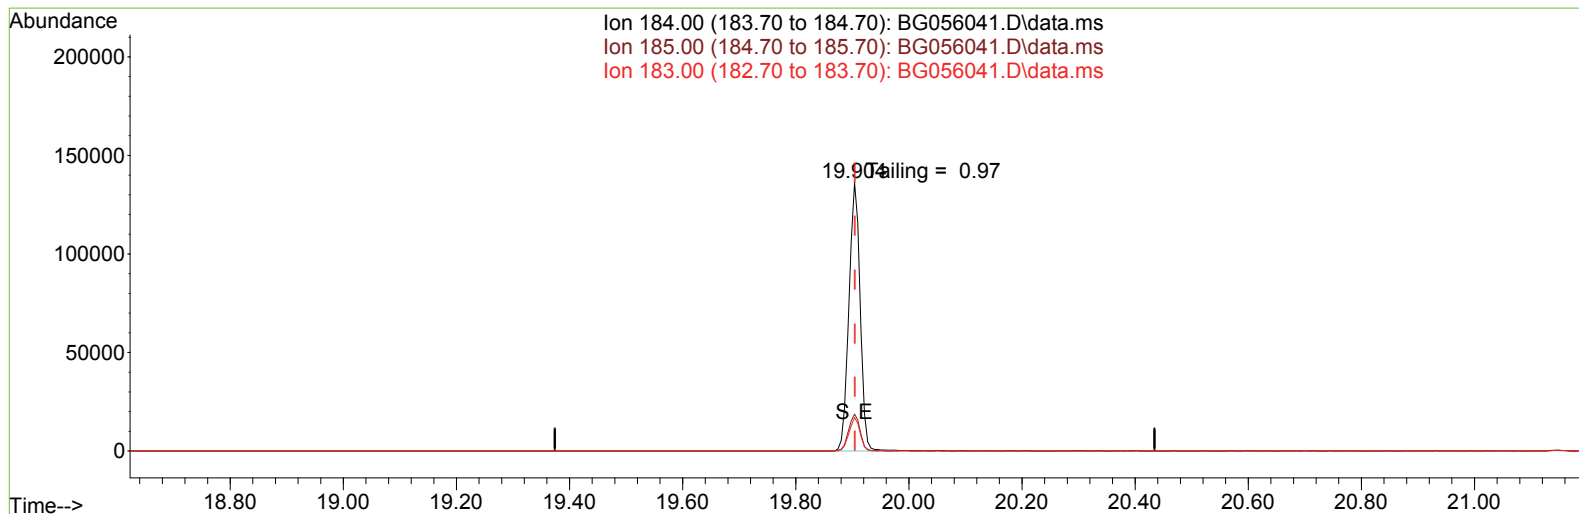

TIC: BG056041.D\data.ms

(77) Benzidine

19.904min (-0.000) 188989.92 ng

response 189182

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.82
183.00	11.50	12.46
0.00	0.00	0.00