

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122122\
 Data File : BG056056.D
 Acq On : 21 Dec 2022 20:08
 Operator : CG/JU
 Sample : N6071-05 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FVSub-TP7-COMP-07

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG056056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.394	13	18	25	rVB2	2514	3996	1.71%	0.316%
2	5.879	436	441	446	rBB	14663	21698	9.29%	1.718%
3	7.495	710	716	721	rBV	15371	24884	10.65%	1.970%
4	8.364	858	864	870	rBB	42779	71833	30.74%	5.687%
5	9.533	1058	1063	1068	rBB3	9263	15307	6.55%	1.212%
6	11.196	1339	1346	1353	rBB	57514	98298	42.07%	7.782%
7	13.593	1749	1754	1761	rBB	32174	46421	19.87%	3.675%
8	14.968	1981	1988	1995	rBB	98100	153335	65.63%	12.139%
9	16.443	2234	2239	2246	rVB	36079	50366	21.56%	3.987%
10	17.706	2448	2454	2464	rVB	135928	204685	87.61%	16.204%
11	18.546	2594	2597	2601	rBV4	3711	5810	2.49%	0.460%
12	18.881	2651	2654	2659	rBV4	1763	3101	1.33%	0.245%
13	18.999	2672	2674	2678	rVB4	2622	3154	1.35%	0.250%
14	19.058	2678	2684	2685	rBV5	3305	5310	2.27%	0.420%
15	19.363	2734	2736	2739	rBV4	2308	2928	1.25%	0.232%
16	19.557	2766	2769	2772	rBV5	3360	5227	2.24%	0.414%
17	19.581	2772	2773	2775	rVB2	3960	2596	1.11%	0.206%
18	19.657	2784	2786	2789	rBV4	3356	4295	1.84%	0.340%
19	19.727	2796	2798	2799	rBV2	4217	3204	1.37%	0.254%
20	19.804	2809	2811	2813	rBV3	3701	3067	1.31%	0.243%
21	19.839	2815	2817	2819	rBV3	3678	3328	1.42%	0.263%
22	20.168	2871	2873	2875	rBV3	5837	5157	2.21%	0.408%
23	20.203	2877	2879	2882	rVB4	6598	4820	2.06%	0.382%
24	20.274	2887	2891	2899	rVB	65920	98142	42.00%	7.769%
25	22.013	3181	3187	3193	rVB	137134	233645	100.00%	18.496%
26	25.503	3775	3781	3791	rVB2	64506	188590	80.72%	14.930%


Sum of corrected areas: 1263197

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122122\
Data File : BG056056.D
Acq On : 21 Dec 2022 20:08
Operator : CG/JU
Sample : N6071-05 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FVSUB-TP7-COMP-07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

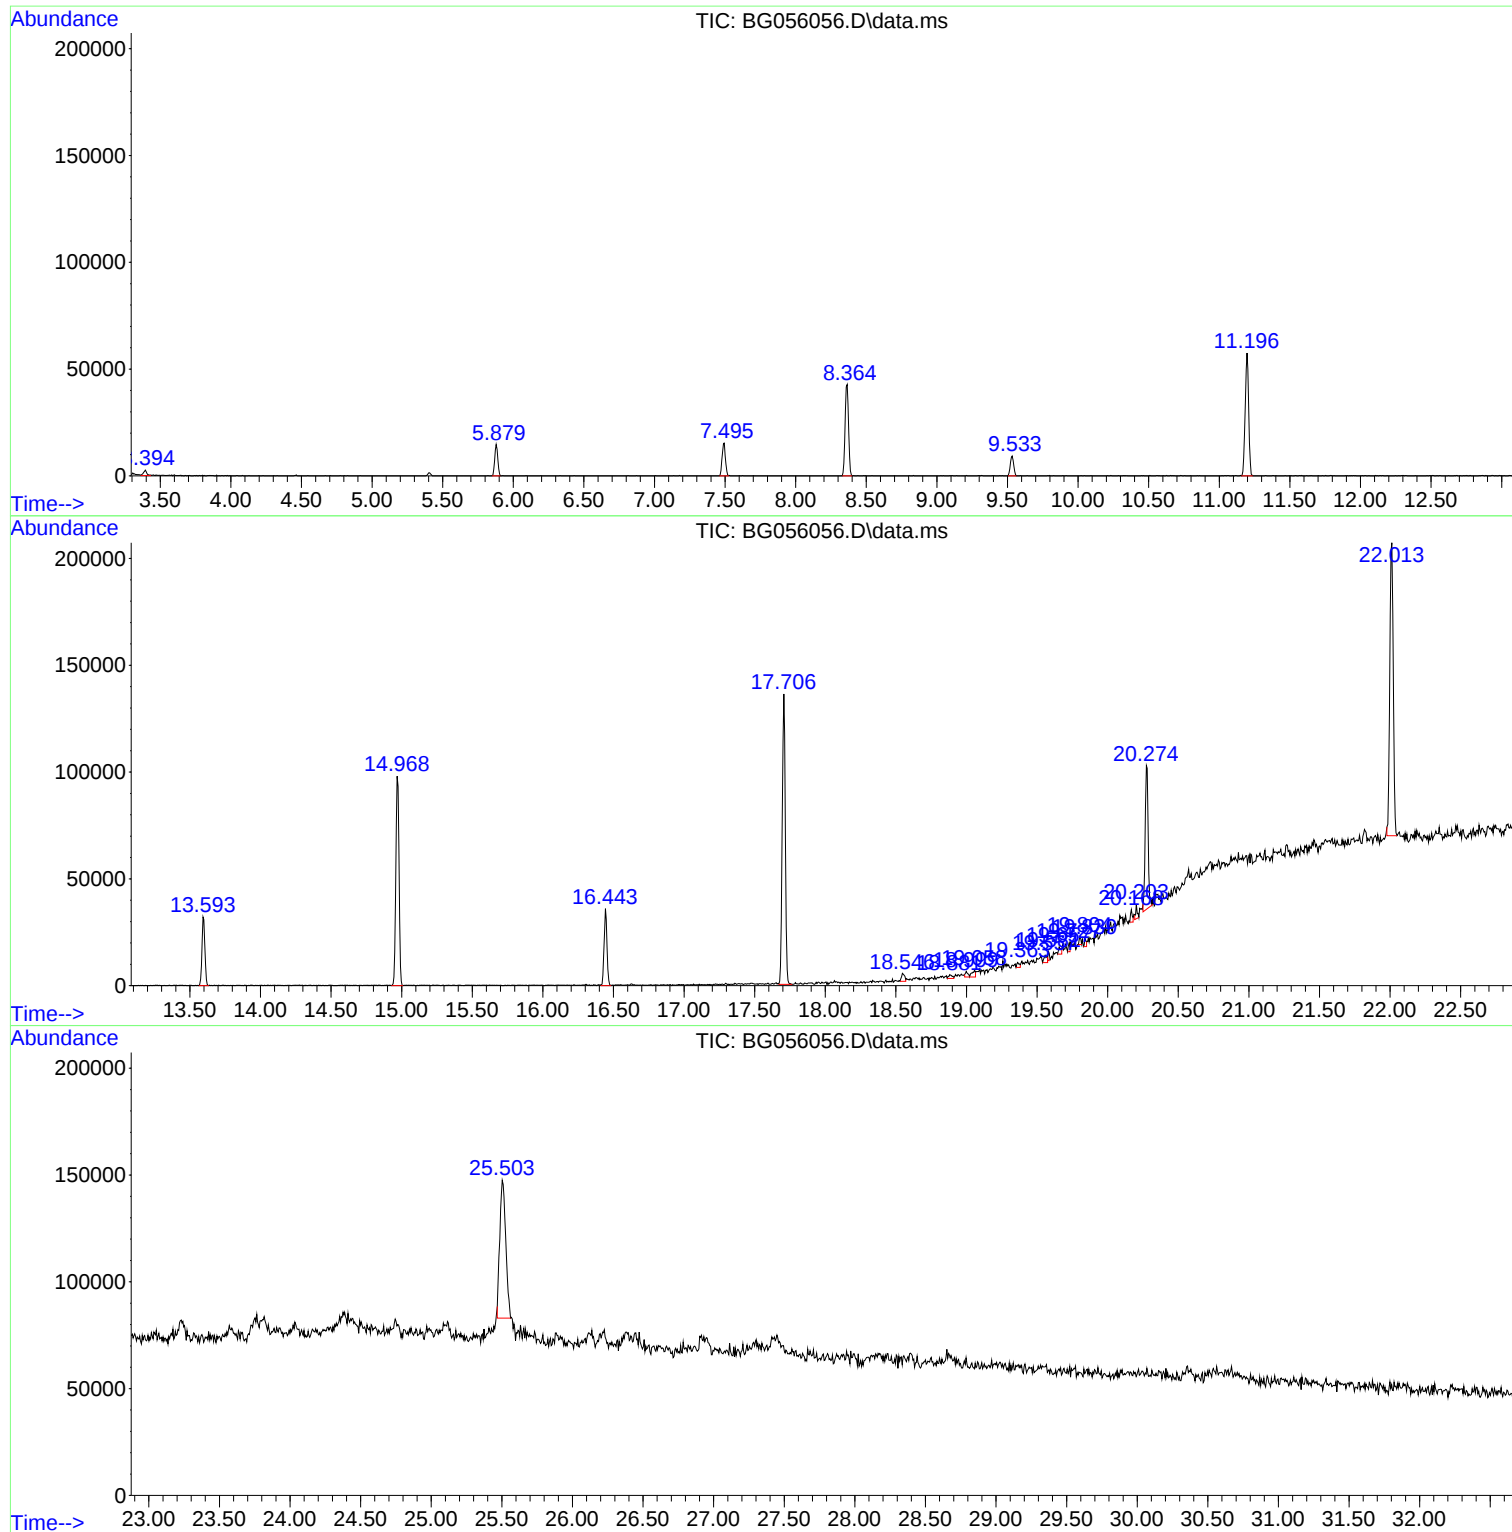

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122122\
Data File : BG056056.D
Acq On : 21 Dec 2022 20:08
Operator : CG/JU
Sample : N6071-05 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FVSUB-TP7-COMP-07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122122\
Data File : BG056056.D
Acq On : 21 Dec 2022 20:08
Operator : CG/JU
Sample : N6071-05 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FVSub-TP7-COMP-07

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------