

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122122\
 Data File : BG056057.D
 Acq On : 21 Dec 2022 20:49
 Operator : CG/JU
 Sample : N6071-01 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FVSUB-TP4-COMP-04

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG056057.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.878	436	441	447	rBB2	11758	17830	7.43%	1.707%
2	7.494	710	716	721	rBB3	13279	21521	8.97%	2.060%
3	8.364	858	864	870	rBB	47226	78908	32.89%	7.553%
4	9.533	1057	1063	1069	rBB2	8181	13565	5.65%	1.298%
5	11.196	1339	1346	1353	rBB	59693	106834	44.53%	10.226%
6	13.599	1749	1755	1761	rBB	28829	40686	16.96%	3.894%
7	14.968	1980	1988	1997	rBB	102574	161914	67.49%	15.498%
8	16.448	2234	2240	2246	rBB	27145	39136	16.31%	3.746%
9	17.706	2447	2454	2462	rBV	139665	207806	86.62%	19.891%
10	19.633	2780	2782	2784	rBV3	3362	3235	1.35%	0.310%
11	19.668	2784	2788	2791	rVV6	4756	7326	3.05%	0.701%
12	19.697	2791	2793	2794	rVV2	3331	2731	1.14%	0.261%
13	19.739	2798	2800	2803	rBV4	3439	3961	1.65%	0.379%
14	19.850	2817	2819	2823	rBV5	2931	3648	1.52%	0.349%
15	19.979	2839	2841	2843	rBV3	4945	3023	1.26%	0.289%
16	20.167	2871	2873	2876	rBV4	5485	3140	1.31%	0.301%
17	20.238	2884	2885	2887	rBV2	5137	4890	2.04%	0.468%
18	20.279	2887	2892	2897	rVV	59284	84671	35.29%	8.104%
19	22.012	3182	3187	3193	rVB	142470	239918	100.00%	22.964%




Sum of corrected areas: 1044743

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122122\
Data File : BG056057.D
Acq On : 21 Dec 2022 20:49
Operator : CG/JU
Sample : N6071-01 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FVSUB-TP4-COMP-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

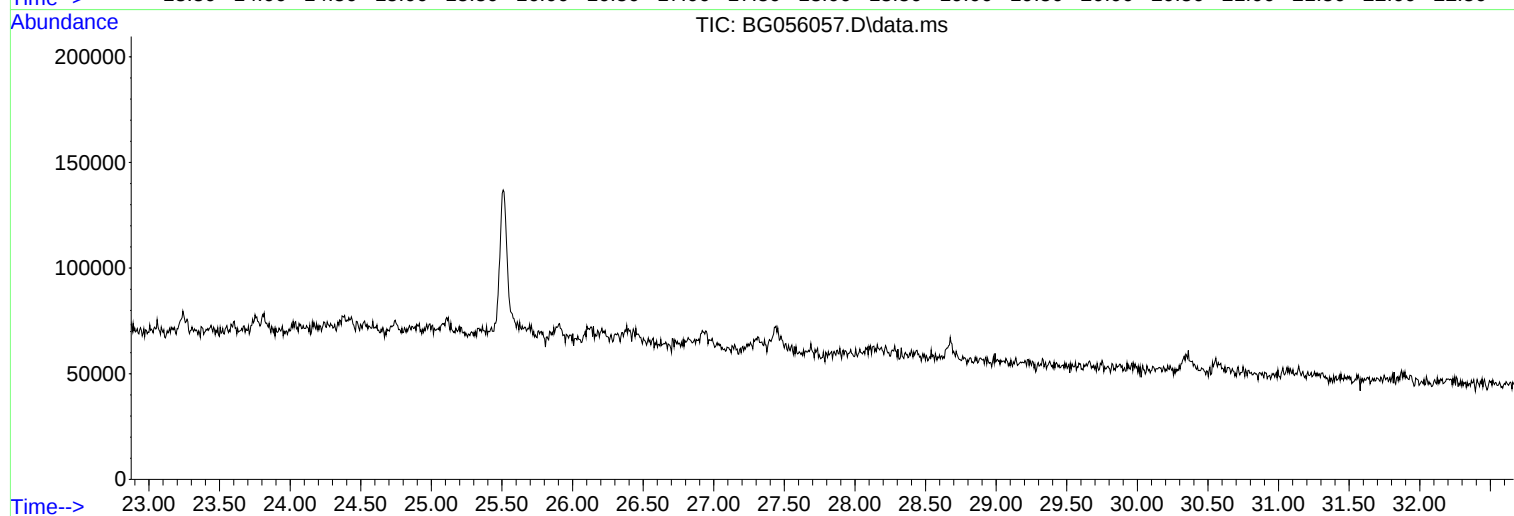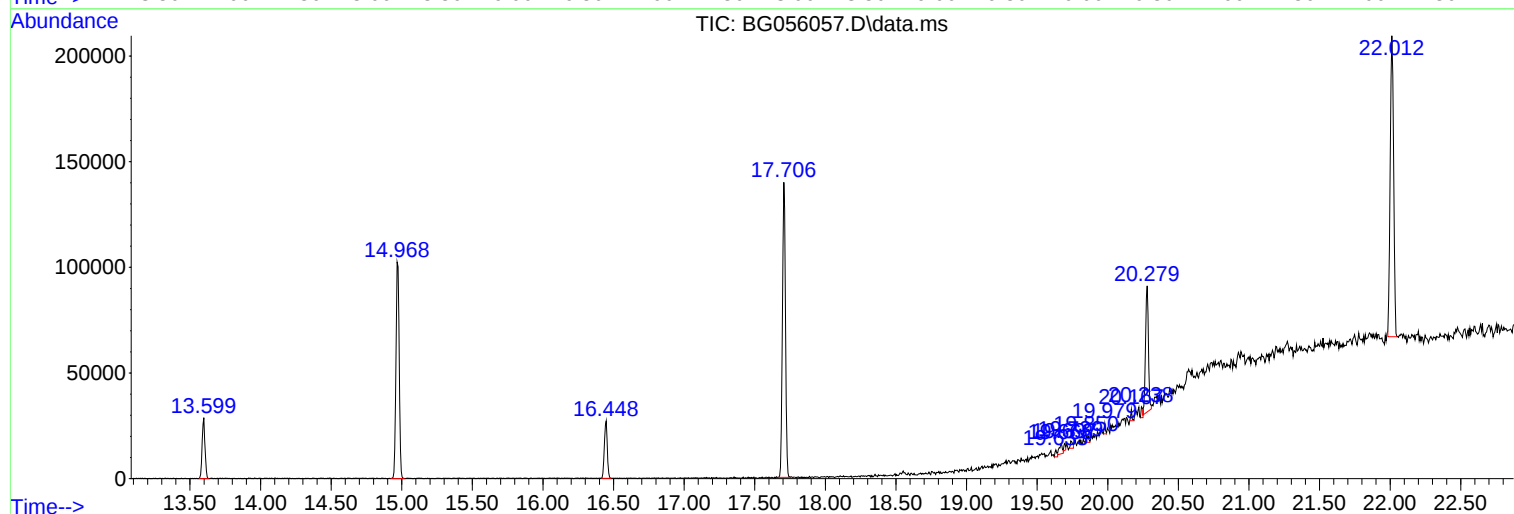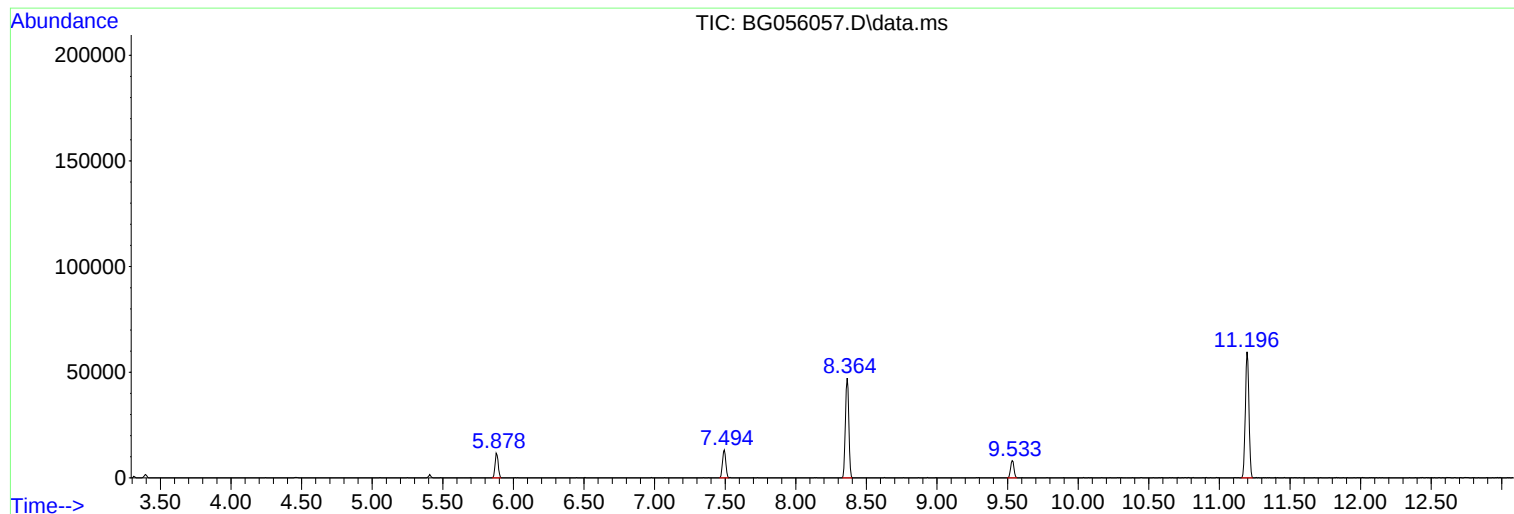

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122122\
Data File : BG056057.D
Acq On : 21 Dec 2022 20:49
Operator : CG/JU
Sample : N6071-01 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FVSUB-TP4-COMP-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122122\
Data File : BG056057.D
Acq On : 21 Dec 2022 20:49
Operator : CG/JU
Sample : N6071-01 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FVSub-TP4-COMP-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------