
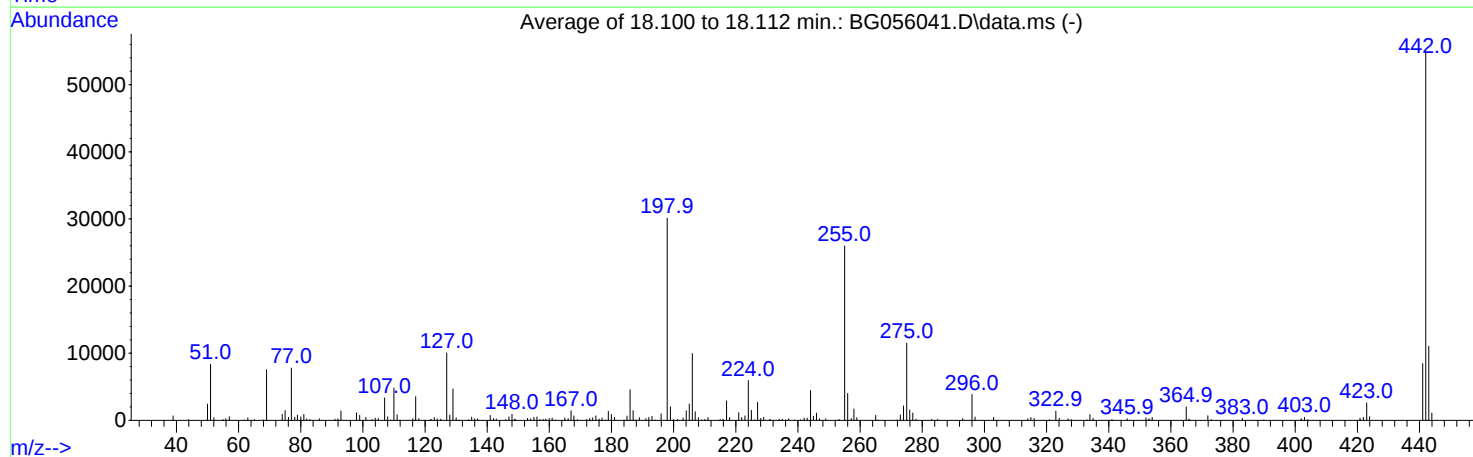


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122122\
 Data File : BG056041.D
 Acq On : 21 Dec 2022 9:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 23 05:09:54 2022

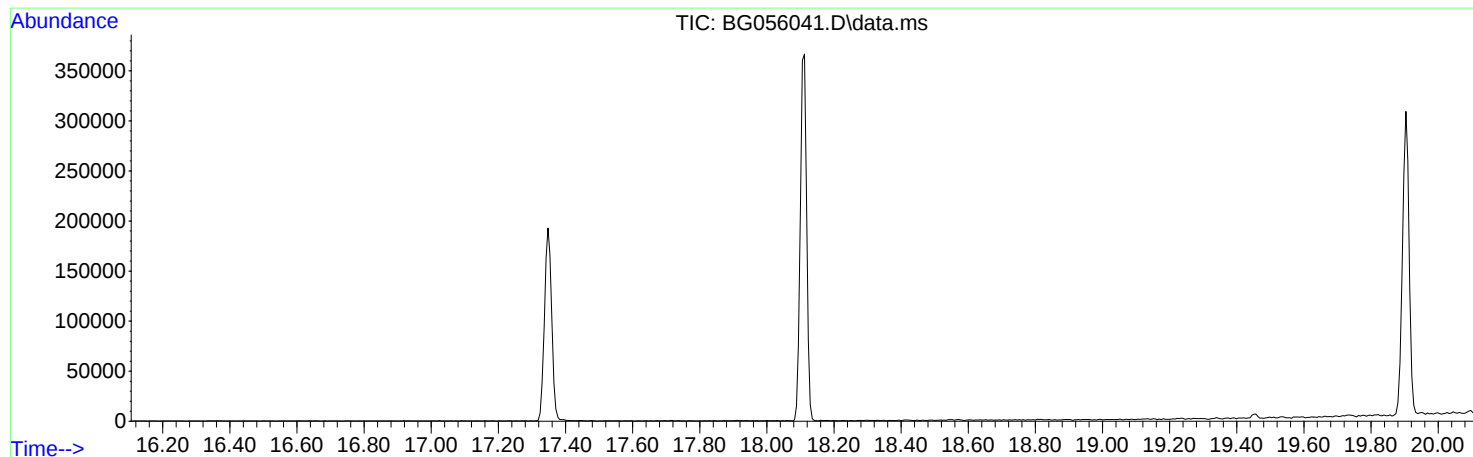




AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.8	8370	PASS
68	69	0.00	2	1.0	72	PASS
69	198	0.00	100	25.0	7544	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.3	10034	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	30139	PASS
199	198	5	9	6.7	2030	PASS
275	198	10	60	38.2	11506	PASS
365	198	1	100	6.6	1994	PASS
441	198	0.01	100	28.1	8464	PASS
442	442	50	100	100.0	54797	PASS
443	442	15	24	20.1	11026	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122122\
Data File : BG056041.D
Acq On : 21 Dec 2022 9:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 22 04:13:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 01:11:10 2022
Response via : Initial Calibration

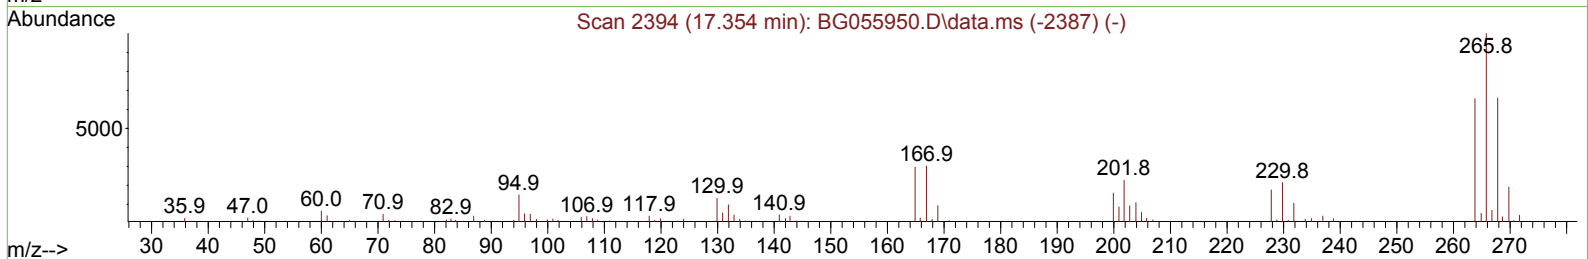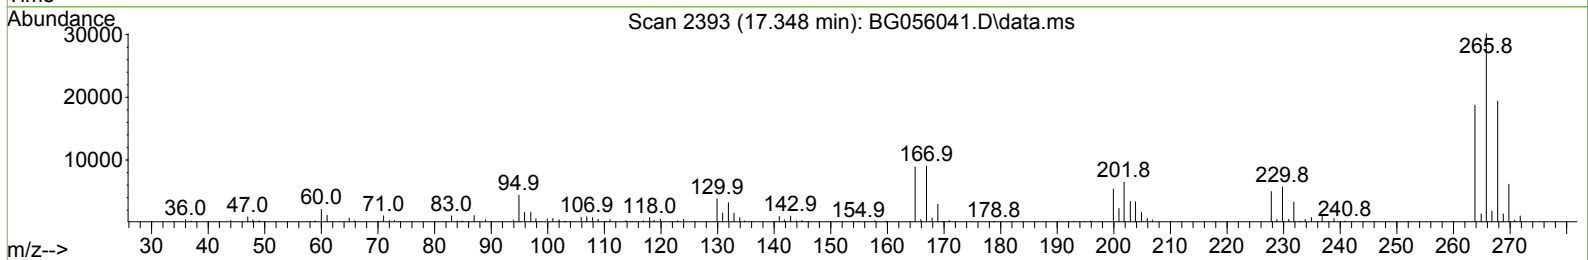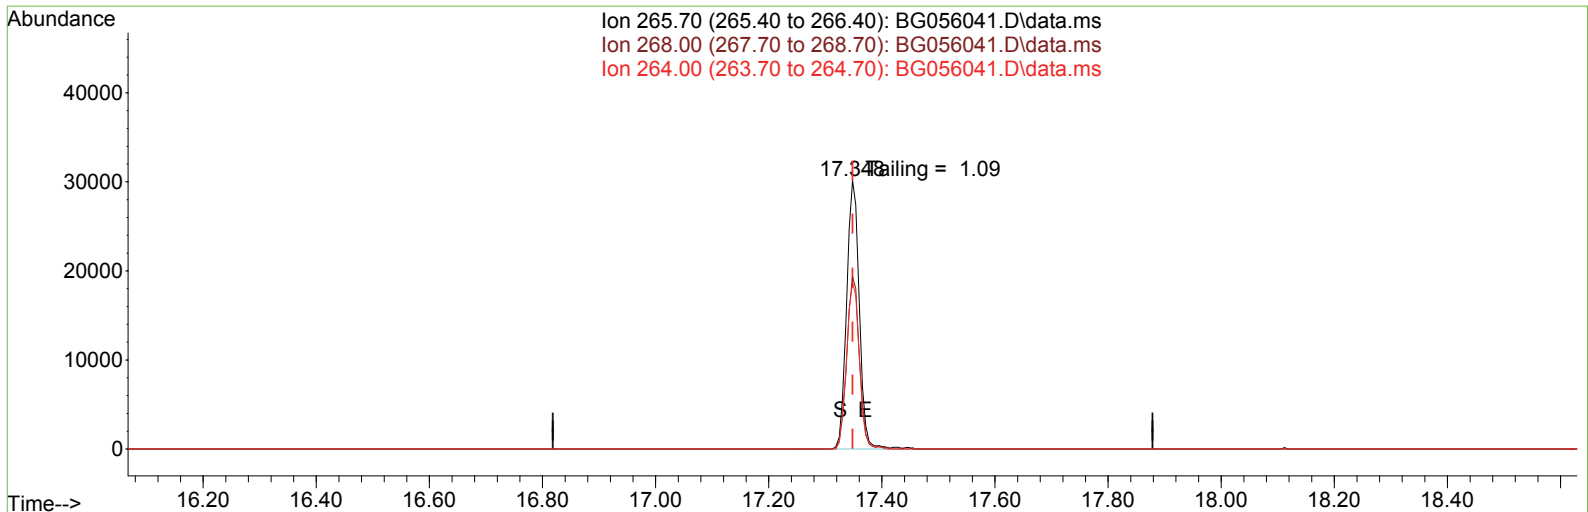

TIC: BG056041.D\data.ms

(70) Pentachlorophenol (C)

17.348min (-0.000) 73079.46 ng




response 46752

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.40	64.24
264.00	65.70	62.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122122\
Data File : BG056041.D
Acq On : 21 Dec 2022 9:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 22 04:13:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 21 01:11:10 2022
Response via : Initial Calibration

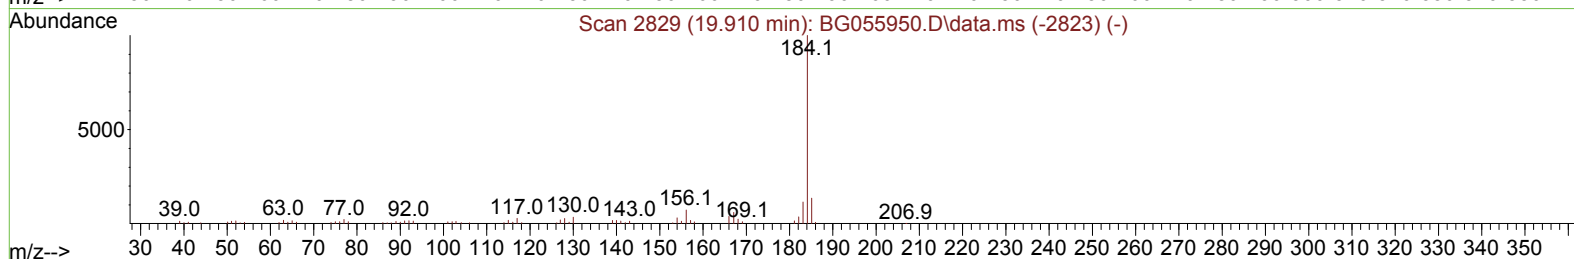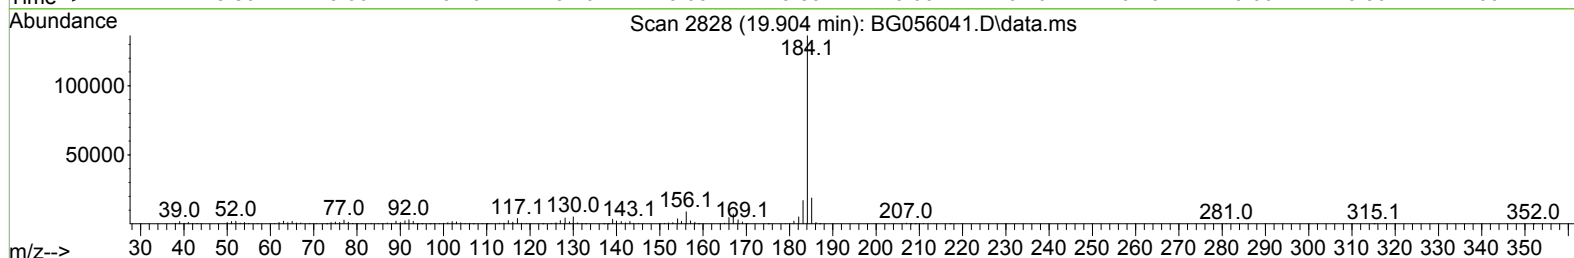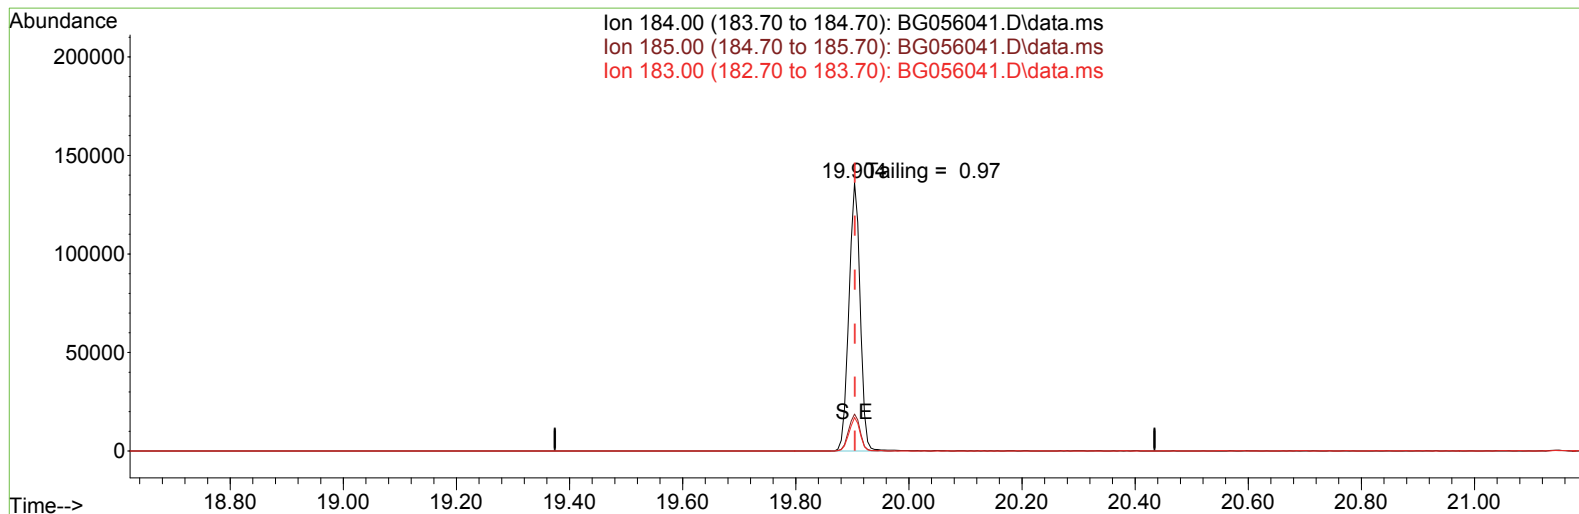

TIC: BG056041.D\data.ms

(77) Benzidine

19.904min (-0.000) 188989.92 ng

response 189182

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.82
183.00	11.50	12.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/21/2022	BNA_G	BG056041.D
Compound Name	Response	Retention Time
DDT	103536	21.143
DDD	4333	20.685
DDE	0	20.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4333	107869	4.02

Instrument :
BNA_G
ClientSampleId :
DFTPP