
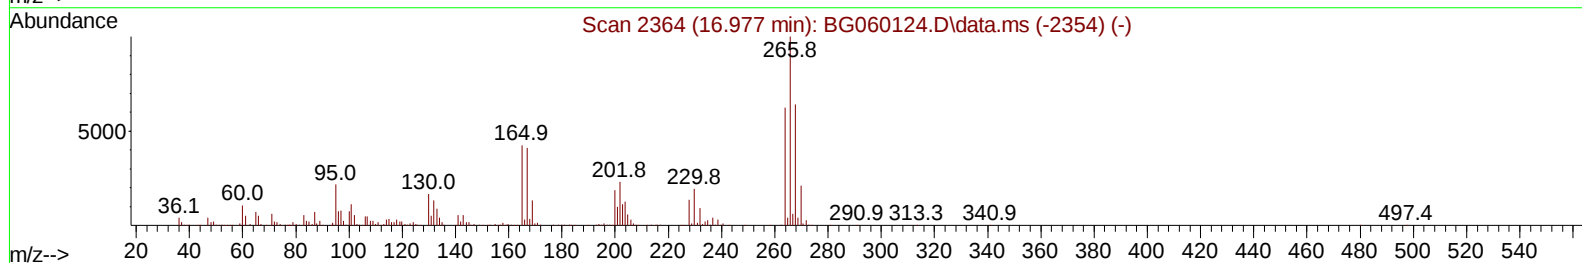
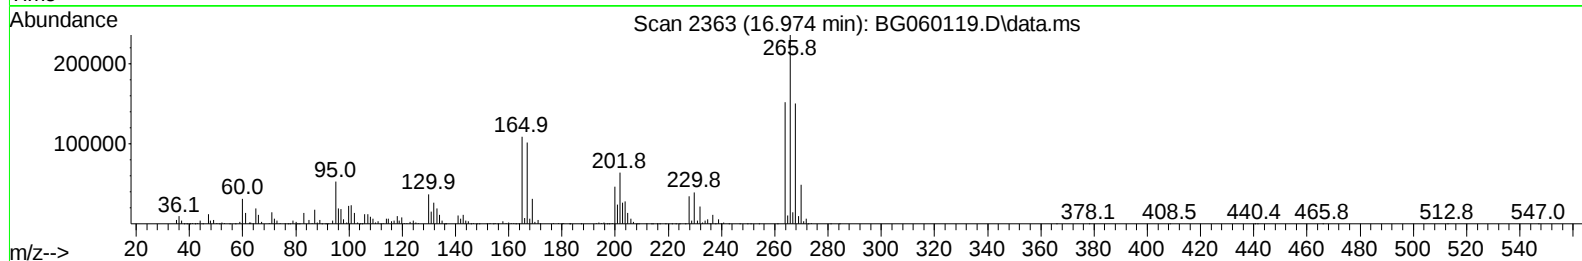


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122123\
Data File : BG060119.D
Acq On : 21 Dec 2023 12:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 03:46:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 03:42:04 2023
Response via : Initial Calibration

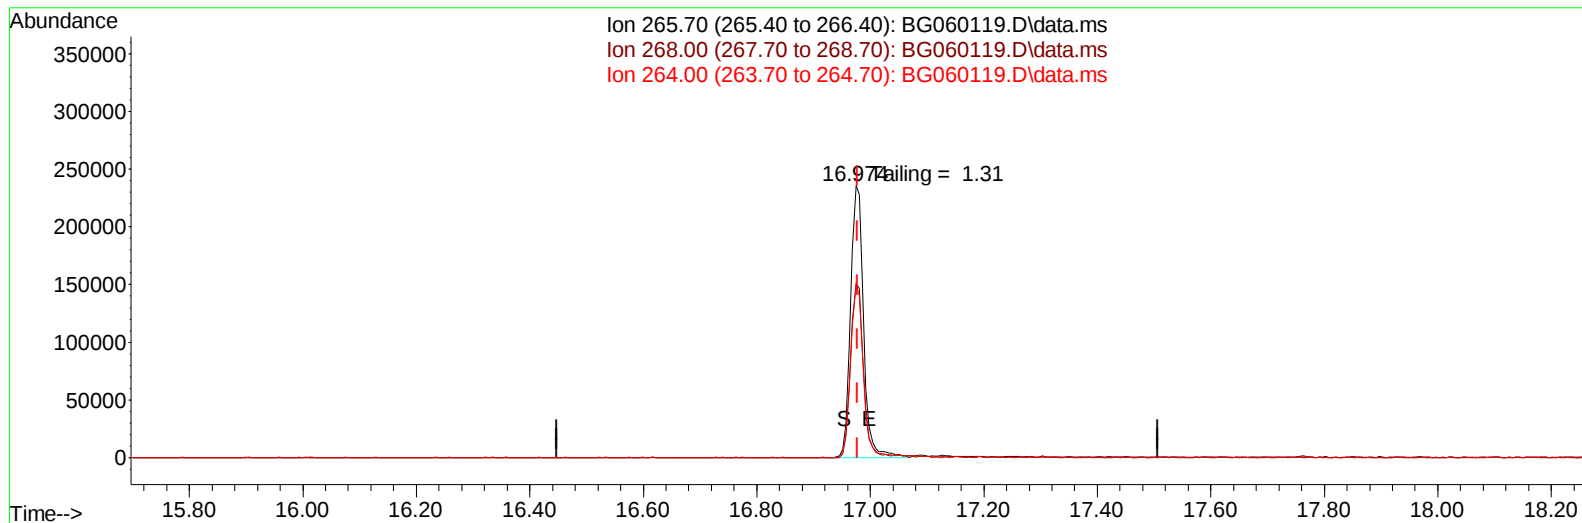

TIC: BG060119.D\data.ms

(70) Pentachlorophenol (C)




16.974min (-0.003) 835866.85 ng

response 374020

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.80	63.71
264.00	62.50	64.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122123\
Data File : BG060119.D
Acq On : 21 Dec 2023 12:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 03:46:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 03:42:04 2023
Response via : Initial Calibration

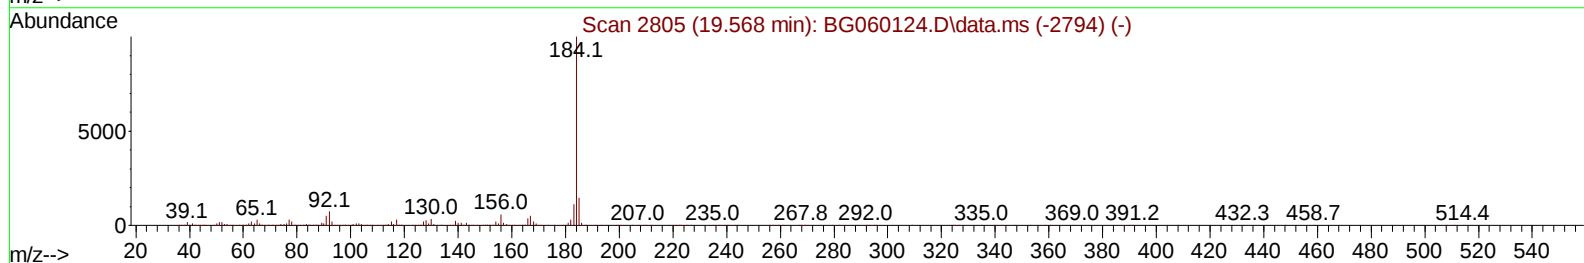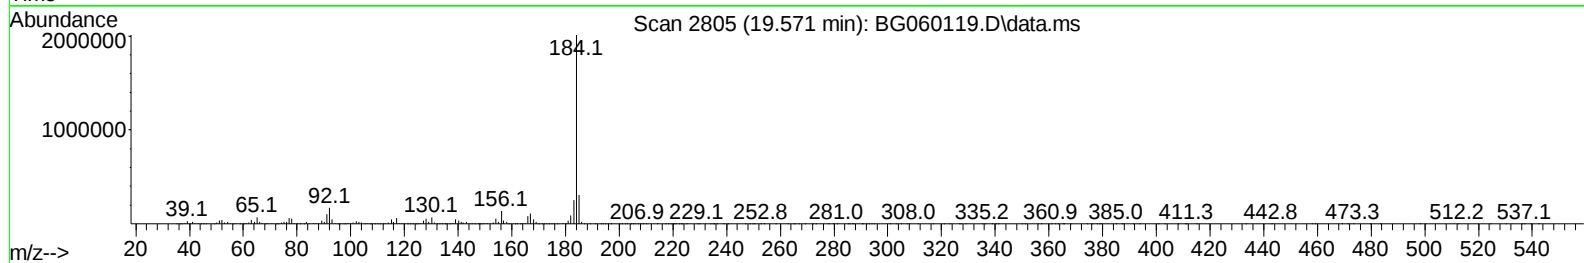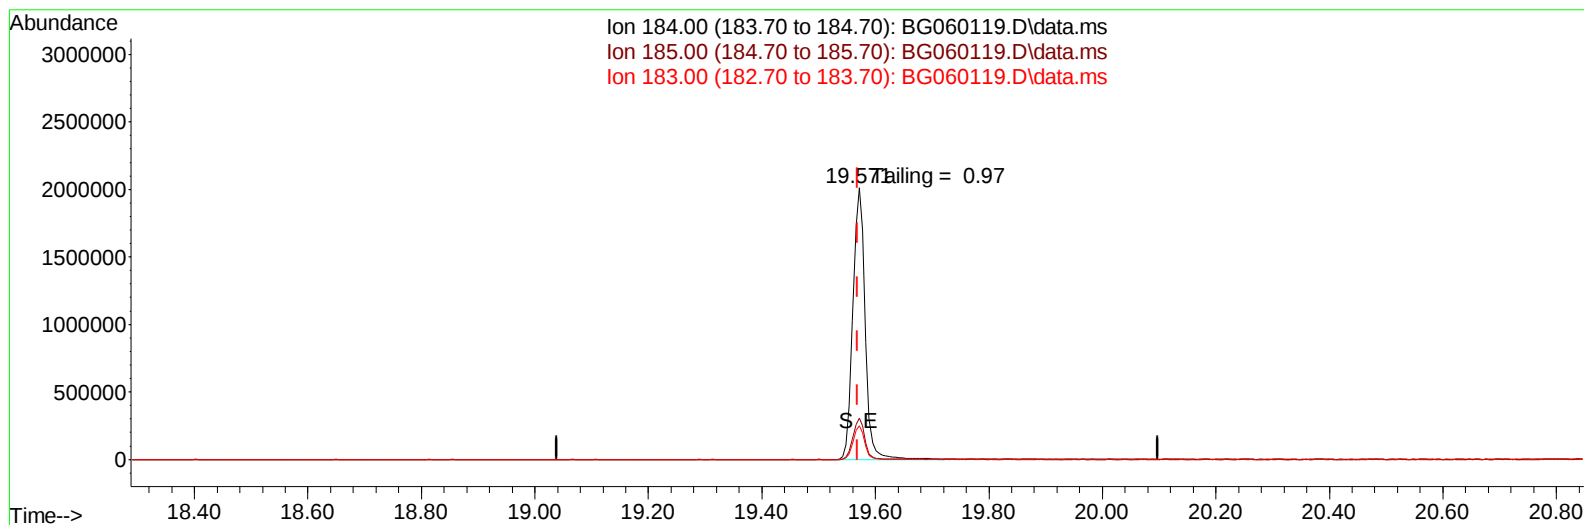

TIC: BG060119.D\data.ms

(77) Benzidine**19.571min (+ 0.003) 143927.83 ng****response 3039218**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	15.34
183.00	11.30	12.40
0.00	0.00	0.00