


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122123\
Data File : BG060119.D
Acq On : 21 Dec 2023 12:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 22 03:42:04 2023

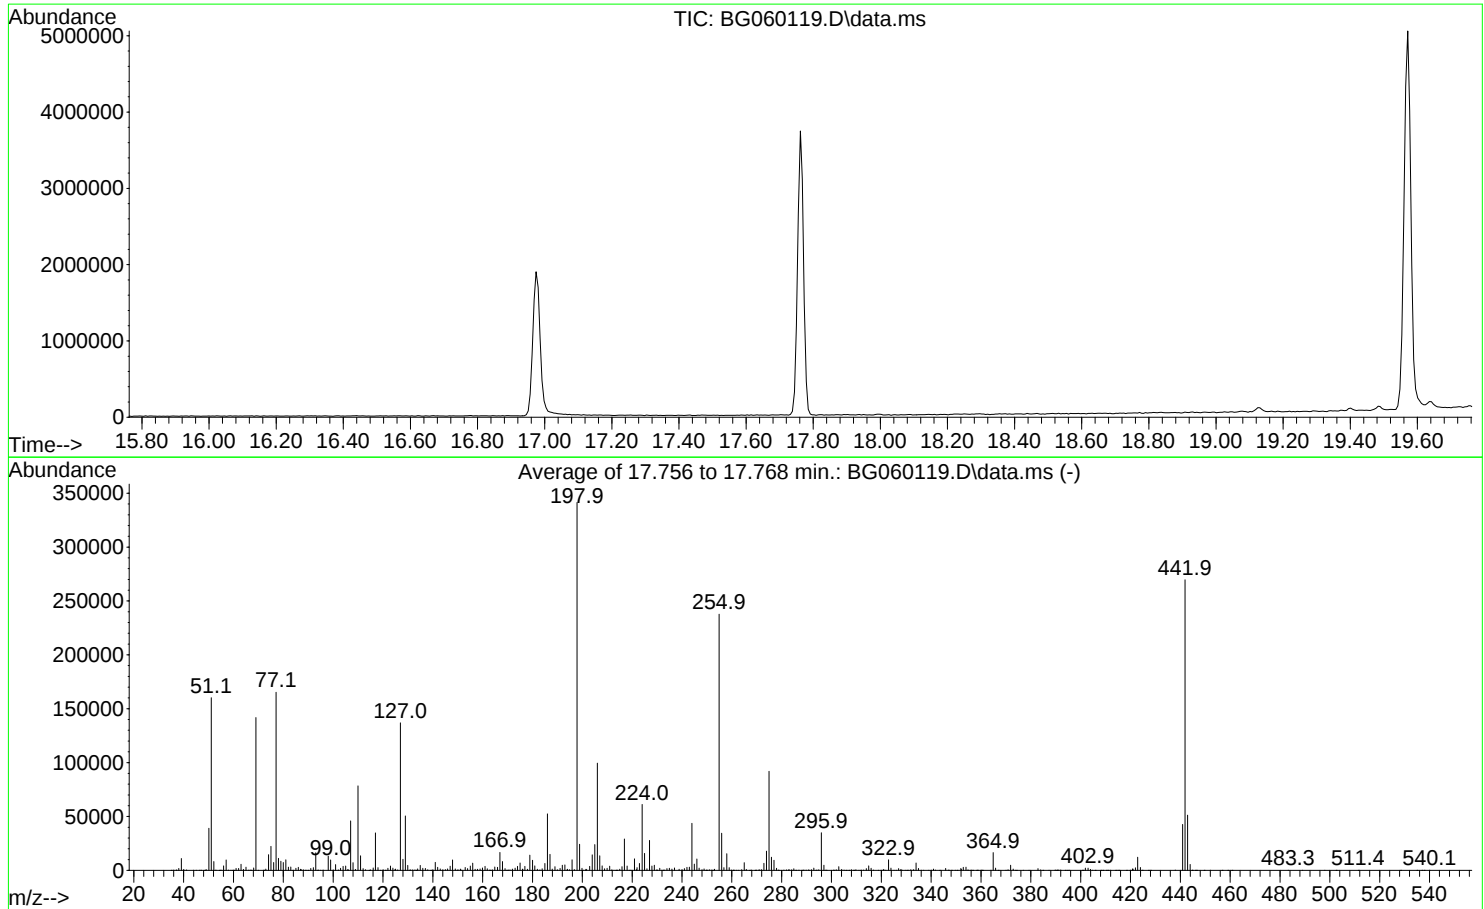




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	46.9	160149	PASS
68	69	0.00	2	1.5	2173	PASS
69	198	0.00	100	41.6	141879	PASS
70	69	0.00	2	0.1	94	PASS
127	198	10	80	40.1	136936	PASS
197	198	0.00	2	0.2	764	PASS
198	198	100	100	100.0	341376	PASS
199	198	5	9	7.1	24240	PASS
275	198	10	60	26.9	91845	PASS
365	198	1	100	4.8	16484	PASS
441	198	0.01	100	12.5	42571	PASS
442	442	50	100	100.0	269683	PASS
443	442	15	24	19.0	51237	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122123\
Data File : BG060119.D
Acq On : 21 Dec 2023 12:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 22 03:46:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 03:42:04 2023
Response via : Initial Calibration

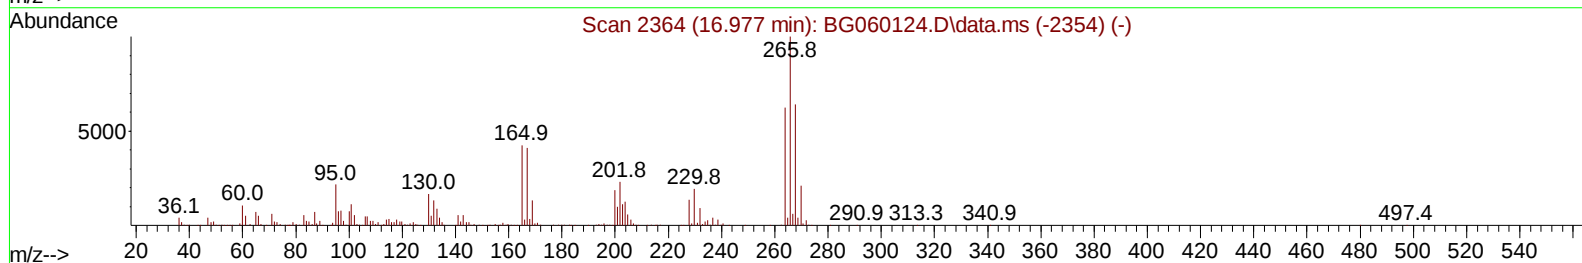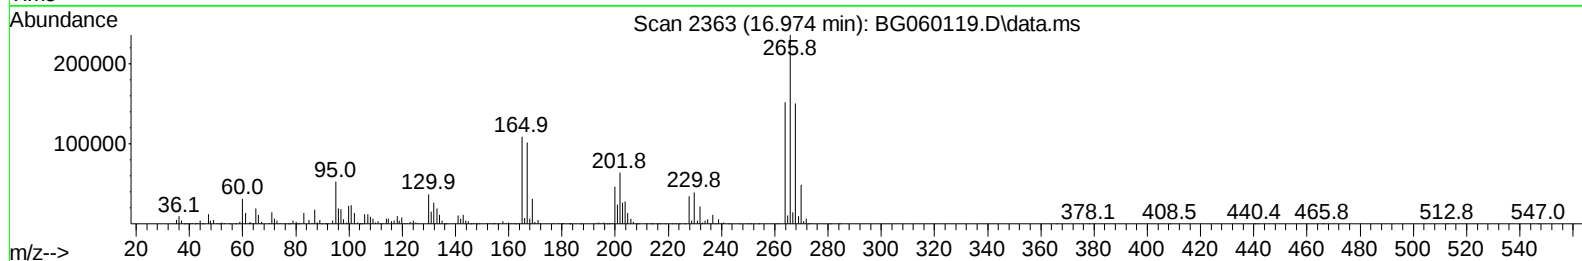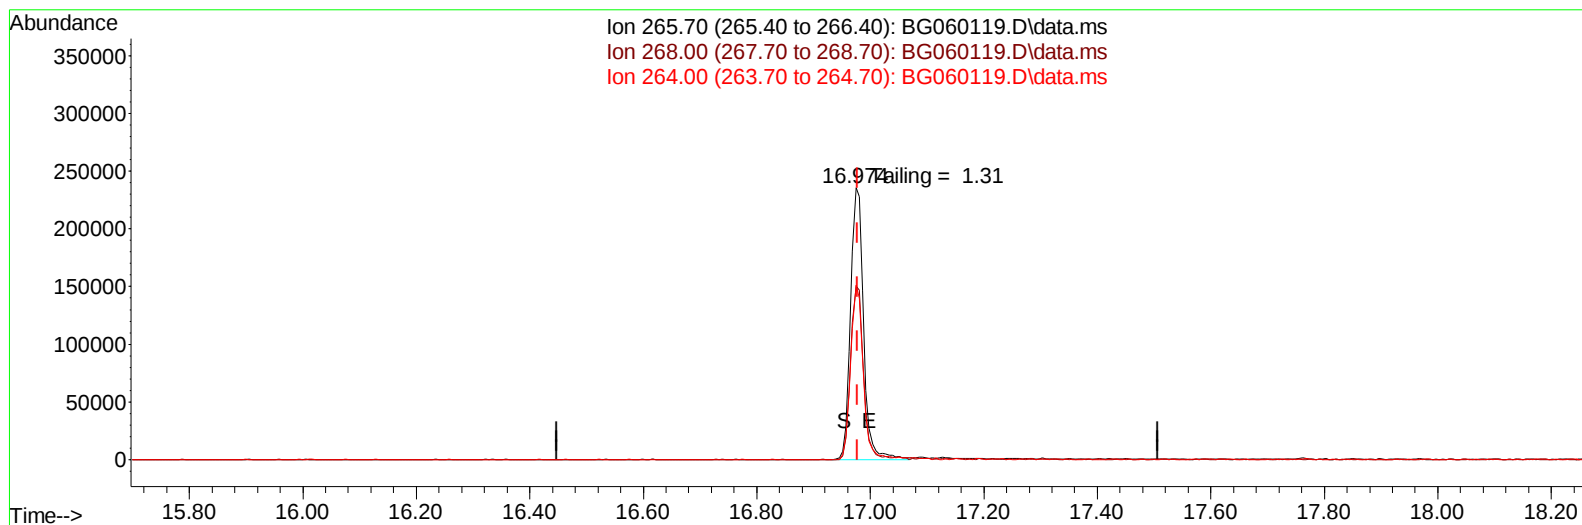

TIC: BG060119.D\data.ms

(70) Pentachlorophenol (C)

16.974min (-0.003) 835866.85 ng




response 374020

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.80	63.71
264.00	62.50	64.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122123\
Data File : BG060119.D
Acq On : 21 Dec 2023 12:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 22 03:46:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 03:42:04 2023
Response via : Initial Calibration

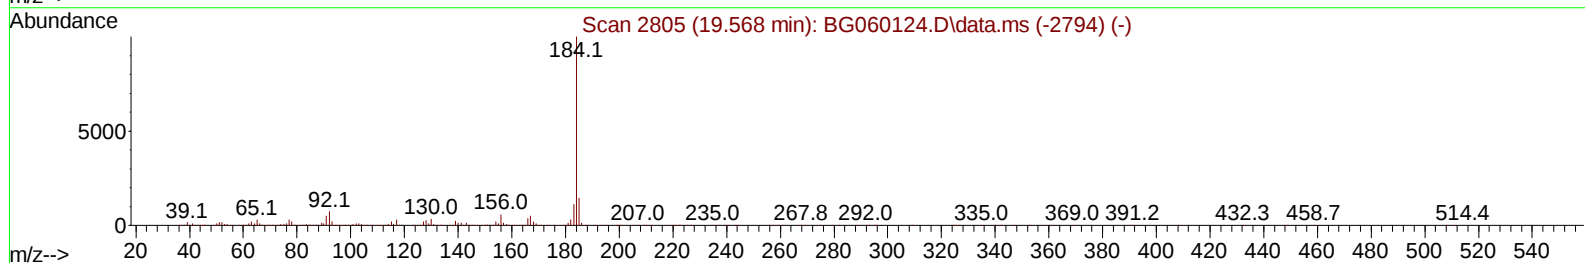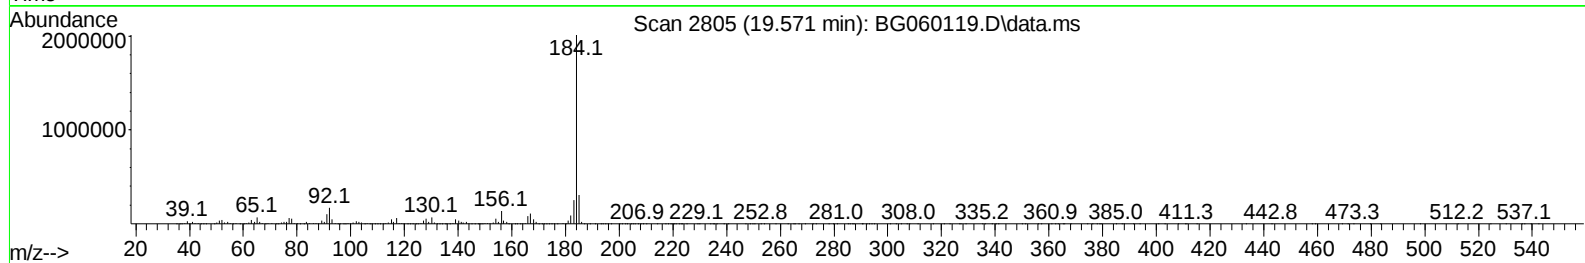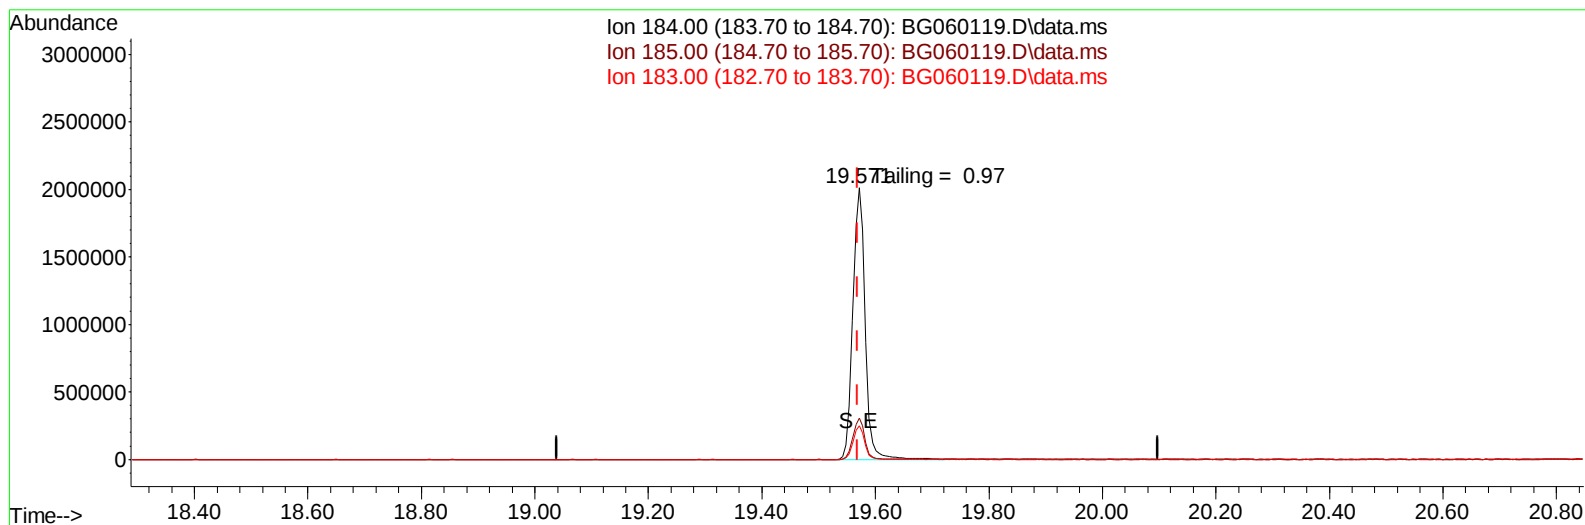

TIC: BG060119.D\data.ms

(77) Benzidine

19.571min (+ 0.003) 143927.83 ng

response 3039218

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	15.34
183.00	11.30	12.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/21/2023	BNA_G	<u>BG060119.D</u>
Compound Name	Response	Retention Time
DDT	1100891	20.799
DDD	15369	20.412
DDE	954	19.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16323	1117214	1.46

Instrument :
BNA_G
ClientSampleId :
DFTPP