

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122215\
 Data File : BG020410.D
 Acq On : 22 Dec 2015 15:37
 Operator : UM/SJ
 Sample : PB87484BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK84

Quant Time: Dec 23 04:13:43 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 23 04:11:09 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	15418	20.00	ng/ul	0.00
18) Naphthalene-d8	10.90	136	70866	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.71	164	60212	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.46	188	159520	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	170393	20.00	ng/ul	0.00
86) Perylene-d12	25.00	264	163825	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.45	96	1806	6.47	ng/uL	0.00
5) Phenol-d5	7.24	99	45132	33.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.41	67	29168	35.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.61	132	37237	37.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.79	113	41468	35.67	ng/ul	0.00
19) Nitrobenzene-d5	9.25	128	21150	38.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.98	143	26371	42.90	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	45543	36.58	ng/ul	0.00
29) 4-Chloroaniline-d4	11.04	131	64365	46.02	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	200113	41.09	ng/ul	0.00
47) Acenaphthylene-d8	14.41	160	208519	36.80	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	25750	29.48	ng/ul	0.00
58) Fluorene-d10	15.71	176	169187	38.30	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	13761	14.55	ng/ul	-0.01
71) Anthracene-d10	17.56	188	284904	38.76	ng/ul	0.00
79) Pyrene-d10	19.84	212	292288	36.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.78	264	318467	38.97	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.79	70	975	1.01 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122215\
Data File : BG020410.D
Acq On : 22 Dec 2015 15:37
Operator : UM/SJ
Sample : PB87484BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK84

Quant Time: Dec 23 04:13:43 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 23 04:11:09 2015
Response via : Initial Calibration

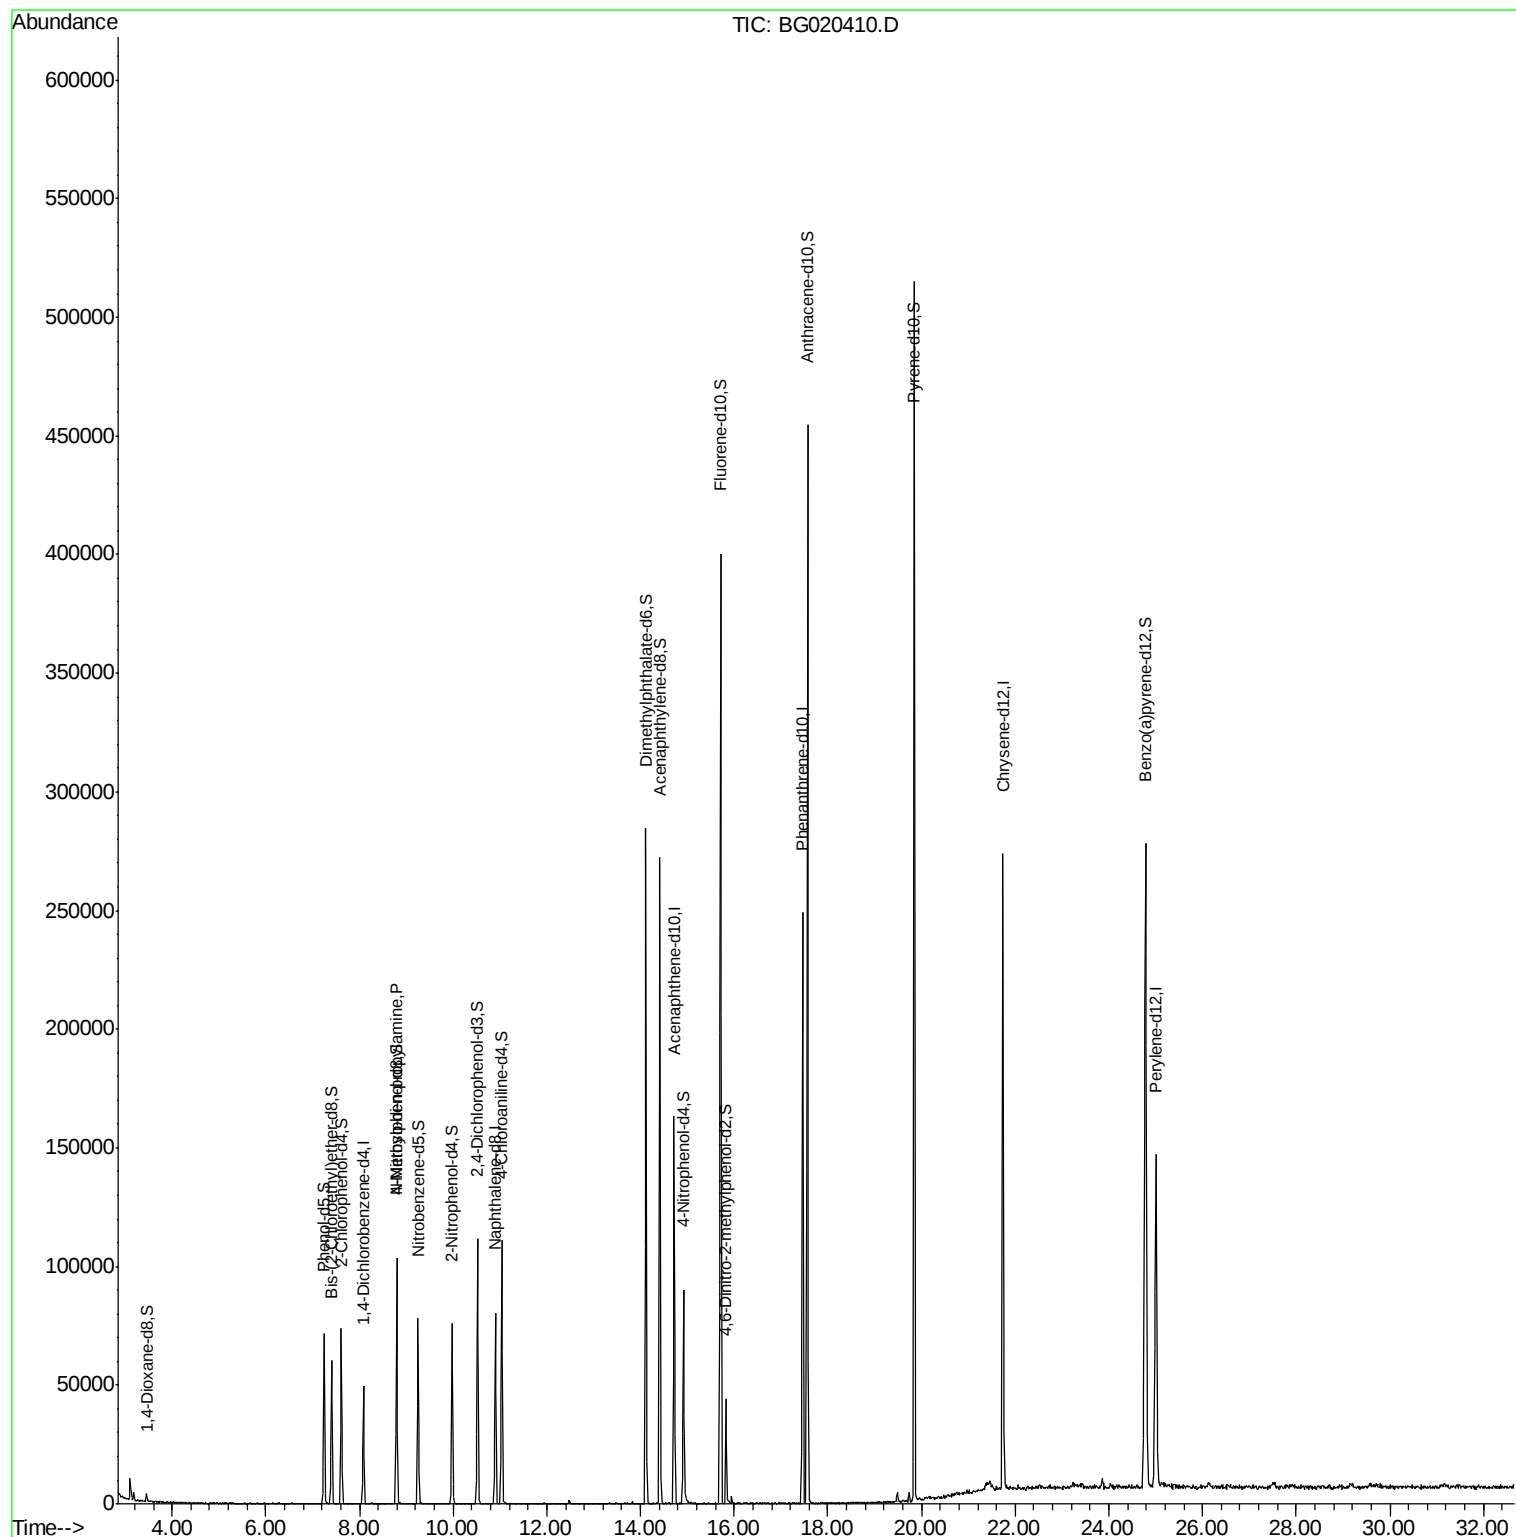

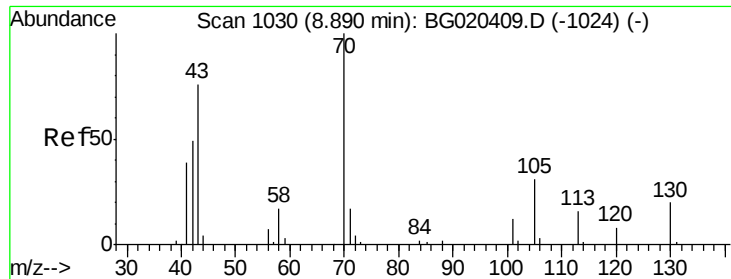

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.01 ng/ul
 RT: 8.79 min Scan# 1013
 Delta R.T. -0.10 min
 Lab File: BG020410.D
 Acq: 22 Dec 2015 15:37

Instrument :
 BNA_G
 ClientSampleId :
 SBLK84

Tgt Ion:	70	Resp:	975
Ion	Ratio	Lower	Upper
70	100		
42	335.6	44.3	66.5#
101	0.0	7.6	11.4#
130	0.0	17.0	25.4#

