

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122215\
 Data File : BG020422.D
 Acq On : 23 Dec 2015 00:53
 Operator : UM/SJ
 Sample : PB87451BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK51

Quant Time: Dec 23 07:41:08 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 23 07:35:51 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	15746	20.00	ng/ul	0.00
18) Naphthalene-d8	10.90	136	68219	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.72	164	51035	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.46	188	133719	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	163838	20.00	ng/ul	0.00
86) Perylene-d12	25.00	264	155982	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.45	96	2107	7.39	ng/uL	0.00
5) Phenol-d5	7.24	99	47507	34.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.40	67	31036	37.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.61	132	39019	38.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.79	113	43092	36.29	ng/ul	0.00
19) Nitrobenzene-d5	9.25	128	21593	40.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.98	143	25688	43.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	45741	38.16	ng/ul	0.00
29) 4-Chloroaniline-d4	11.03	131	62203	46.20	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	177871	43.09	ng/ul	0.00
47) Acenaphthylene-d8	14.41	160	196351	40.88	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	24927	33.67	ng/ul	0.00
58) Fluorene-d10	15.70	176	154229	41.19	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	20985	26.47	ng/ul	0.00
71) Anthracene-d10	17.56	188	255131	41.41	ng/ul	0.00
79) Pyrene-d10	19.84	212	299691	39.25	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.78	264	329712	42.38	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.79	70	1101	1.12	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122215\
Data File : BG020422.D
Acq On : 23 Dec 2015 00:53
Operator : UM/SJ
Sample : PB87451BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK51

Quant Time: Dec 23 07:41:08 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 23 07:35:51 2015
Response via : Initial Calibration

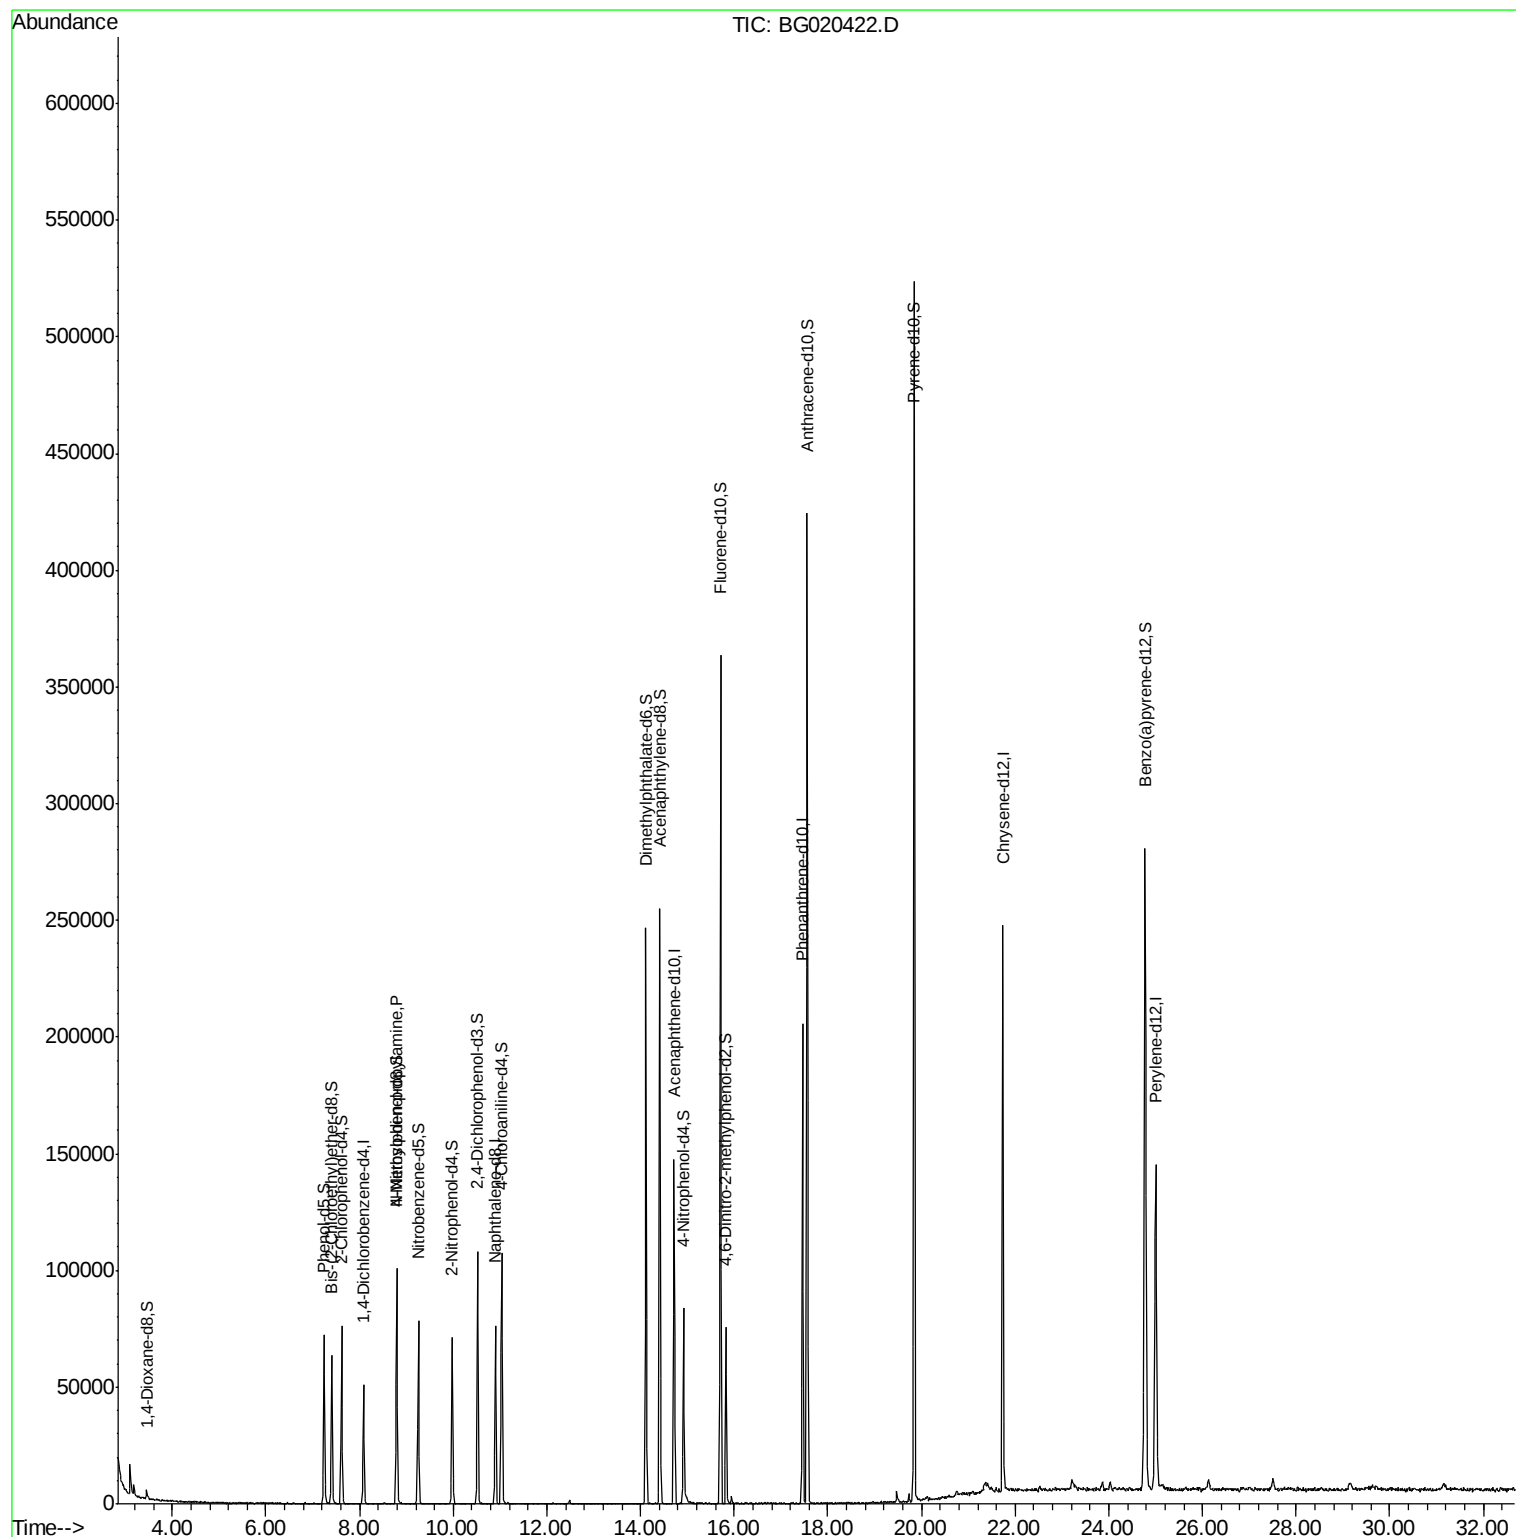

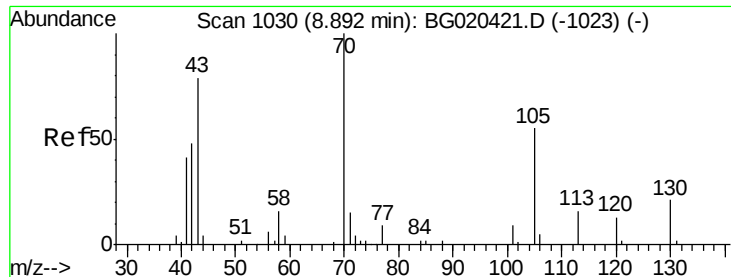

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.12 ng/ul
 RT: 8.79 min Scan# 1013
 Delta R.T. -0.10 min
 Lab File: BG020422.D
 Acq: 23 Dec 2015 00:53

Instrument :
 BNA_G
 ClientSampleId :
 SBLK51

Tgt Ion: 70 Resp: 1101

Ion	Ratio	Lower	Upper
70	100		
42	319.0	44.3	66.5#
101	0.0	7.6	11.4#
130	0.0	17.0	25.4#

