

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122215\
 Data File : BG020422.D
 Acq On : 23 Dec 2015 00:53
 Operator : UM/SJ
 Sample : PB87451BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.102	41	45	55	rBV2	12508	23567	3.06%	0.356%
2	3.184	55	59	65	rVB4	4872	8201	1.06%	0.124%
3	3.454	102	105	110	rVB3	3765	4808	0.62%	0.073%
4	4.148	218	223	224	rVV3	520	811	0.11%	0.012%
5	7.244	743	750	760	rBV	72354	128704	16.70%	1.946%
6	7.403	770	777	787	rBV	63542	104757	13.59%	1.584%
7	7.614	807	813	824	rVB	76183	133152	17.27%	2.013%
8	8.084	886	893	902	rBB	50823	85997	11.16%	1.300%
9	8.789	1007	1013	1028	rBB	100940	179107	23.24%	2.708%
10	9.253	1085	1092	1104	rBV	78320	141980	18.42%	2.146%
11	9.976	1208	1215	1224	rBV	71413	128438	16.66%	1.942%
12	10.517	1300	1307	1317	rBB	108212	193602	25.12%	2.927%
13	10.899	1365	1372	1381	rBV	76520	136949	17.77%	2.070%
14	11.034	1388	1395	1408	rBV	107766	196531	25.50%	2.971%
15	12.479	1637	1641	1646	rBB2	1419	2337	0.30%	0.035%
16	14.118	1913	1920	1929	rBV	246644	362937	47.09%	5.487%
17	14.412	1962	1970	1979	rBV	255022	400862	52.01%	6.060%
18	14.718	2014	2022	2030	rBB2	147677	227983	29.58%	3.446%
19	14.917	2050	2056	2077	rBV	83957	144236	18.71%	2.180%
20	15.705	2184	2190	2199	rBV	363258	544221	70.61%	8.227%
21	15.822	2204	2210	2221	rBV	75277	110136	14.29%	1.665%
22	15.946	2227	2231	2236	rVB3	3497	4758	0.62%	0.072%
23	17.250	2450	2453	2458	rBB2	722	1158	0.15%	0.018%
24	17.461	2482	2489	2499	rBV	205640	306245	39.73%	4.630%
25	17.561	2499	2506	2515	rBV	423906	620282	80.47%	9.377%
26	19.477	2826	2832	2837	rBV	4757	7793	1.01%	0.118%
27	19.729	2872	2875	2878	rBV	3263	4280	0.56%	0.065%
28	19.841	2888	2894	2901	rVV	522256	753129	97.71%	11.385%
29	19.994	2917	2920	2922	rBV2	814	1163	0.15%	0.018%
30	20.088	2934	2936	2938	rVV	863	879	0.11%	0.013%
31	20.105	2938	2939	2941	rVV2	1053	974	0.13%	0.015%
32	20.129	2941	2943	2944	rVV2	1495	1127	0.15%	0.017%
33	20.164	2948	2949	2952	rBV2	1415	1260	0.16%	0.019%
34	20.205	2952	2956	2957	rBV2	778	943	0.12%	0.014%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122215\
 Data File : BG020422.D
 Acq On : 23 Dec 2015 00:53
 Operator : UM/SJ
 Sample : PB87451BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
 Title : SVOA CALIBRATION

35	20.282	2967	2969	2972	rBV3	621	774	0.10%	0.012%
36	20.352	2978	2981	2983	rBV3	876	1006	0.13%	0.015%
37	20.429	2992	2994	2995	rBV	956	867	0.11%	0.013%
38	20.669	3033	3035	3038	rBV3	770	901	0.12%	0.014%
39	20.740	3045	3047	3050	rBV3	1353	1018	0.13%	0.015%
40	20.916	3075	3077	3080	rBV3	1117	836	0.11%	0.013%
41	21.028	3094	3096	3097	rVB2	1270	774	0.10%	0.012%
42	21.040	3097	3098	3100	rBV2	1613	1177	0.15%	0.018%
43	21.116	3110	3111	3113	rVB2	1311	847	0.11%	0.013%
44	21.239	3130	3132	3134	rVB3	1292	905	0.12%	0.014%
45	21.333	3146	3148	3149	rBV2	1893	1307	0.17%	0.020%
46	21.580	3187	3190	3191	rBV3	1126	1342	0.17%	0.020%
47	21.733	3209	3216	3223	rBV	242377	399721	51.86%	6.043%
48	22.085	3273	3276	3279	rBV5	1068	1529	0.20%	0.023%
49	22.503	3345	3347	3348	rBV2	1798	1795	0.23%	0.027%
50	22.526	3349	3351	3356	rVB5	2534	2973	0.39%	0.045%
51	22.585	3359	3361	3362	rBV2	984	865	0.11%	0.013%
52	23.219	3465	3469	3473	rVV5	3913	6264	0.81%	0.095%
53	23.272	3477	3478	3481	rVV3	1305	941	0.12%	0.014%
54	23.449	3507	3508	3511	rBV2	1135	840	0.11%	0.013%
55	23.830	3571	3573	3575	rBV3	1607	1697	0.22%	0.026%
56	23.860	3575	3578	3584	rVB6	3914	7290	0.95%	0.110%
57	24.024	3604	3606	3615	rVB6	3704	7397	0.96%	0.112%
58	24.436	3674	3676	3677	rBV	1107	784	0.10%	0.012%
59	24.494	3684	3686	3690	rVB3	1248	1388	0.18%	0.021%
60	24.776	3723	3734	3745	rBV	274633	770779	100.00%	11.652%
61	25.000	3762	3772	3785	rVB3	137652	376891	48.90%	5.698%
62	25.211	3806	3808	3809	rBV2	1024	1045	0.14%	0.016%
63	25.270	3816	3818	3819	rBV2	1336	837	0.11%	0.013%
64	25.311	3824	3825	3827	rBV2	1663	1299	0.17%	0.020%
65	25.517	3856	3860	3862	rVB4	1067	1272	0.17%	0.019%
66	25.599	3872	3874	3877	rBV4	903	904	0.12%	0.014%
67	25.987	3938	3940	3942	rBV3	1243	1455	0.19%	0.022%
68	26.069	3952	3954	3955	rBV2	1232	940	0.12%	0.014%
69	26.134	3958	3965	3968	rVV4	3797	8295	1.08%	0.125%
70	26.674	4054	4057	4060	rBV4	1334	1723	0.22%	0.026%
71	26.850	4085	4087	4089	rBV3	1243	1013	0.13%	0.015%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122215\
Data File : BG020422.D
Acq On : 23 Dec 2015 00:53
Operator : UM/SJ
Sample : PB87451BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Title : SVOA CALIBRATION

72	27.191	4143	4145	4146	rBV	1202	917	0.12%	0.014%
73	27.438	4183	4187	4189	rBV5	1340	1658	0.22%	0.025%
74	27.491	4189	4196	4197	rBV6	3631	6183	0.80%	0.093%
75	27.949	4272	4274	4275	rBV2	1033	834	0.11%	0.013%
76	28.020	4285	4286	4288	rBV2	1261	812	0.11%	0.012%
77	28.143	4303	4307	4309	rBV4	1658	1433	0.19%	0.022%
78	28.225	4319	4321	4323	rBV3	1005	1122	0.15%	0.017%
79	28.496	4365	4367	4370	rBV4	1082	1275	0.17%	0.019%
80	29.154	4470	4479	4481	rBV8	3194	9157	1.19%	0.138%
81	29.594	4553	4554	4556	rBV	1824	1366	0.18%	0.021%
82	29.853	4596	4598	4599	rBV	1159	803	0.10%	0.012%
83	30.011	4623	4625	4628	rVB4	1169	1071	0.14%	0.016%
84	30.358	4681	4684	4686	rBV4	1666	2163	0.28%	0.033%
85	30.640	4730	4732	4733	rVB2	1741	1091	0.14%	0.016%
86	30.658	4733	4735	4737	rBV3	1400	1452	0.19%	0.022%
87	30.746	4748	4750	4753	rBV3	1803	1849	0.24%	0.028%
88	31.128	4813	4815	4816	rBV2	1525	1144	0.15%	0.017%
89	31.292	4841	4843	4846	rVB3	1194	955	0.12%	0.014%
90	31.780	4925	4926	4929	rBV3	1259	1464	0.19%	0.022%
91	31.950	4953	4955	4960	rVB2	1502	1394	0.18%	0.021%
92	32.356	5023	5024	5026	rBV	1323	924	0.12%	0.014%
93	32.485	5044	5046	5048	rVB3	1204	872	0.11%	0.013%


Sum of corrected areas: 6614937

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122215\
Data File : BG020422.D
Acq On : 23 Dec 2015 00:53
Operator : UM/SJ
Sample : PB87451BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK51

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

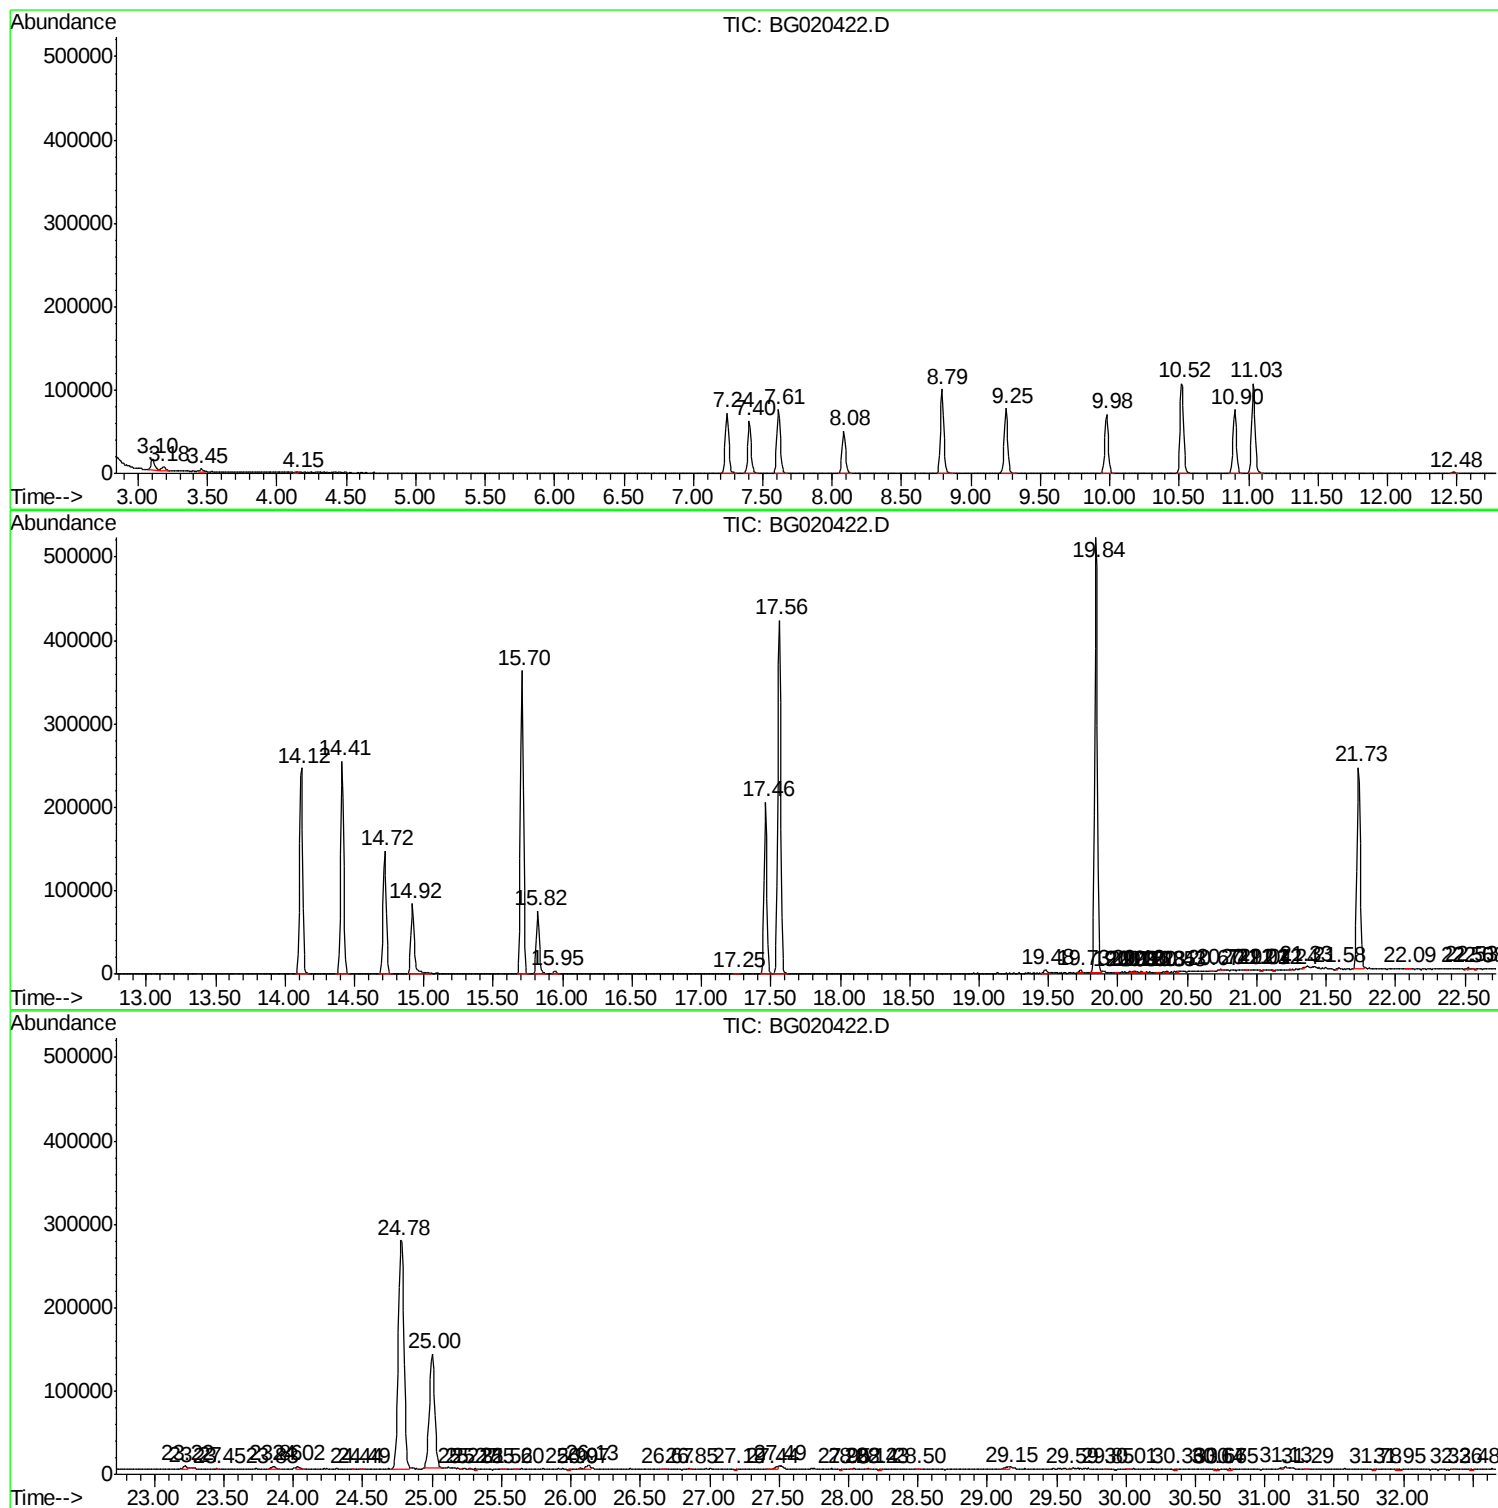

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122215\
Data File : BG020422.D
Acq On : 23 Dec 2015 00:53
Operator : UM/SJ
Sample : PB87451BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK51

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG122215\
Data File : BG020422.D
Acq On : 23 Dec 2015 00:53
Operator : UM/SJ
Sample : PB87451BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK51

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc