


Data Path : Z:\HPCHEM1\BNA G\Data\BG122215\
Data File : BG020408.D
Acq On : 22 Dec 2015 12:31
Operator : UM/SJ
Sample : DFTPP13
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP13

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG121415.M
Title : SVOA CALIBRATION
Last Update : Thu Dec 24 02:43:25 2015

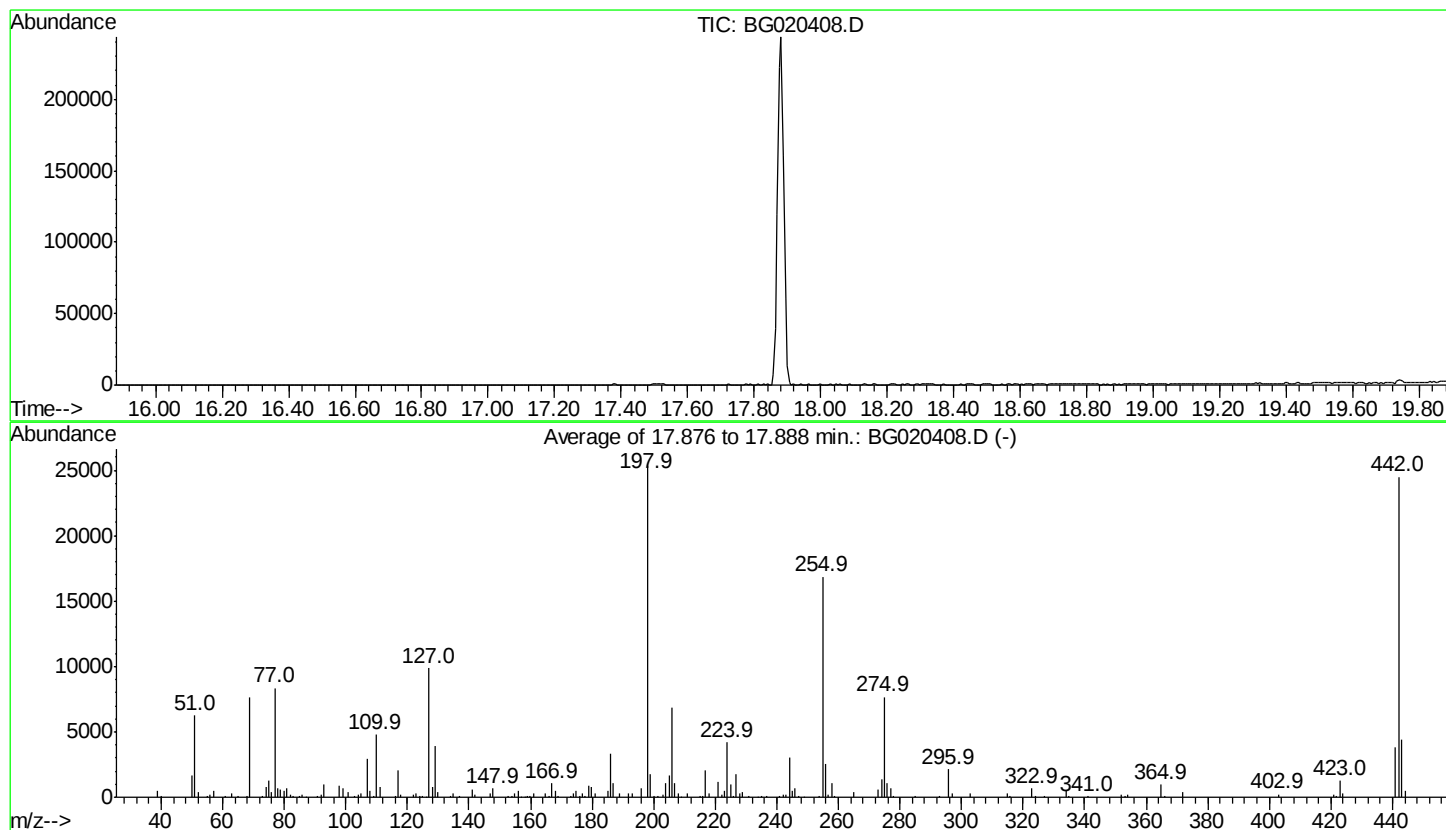

AutoFind: Scans 2559, 2560, 2561; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.6	6228	PASS
68	69	0.00	2	1.0	73	PASS
69	198	0.00	100	30.1	7622	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.8	9848	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	25352	PASS
199	198	5	9	6.8	1736	PASS
275	198	10	60	30.2	7647	PASS
365	198	1	100	3.7	948	PASS
441	442	0.01	24	15.4	3777	PASS
442	198	50	100	96.5	24477	PASS
443	442	15	24	18.2	4445	PASS

m/z	Abundance
39.00	275.0
44.00	156.0
50.00	1154.0
51.00	3909.0
52.00	188.0
57.00	269.0
63.00	196.0
68.90	4998.0
73.90	434.0
75.00	881.0
75.90	305.0
77.00	5536.0
78.00	448.0
79.00	297.0
79.90	379.0
80.90	513.0
85.90	171.0
90.90	153.0
92.90	652.0
98.00	785.0
98.90	456.0
100.90	263.0
104.90	152.0
106.90	2048.0
107.90	356.0
109.90	3107.0
110.90	609.0
117.00	1413.0
117.90	163.0
122.90	277.0
127.00	7121.0
127.90	460.0
128.90	3152.0
129.90	287.0
134.90	240.0
140.90	466.0
146.80	260.0
147.90	487.0
154.90	240.0
155.90	379.0
161.00	291.0
164.90	222.0
167.00	696.0
168.00	369.0
174.00	212.0
175.00	453.0
176.80	193.0
178.90	783.0
180.00	582.0
181.00	266.0
184.90	372.0
185.90	2586.0
186.90	925.0
189.00	213.0
191.90	255.0
193.00	288.0
195.90	618.0
197.90	18832.0
198.90	1353.0
200.00	237.0
203.90	822.0
205.00	1272.0
206.00	5228.0
207.00	752.0
207.90	270.0
210.90	303.0
216.90	1575.0
217.90	194.0
220.90	930.0
222.90	396.0
224.00	3399.0
225.00	740.0
226.90	1316.0
227.90	179.0
228.90	315.0
236.90	171.0
242.00	193.0
242.90	211.0
244.00	2844.0
244.90	254.0
245.90	701.0
254.90	13489.0
255.90	1996.0
256.80	166.0
257.90	852.0
258.90	244.0
264.90	325.0
272.90	482.0
273.90	1057.0
274.90	6130.0
275.90	961.0
276.90	548.0

Instrument :
BNA_G
ClientSampleId :
DFTPP13

295.90	1838.0
296.90	258.0
302.90	230.0
314.90	154.0
322.90	718.0
333.90	382.0
354.00	170.0
364.90	808.0
371.90	445.0
402.90	235.0
420.90	172.0
423.00	1261.0
423.90	292.0
441.00	3812.0
442.00	23480.0
443.00	4122.0
444.00	383.0

Instrument :
BNA_G
ClientSampleId :
DFTPP13

m/z	Abundance
39.00	574.0
39.90	159.0
43.90	240.0
50.00	2010.0
51.00	7345.0
52.00	367.0
56.00	235.0
57.00	602.0
61.00	198.0
63.00	366.0
65.10	184.0
68.90	8846.0
73.00	177.0
74.00	954.0
75.00	1552.0
76.00	409.0
77.00	9821.0
78.00	670.0
78.90	777.0
79.90	675.0
80.90	901.0
81.90	179.0
83.00	210.0
84.90	183.0
85.90	180.0
92.00	225.0
92.90	1327.0
98.00	1006.0
98.90	692.0
100.90	428.0
104.00	229.0
104.90	388.0
107.00	3579.0
107.90	522.0
108.90	165.0
109.90	5494.0
111.00	951.0
116.90	2501.0
118.00	232.0
121.90	248.0
122.90	358.0
123.90	181.0
124.90	179.0
125.90	152.0
127.00	11224.0
128.00	860.0
128.90	4616.0
129.90	553.0
134.00	220.0
134.90	419.0
136.90	243.0
140.90	740.0
141.90	305.0
146.90	344.0
147.90	807.0
152.90	198.0
154.00	204.0
154.90	325.0
156.00	609.0
157.00	153.0
158.00	151.0
159.90	185.0
160.90	226.0
164.90	254.0
165.90	211.0
166.90	1350.0
167.90	545.0
174.00	395.0
174.90	609.0
176.90	345.0
178.90	997.0
179.90	742.0
181.00	277.0
185.00	582.0
186.00	3867.0
186.90	1066.0
188.80	281.0
191.90	295.0
193.00	403.0
195.90	775.0
197.90	29552.0
198.90	2058.0
200.00	179.0
201.30	158.0
203.00	271.0
203.90	1138.0
205.00	1923.0
206.00	8101.0
206.90	1312.0
207.90	279.0
208.90	155.0
210.90	274.0

Instrument :
BNA_G
ClientSampleId :
DFTPP13

214.90	162.0
216.00	177.0
216.90	2269.0
218.00	256.0
220.90	1446.0
222.00	233.0
222.90	520.0
223.90	4618.0
225.00	1038.0
225.90	215.0
226.90	2098.0
227.90	360.0
228.90	472.0
230.80	190.0
234.90	245.0
236.90	163.0
241.90	279.0
243.00	223.0
244.00	3228.0
244.90	449.0
245.90	746.0
247.00	161.0
254.90	19856.0
255.90	3017.0
256.90	294.0
257.90	1089.0
258.90	172.0
264.90	423.0
272.90	770.0
273.90	1609.0
274.90	9073.0
275.90	1147.0
276.90	813.0
278.00	166.0
292.90	196.0
295.90	2337.0
296.90	352.0
302.90	286.0
314.90	309.0
315.90	182.0
323.00	683.0
326.90	160.0
334.00	598.0
334.90	189.0
341.00	216.0
351.90	310.0
352.90	171.0
353.90	273.0
364.90	1107.0
372.00	494.0
402.90	171.0
421.00	220.0
421.90	222.0
423.00	1470.0
424.00	310.0
441.00	4469.0
442.00	28144.0
443.00	4858.0
444.00	552.0

Instrument :
BNA_G
ClientSampleId :
DFTPP13

m/z	Abundance
39.00	709.0
39.90	200.0
43.90	162.0
50.00	1795.0
51.00	7430.0
52.00	510.0
55.00	198.0
55.90	216.0
56.90	650.0
63.00	388.0
65.00	200.0
67.90	219.0
68.90	9023.0
74.00	912.0
75.00	1336.0
76.00	486.0
77.00	9670.0
78.00	848.0
78.90	686.0
79.90	499.0
81.00	752.0
82.00	344.0
83.00	164.0
85.90	338.0
87.00	154.0
90.90	207.0
92.00	275.0
92.90	1022.0
97.90	899.0
98.90	825.0
100.90	436.0
102.90	203.0
104.00	279.0
104.90	319.0
106.90	3233.0
107.90	501.0
109.10	156.0
109.90	5687.0
110.90	878.0
116.10	195.0
116.90	2402.0
117.90	231.0
121.90	223.0
122.90	343.0
127.00	11199.0
128.00	974.0
128.90	4129.0
129.90	333.0
134.90	378.0
140.90	595.0
142.00	198.0
147.00	291.0
147.90	710.0
154.90	419.0
156.00	447.0
159.00	170.0
159.90	203.0
160.90	338.0
164.90	412.0
165.90	203.0
166.90	1174.0
168.00	603.0
168.90	156.0
172.90	204.0
174.00	291.0
175.00	450.0
176.00	214.0
176.90	368.0
177.80	171.0
178.90	912.0
179.90	896.0
180.90	251.0
184.90	581.0
186.00	3673.0
186.90	1213.0
188.90	261.0
191.90	331.0
192.90	337.0
195.90	589.0
197.90	27672.0
198.90	1798.0
201.40	168.0
202.90	268.0
203.90	1173.0
205.00	1913.0
206.00	7356.0
207.00	1214.0
207.90	364.0
211.00	374.0
215.90	167.0
216.90	2195.0
217.90	323.0

Instrument :
BNA_G
ClientSampleId :
DFTPP13

221.00	1034.0
221.90	232.0
222.90	537.0
224.00	4473.0
224.90	1219.0
226.90	1851.0
227.90	215.0
228.80	342.0
230.90	252.0
233.90	150.0
240.80	157.0
241.90	226.0
242.90	250.0
244.00	3132.0
244.90	642.0
245.90	764.0
247.00	191.0
248.90	152.0
253.80	194.0
254.90	17192.0
255.90	2554.0
256.80	186.0
257.90	1188.0
264.90	371.0
272.90	537.0
274.00	1344.0
274.90	7740.0
276.00	1074.0
276.90	725.0
277.90	160.0
285.00	217.0
296.00	2192.0
297.00	351.0
302.90	245.0
314.90	360.0
315.90	206.0
322.90	647.0
324.00	167.0
326.80	180.0
334.00	476.0
351.90	298.0
353.00	229.0
353.90	243.0
364.90	930.0
365.90	171.0
371.90	370.0
402.90	235.0
421.00	160.0
423.00	1074.0
423.90	214.0
440.90	3052.0
442.00	21808.0
443.00	4356.0
444.00	516.0

Instrument :

BNA_G

ClientSampleId :

DFTPP13

Scan 2554 (17.846 min): BG020408.D
DFTPP13

m/z	Abundance
43.90	190.0

Instrument :
BNA_G
ClientSampleId :
DFTPP13