


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122216\
 Data File : BG025378.D
 Acq On : 22 Dec 2016 7:34
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\Methods\8270-BG122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 21 18:42:01 2016

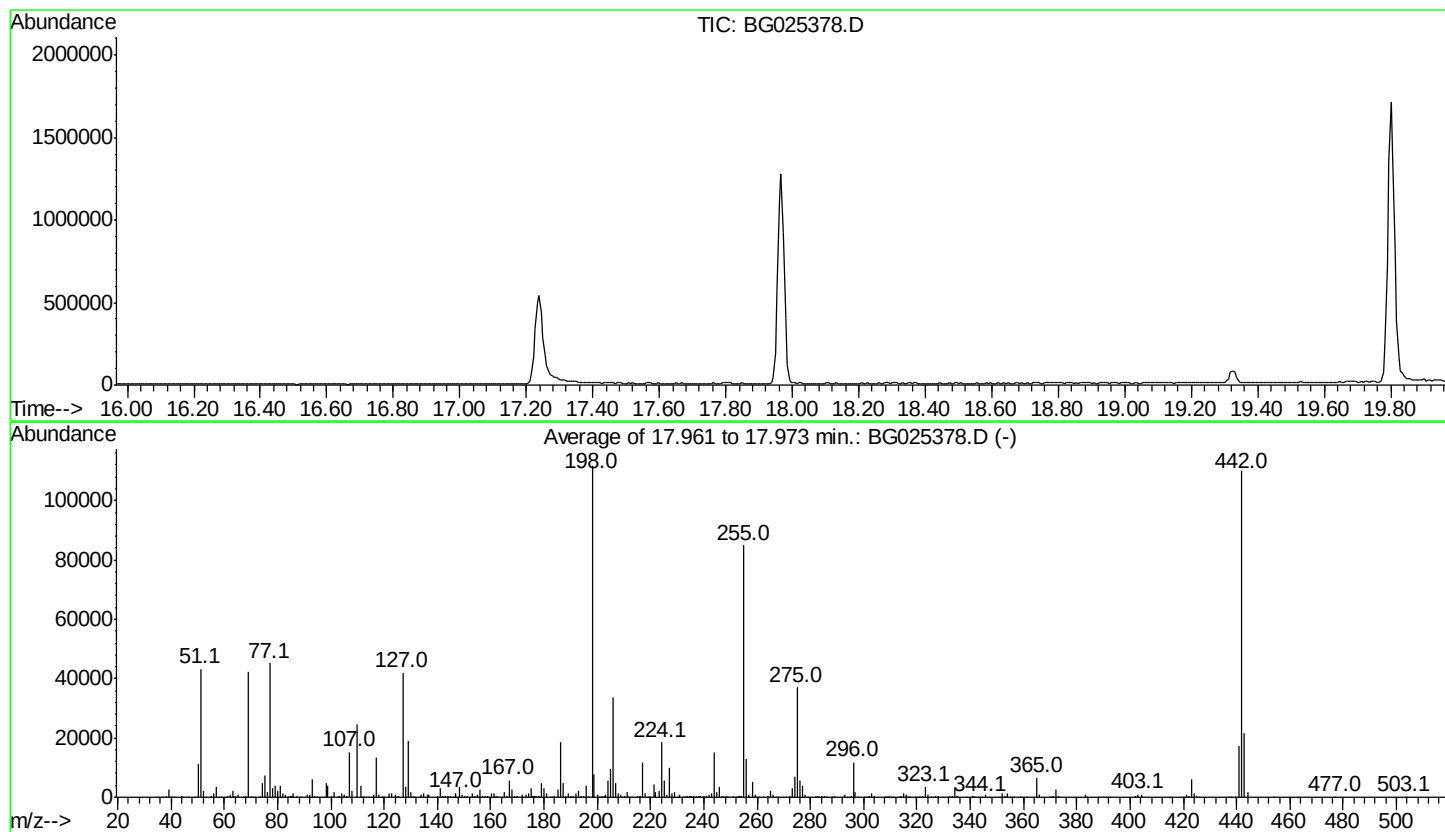

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	43178	PASS
68	69	0.00	2	1.5	620	PASS
69	198	0.00	100	37.7	42144	PASS
70	69	0.00	2	0.5	197	PASS
127	198	10	80	37.5	41946	PASS
197	198	0.00	2	0.3	283	PASS
198	198	100	100	100.0	111760	PASS
199	198	5	9	7.1	7917	PASS
275	198	10	60	33.1	37048	PASS
365	198	1	100	5.9	6570	PASS
441	442	0.01	24	15.8	17460	PASS
442	198	50	100	98.6	110216	PASS
443	442	15	24	19.5	21522	PASS