

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122217\
 Data File : BG031753.D
 Acq On : 23 Dec 2017 17:41
 Operator : SJ/JU
 Sample : I7022-07
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 160

Quant Time: Dec 25 04:48:46 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 22 11:08:55 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.82	152	49647	20.00	ng	-0.02
21) Naphthalene-d8	11.71	136	201328	20.00	ng	-0.01
38) Acenaphthene-d10	15.46	164	134114	20.00	ng	-0.01
63) Phenanthrene-d10	18.19	188	333375	20.00	ng	-0.01
75) Chrysene-d12	22.55	240	392119	20.00	ng	-0.02
86) Perylene-d12	26.33	264	420017	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	6.24	112	396952	145.63	ng	0.00
7) Phenol-d6	7.92	99	456796	129.08	ng	0.00
23) Nitrobenzene-d5	10.03	82	306610	115.00	ng	-0.01
41) 2,4,6-Tribromophenol	16.93	330	328689	160.62	ng	-0.01
44) 2-Fluorobiphenyl	14.09	172	1101383	103.08	ng	-0.01
78) Terphenyl-d14	20.73	244	1937338	112.88	ng	-0.01
Target Compounds						
9) Benzaldehyde	8.33	77	10101	4.740	ng	95
19) n-Nitroso-di-n-propylamine	10.02	70	40617	16.805	ng	# 72
32) Benzoic acid	10.93	122	136	6.751	ng	# 84
50) 2,6-Dinitrotoluene	15.46	165	16681	7.675	ng	# 19
56) 2,4-Dinitrotoluene	15.46	165	16681	5.969	ng	# 17
64) 4,6-Dinitro-2-methylphenol	16.93	198	839	8.734	ng	# 11
66) 4-Bromophenyl-phenylether	16.93	248	25992	5.392	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122217\
Data File : BG031753.D
Acq On : 23 Dec 2017 17:41
Operator : SJ/JU
Sample : I7022-07
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
160

Quant Time: Dec 25 04:48:46 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 11:08:55 2017
Response via : Initial Calibration

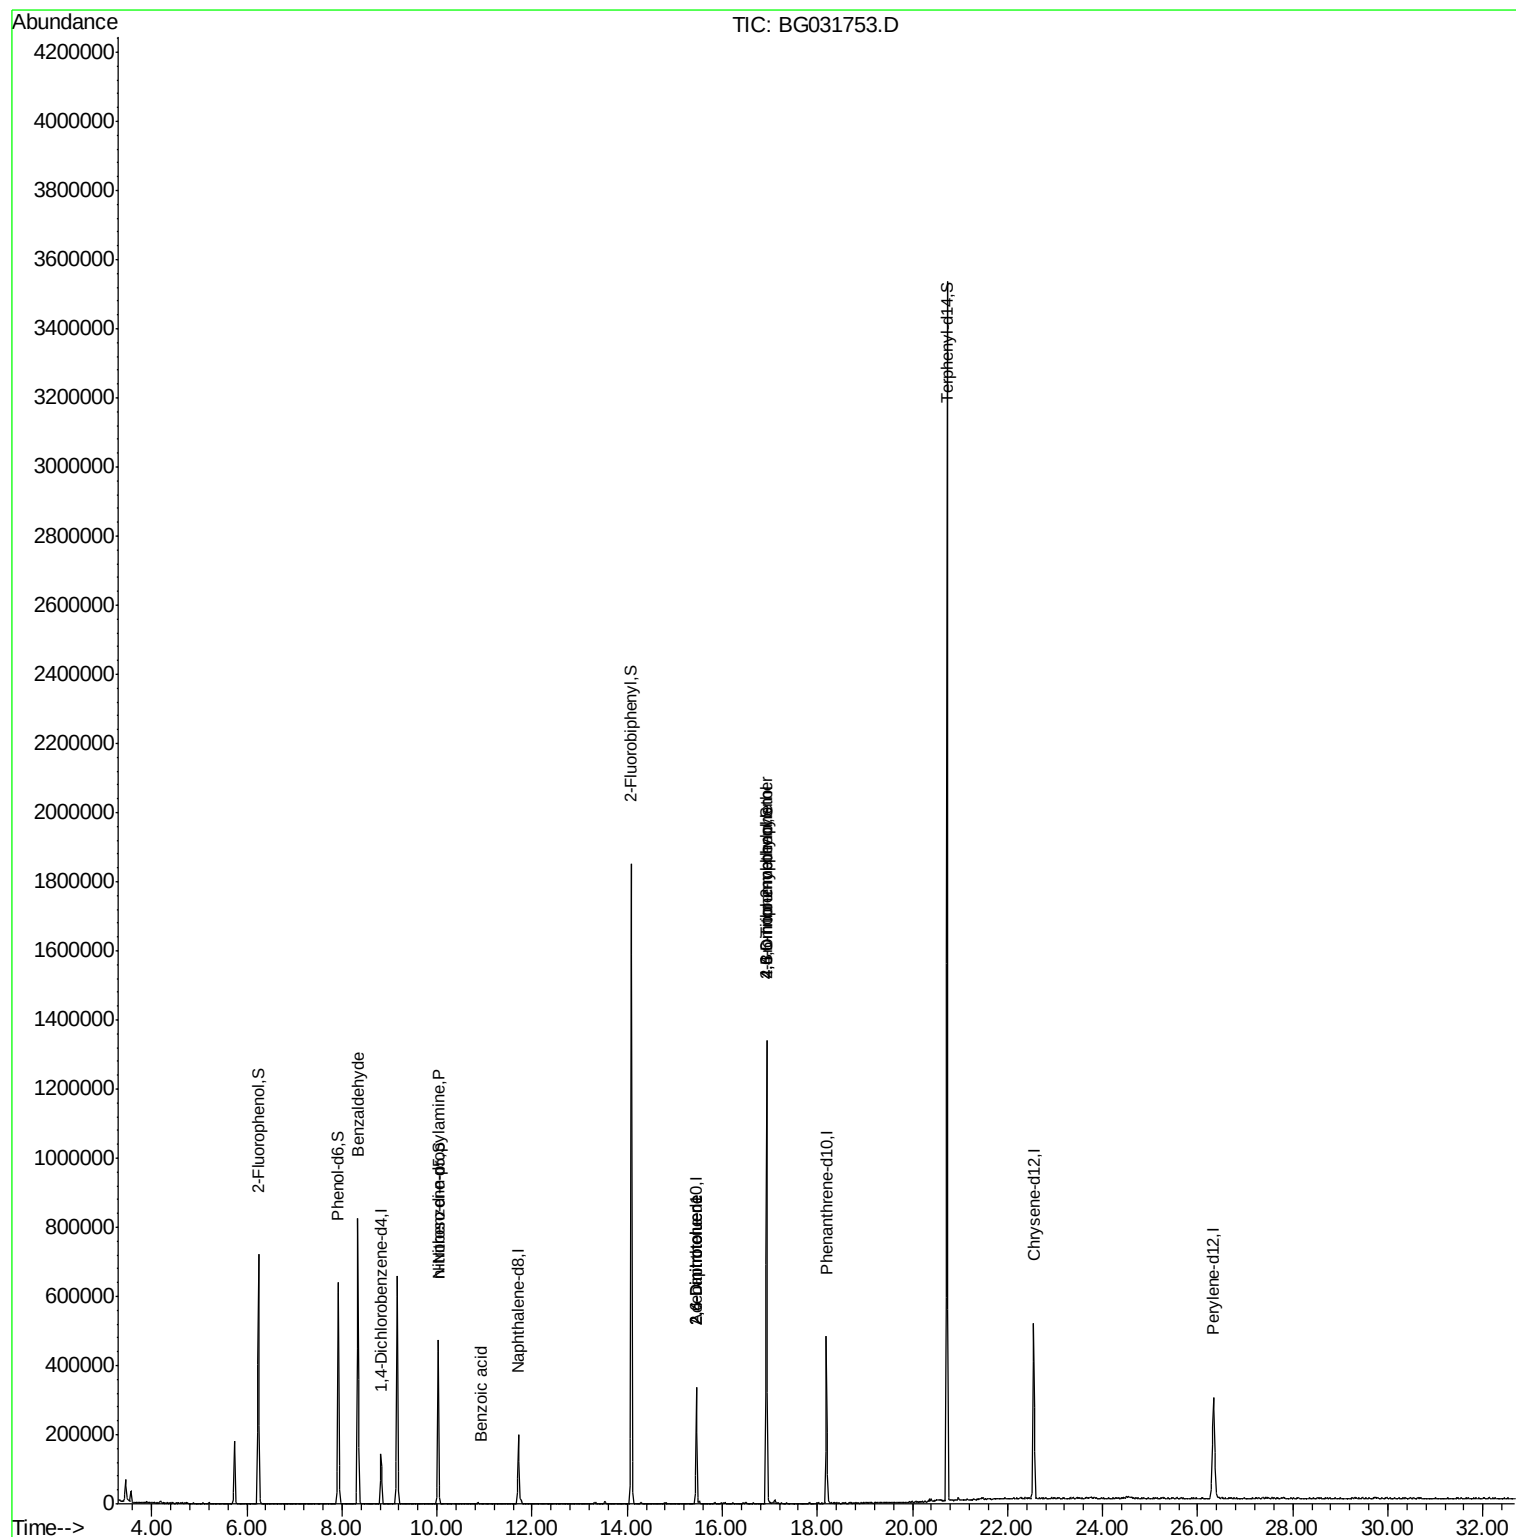

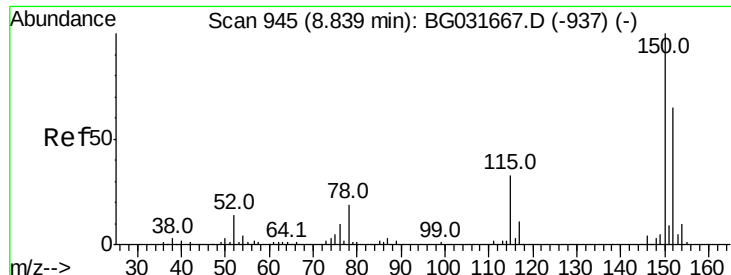


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.82 min Scan# 942
Delta R.T. -0.02 min
Lab File: BG031753.D
Acq: 23 Dec 2017 17:41

Instrument :
BNA_G
ClientSampleId :
160

Tot Ion	Ratio	Lower	Upper
152	100		
150	151.2	126.6	189.8
115	53.4	53.0	79.4

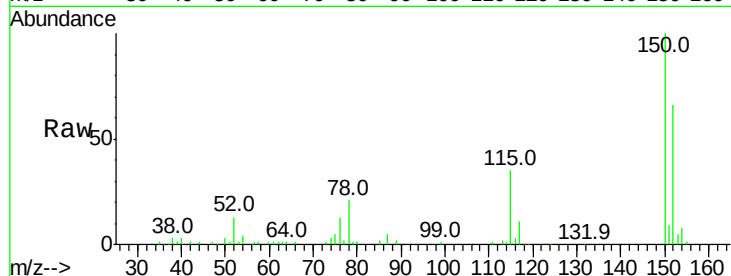


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

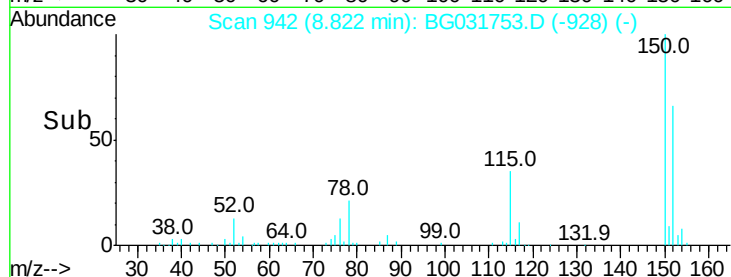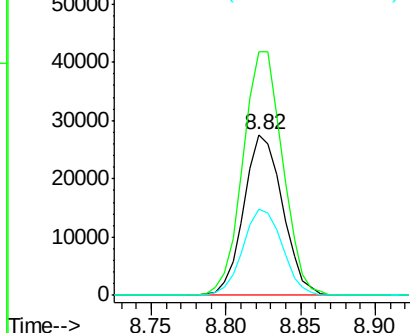



#5


2-Fluorophenol
Concen: 145.629 ng
RT: 6.24 min Scan# 503
Delta R.T. -0.01 min
Lab File: BG031753.D
Acq: 23 Dec 2017 17:41

Tgt Ion	Ratio	Lower	Upper
112	100		
64	46.2	56.3	84.5#
63	25.1	30.1	45.1#



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

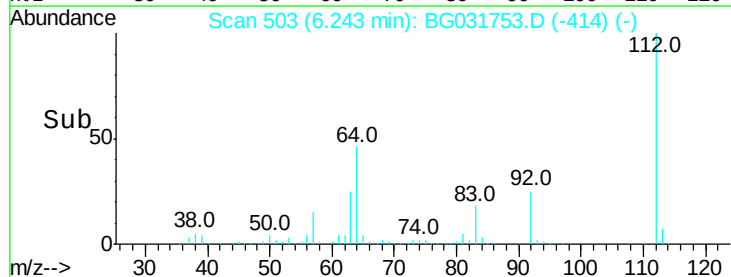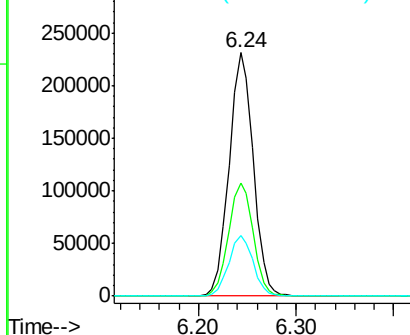

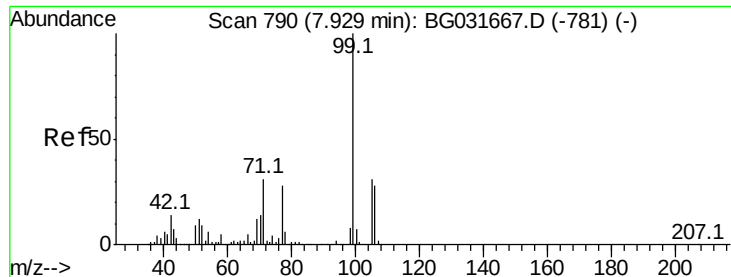

#7

Phenol-d6

Concen: 129.076 ng

RT: 7.92 min Scan# 789

Delta R.T. -0.01 min

Lab File: BG031753.D

Acq: 23 Dec 2017 17:41

Instrument :

BNA_G

ClientSampleId :

160





Tot Ion: 99 Resp: 456796

Ion Ratio Lower Upper

99 100

42 13.7 14.1 21.1#

71 34.4 26.1 39.1

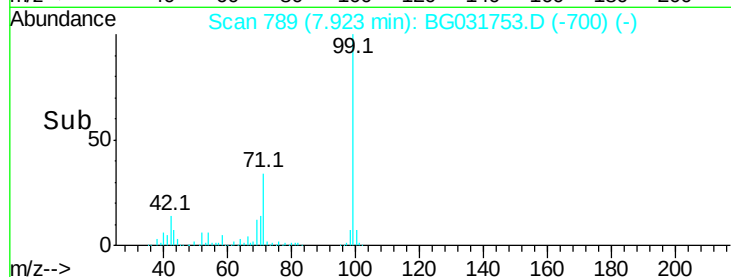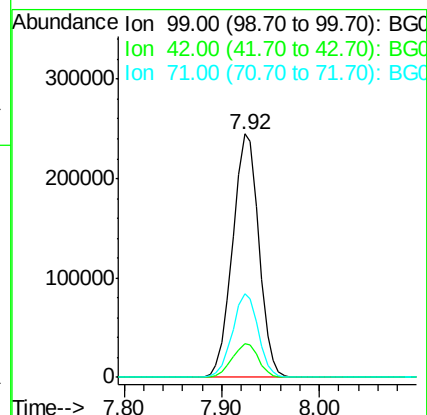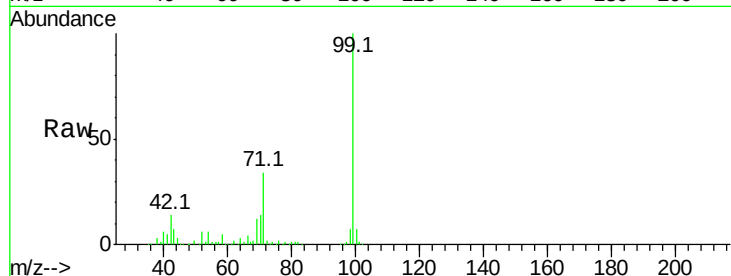

#9

Benzaldehyde

Concen: 4.740 ng

RT: 8.33 min Scan# 859

Delta R.T. 0.40 min

Lab File: BG031753.D

Acq: 23 Dec 2017 17:41




Tgt Ion: 77 Resp: 10101


Ion Ratio Lower Upper

77 100

105 90.5 71.3 111.3

106 74.9 64.2 104.2


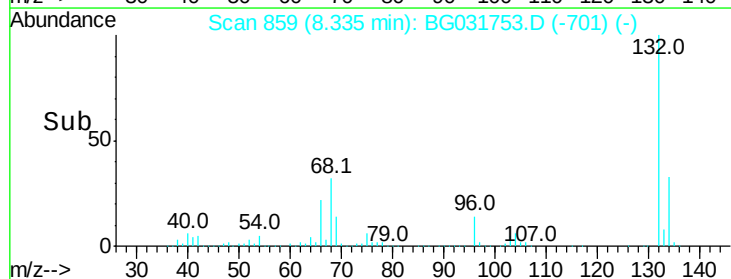
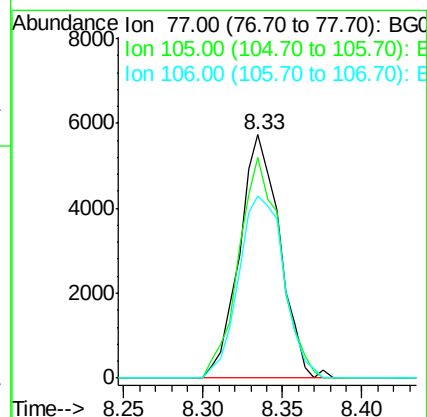



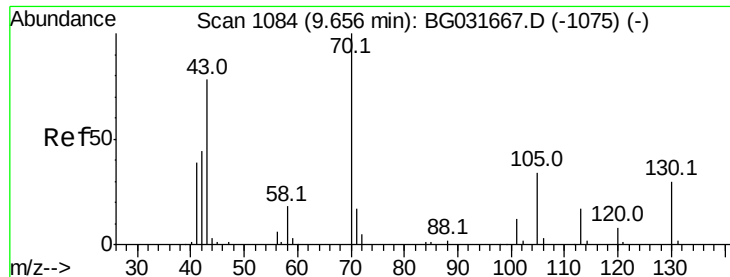

#19
n-Nitroso-di-n-propylamine
Concen: 16.805 ng
RT: 10.02 min Scan# 1146
Delta R.T. 0.36 min
Lab File: BG031753.D
Acq: 23 Dec 2017 17:41




Instrument :
BNA_G
ClientSampleId :
160


Tot Ion: 70 Resp: 40617
Ion Ratio Lower Upper
70 100
42 41.3 49.1 73.7#
101 0.0 8.5 12.7#
130 1.4 13.4 20.0#

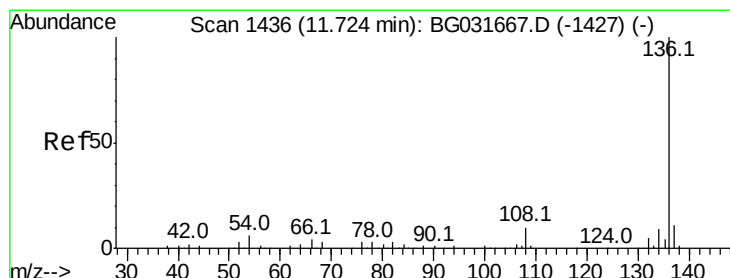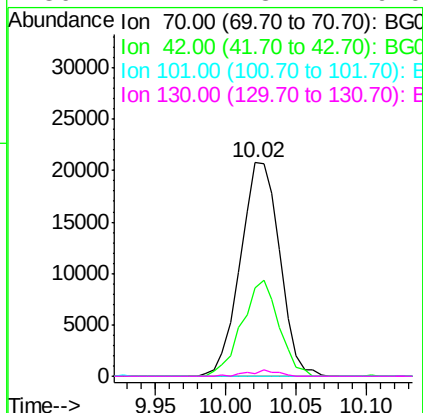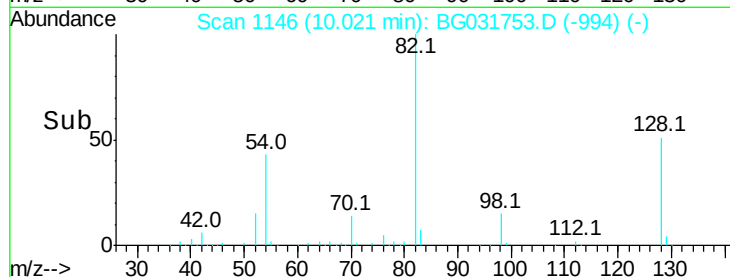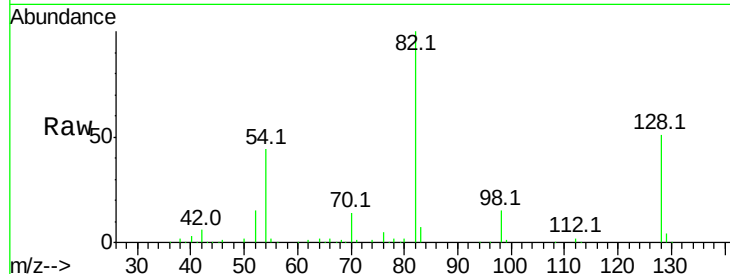

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.71 min Scan# 1434
Delta R.T. -0.01 min
Lab File: BG031753.D
Acq: 23 Dec 2017 17:41

Tgt Ion: 136 Resp: 201328
Ion Ratio Lower Upper
136 100
137 9.6 9.2 13.8
54 4.4 10.3 15.5#
68 3.7 4.5 6.7#


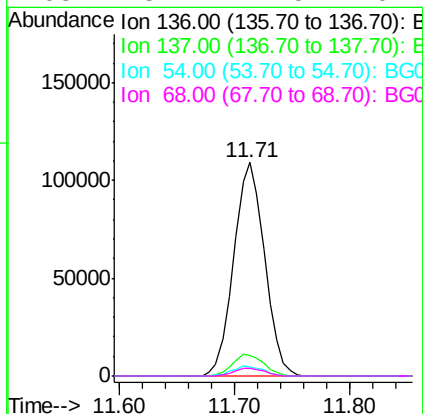
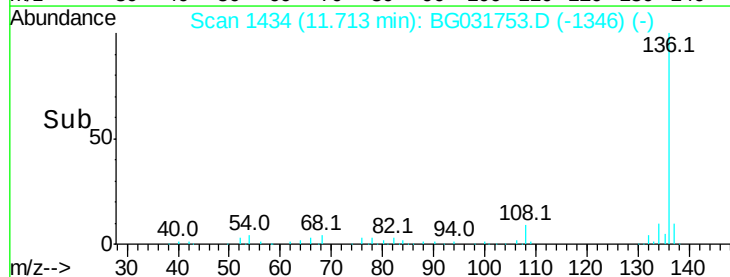
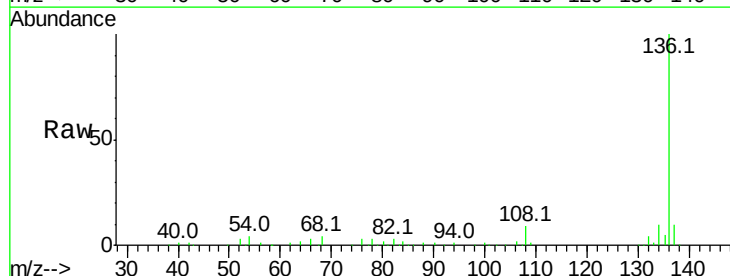


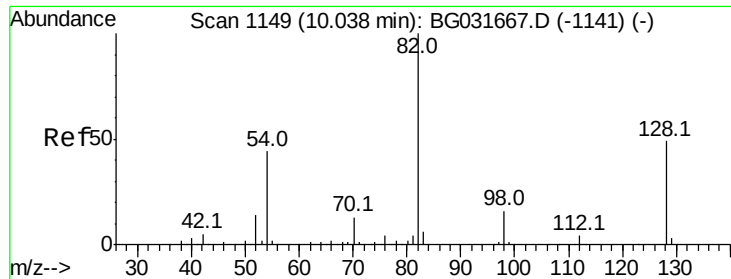

#23
 Nitrobenzene-d5
 Concen: 115.000 ng
 RT: 10.03 min Scan# 1147
 Delta R.T. -0.01 min
 Lab File: BG031753.D
 Acq: 23 Dec 2017 17:41




Instrument :
 BNA_G
 ClientSampleId :
 160


Tot Ion	82	Resp	306610
Ion Ratio	Lower	Upper	
82	100		
128	52.7	29.7	44.5#
54	42.8	43.1	64.7#

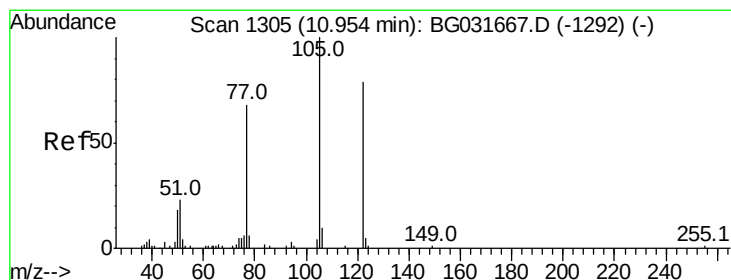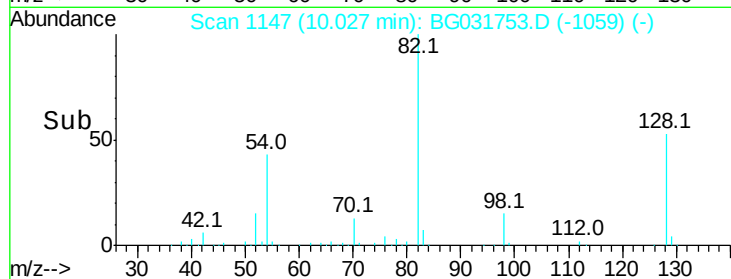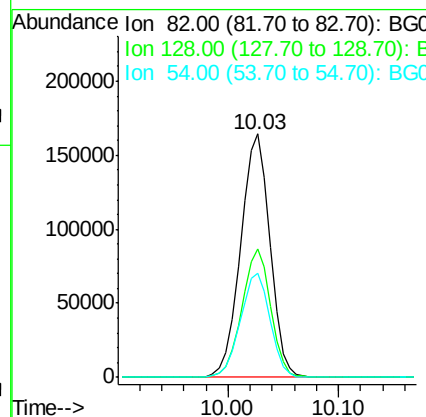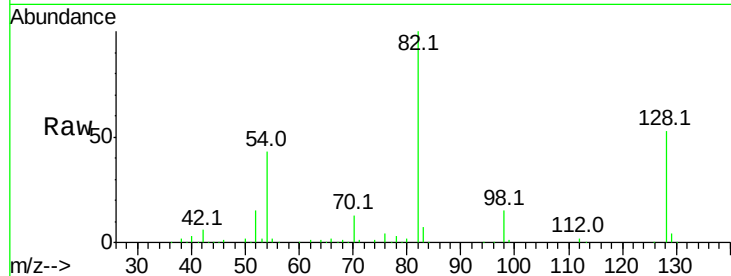

#32
 Benzoic acid
 Concen: 6.751 ng
 RT: 10.93 min Scan# 1300
 Delta R.T. -0.03 min
 Lab File: BG031753.D
 Acq: 23 Dec 2017 17:41

Tgt Ion	122	Resp	136
Ion Ratio	Lower	Upper	
122	100		
105	131.7	123.5	163.5
77	79.4	85.7	125.7#


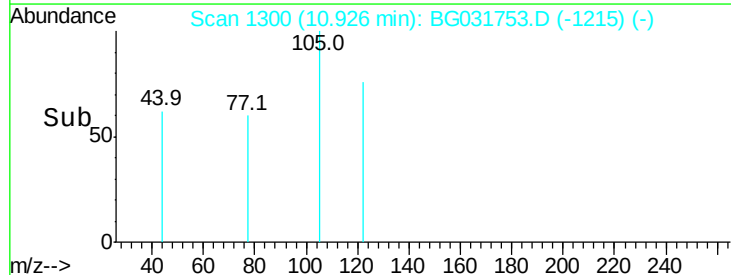
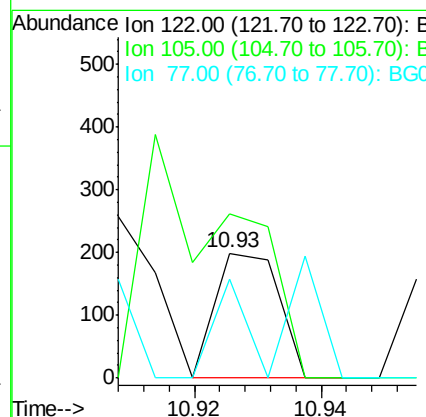



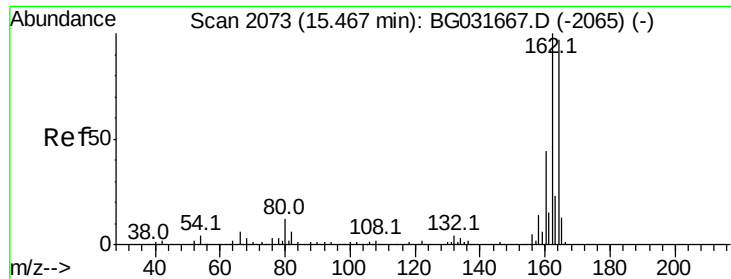

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 15.46 min Scan# 2071
Delta R.T. -0.01 min
Lab File: BG031753.D
Acq: 23 Dec 2017 17:41




Instrument :
BNA_G
ClientSampleId :
160


Tot Ion:164 Resp: 134114
Ion Ratio Lower Upper
164 100
162 104.7 78.8 118.2
160 45.2 35.4 53.0

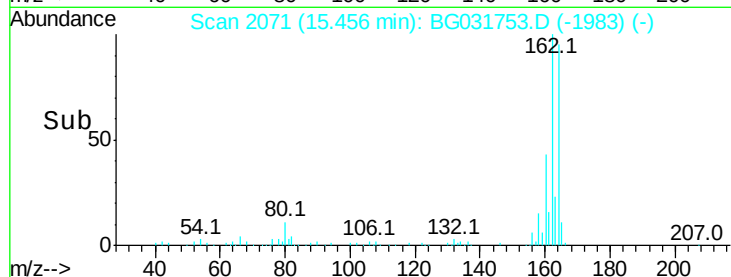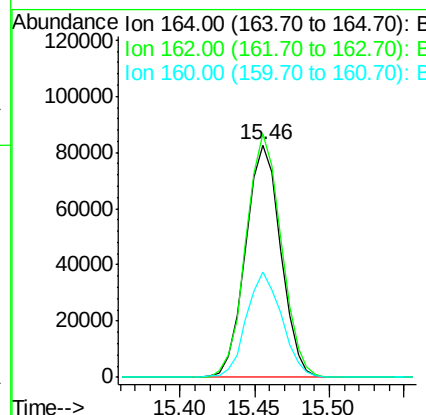

#41
2,4,6-Tribromophenol
Concen: 160.619 ng
RT: 16.93 min Scan# 2322
Delta R.T. -0.01 min
Lab File: BG031753.D
Acq: 23 Dec 2017 17:41

Tgt Ion:330 Resp: 328689
Ion Ratio Lower Upper
330 100
332 97.1 77.0 115.6
141 25.0 25.2 37.8#


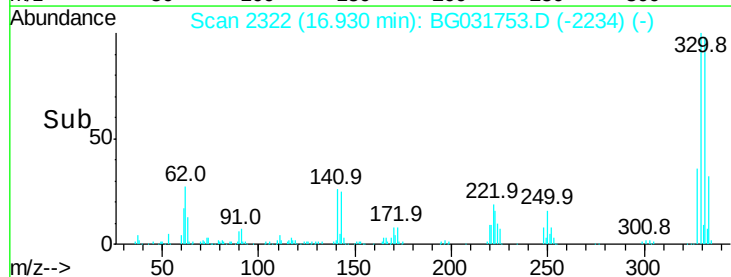
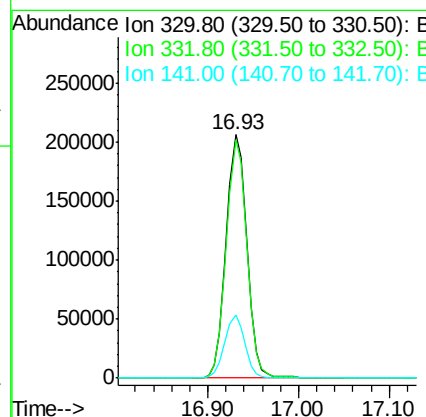



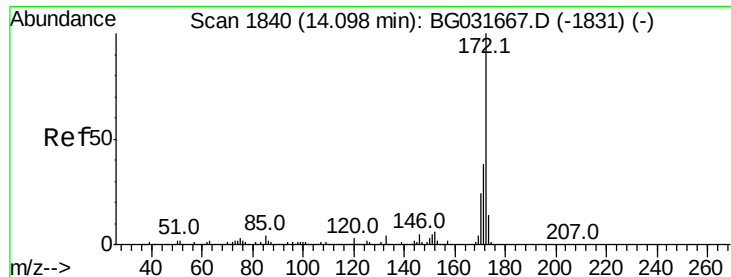

#44
2-Fluorobiphenyl
Concen: 103.075 ng
RT: 14.09 min Scan# 1838
Delta R.T. -0.01 min
Lab File: BG031753.D
Acq: 23 Dec 2017 17:41




Instrument :
BNA_G
ClientSampleId :
160


Tot Ion:172 Resp: 1101383
Ion Ratio Lower Upper
172 100
171 37.7 30.0 45.0
170 23.9 19.5 29.3

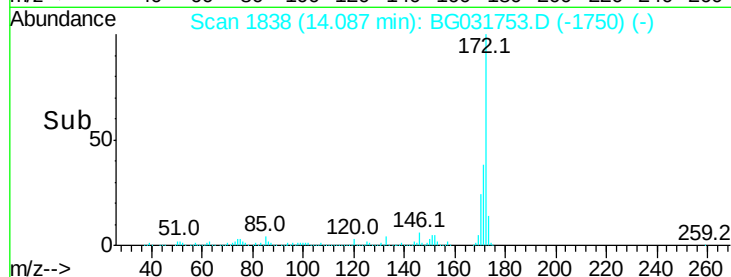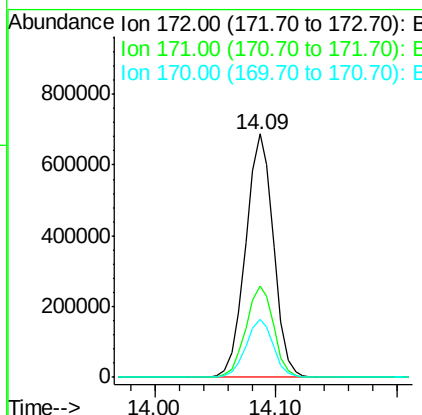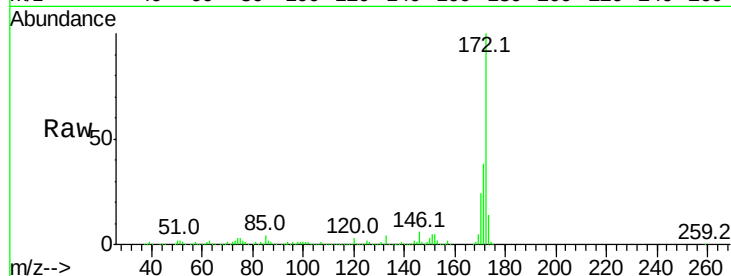

#50
2,6-Dinitrotoluene
Concen: 7.675 ng
RT: 15.46 min Scan# 2071
Delta R.T. 0.44 min
Lab File: BG031753.D
Acq: 23 Dec 2017 17:41

Tgt Ion:165 Resp: 16681
Ion Ratio Lower Upper
165 100
63 1.5 52.7 79.1#
89 0.0 49.2 73.8#


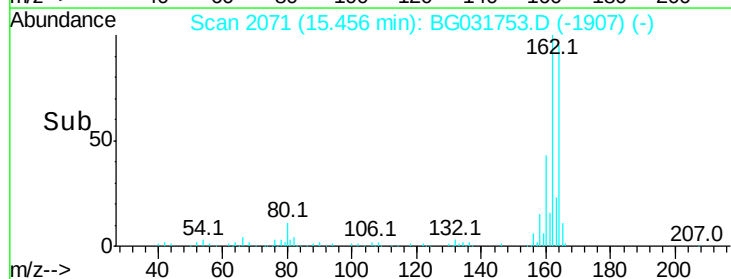
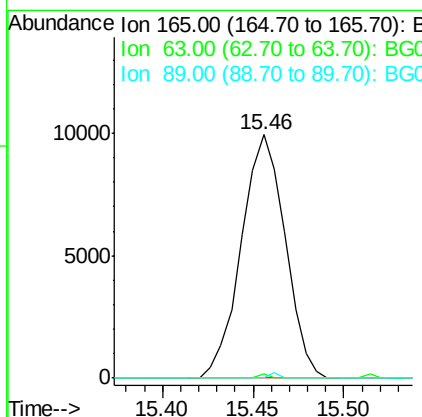



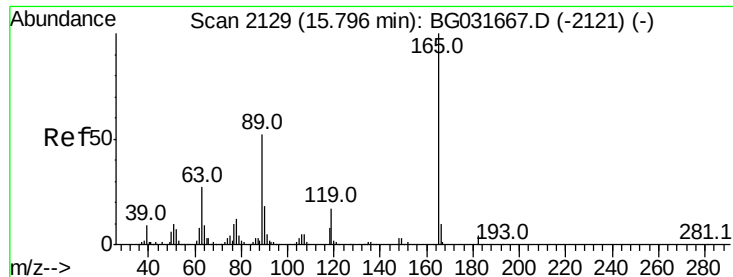

#56
2,4-Dinitrotoluene
Concen: 5.969 ng
RT: 15.46 min Scan# 2071
Delta R.T. -0.34 min
Lab File: BG031753.D
Acq: 23 Dec 2017 17:41




Instrument :
BNA_G
ClientSampleId :
160


Tot Ion	Ratio	Lower	Upper
165	100		
63	1.5	42.0	63.0#
89	0.0	66.9	100.3#
182	0.0	2.6	3.8#

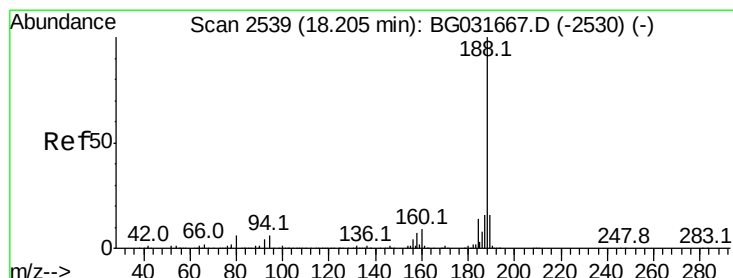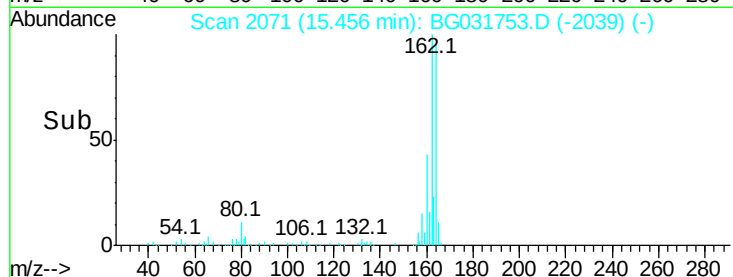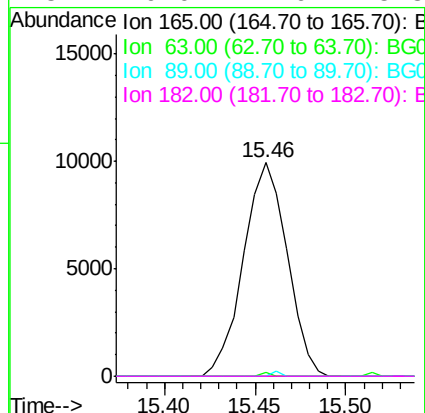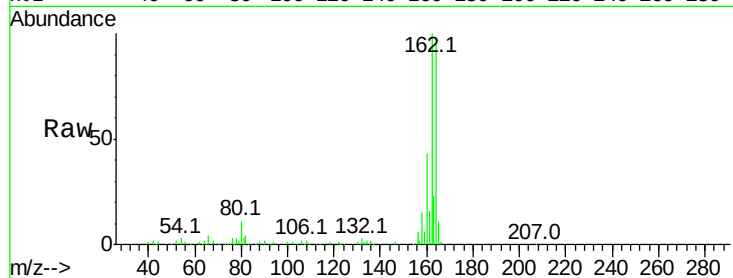

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 18.19 min Scan# 2537
Delta R.T. -0.01 min
Lab File: BG031753.D
Acq: 23 Dec 2017 17:41

Tgt Ion	Ratio	Lower	Upper
188	100		
94	5.4	6.9	10.3#
80	5.6	7.7	11.5#

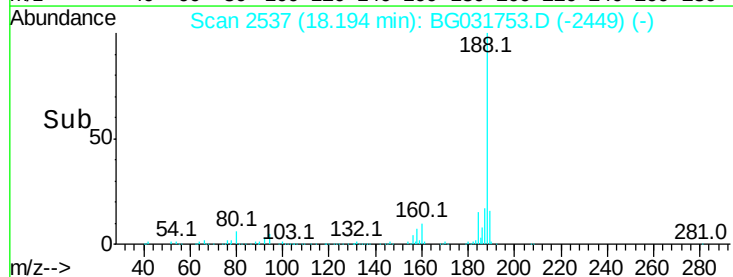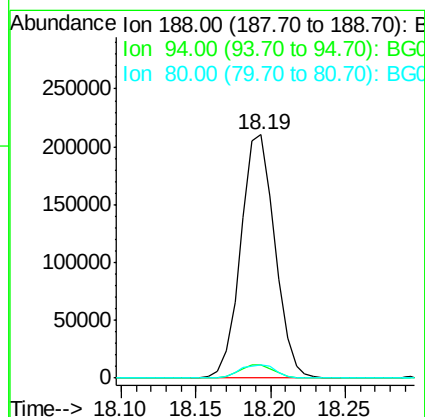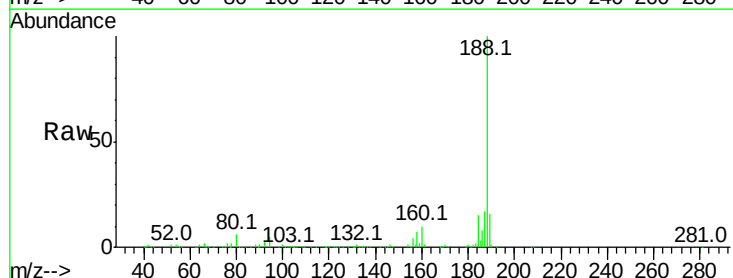


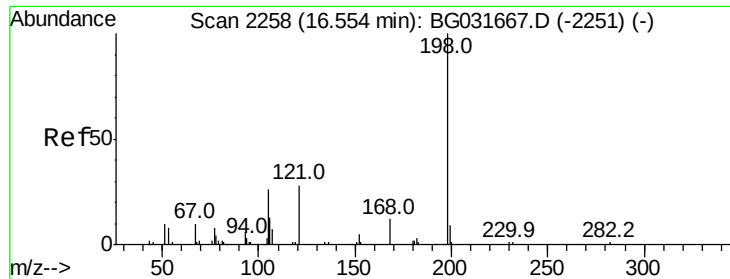




#64
4,6-Dinitro-2-methylphenol
Concen: 8.734 ng
RT: 16.93 min Scan# 2322
Delta R.T. 0.38 min
Lab File: BG031753.D
Acq: 23 Dec 2017 17:41

Instrument :
BNA_G
ClientSampled :
160

Tot Ion:198 Resp: 839
Ion Ratio Lower Upper
198 100
51 75.4 30.6 70.6#
105 141.3 23.8 63.8#

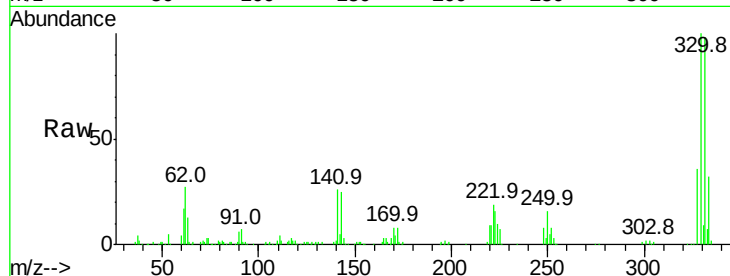


Abundance Ion 198.00 (197.70 to 198.70): E
Ion 51.00 (50.70 to 51.70): BGC
Ion 105.00 (104.70 to 105.70): E

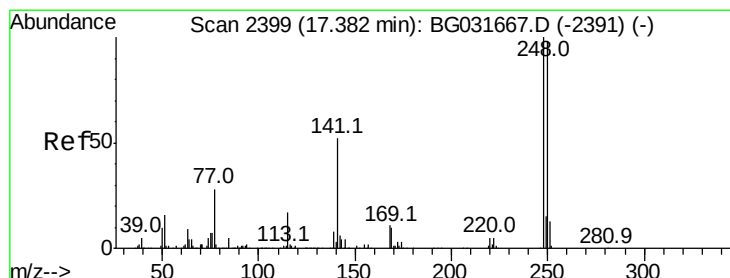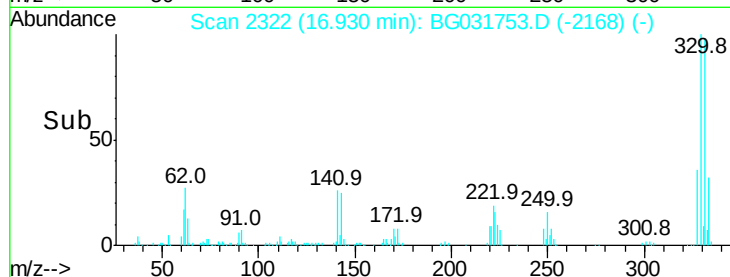
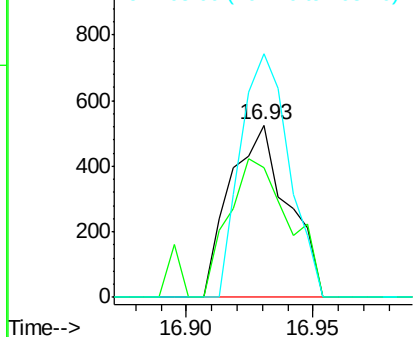



#66
4-Bromophenyl-phenylether
Concen: 5.392 ng
RT: 16.93 min Scan# 2322
Delta R.T. -0.45 min
Lab File: BG031753.D
Acq: 23 Dec 2017 17:41

Tgt Ion:248 Resp: 25992
Ion Ratio Lower Upper
248 100
250 205.8 77.1 115.7#
141 338.3 50.8 76.2#

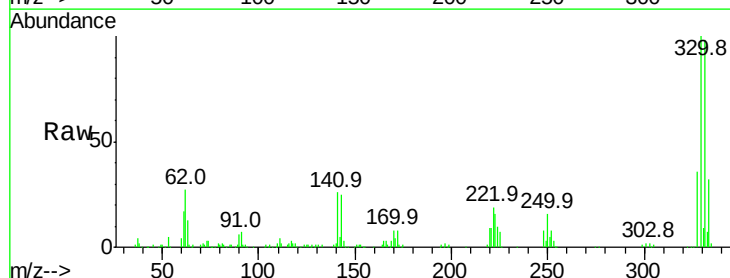

Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

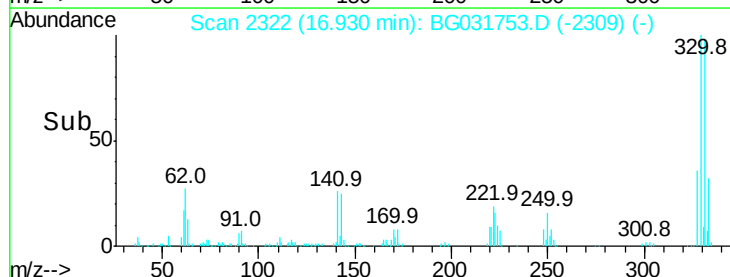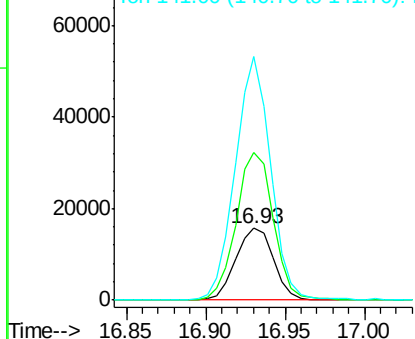

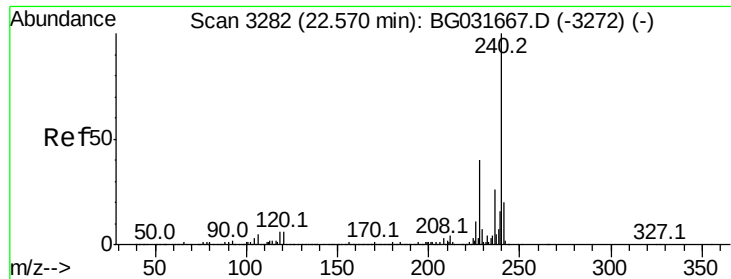

#75

Chrysene-d12

Concen: 20.000 ng

RT: 22.55 min Scan# 3278

Delta R.T. -0.02 min

Lab File: BG031753.D

Acq: 23 Dec 2017 17:41

Instrument :

BNA_G

ClientSampleId :

160


Tot Ion:240 Resp: 392119

Ion Ratio Lower Upper

240 100

120 5.9 6.8 10.2#




236 25.3 20.9 31.3

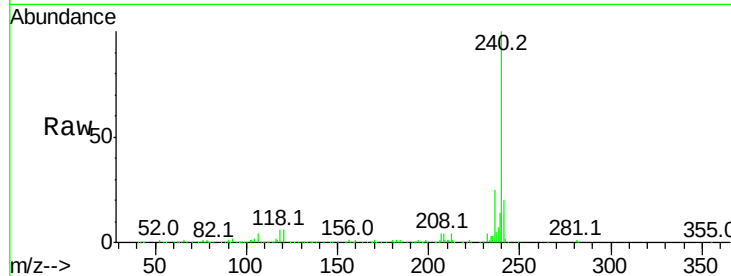

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

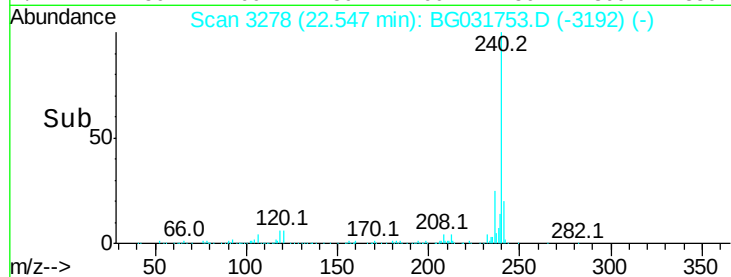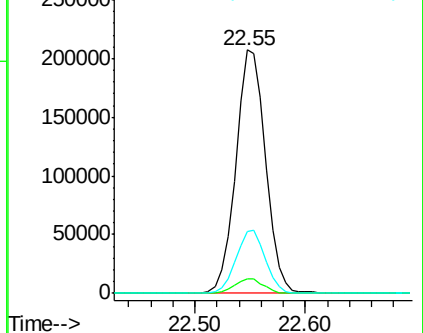

#78

Terphenyl-d14

Concen: 112.877 ng

RT: 20.73 min Scan# 2968

Delta R.T. -0.01 min

Lab File: BG031753.D

Acq: 23 Dec 2017 17:41


Tgt Ion:244 Resp: 1937338

Ion Ratio Lower Upper

244 100

212 7.7 5.8 8.8



122 7.3 7.0 10.4




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

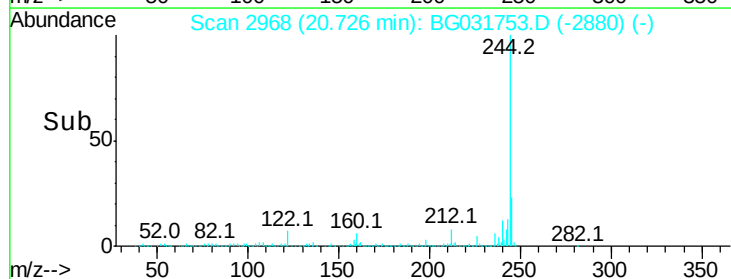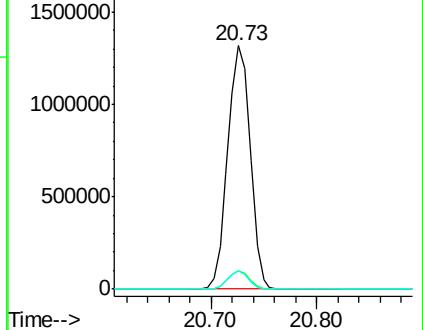


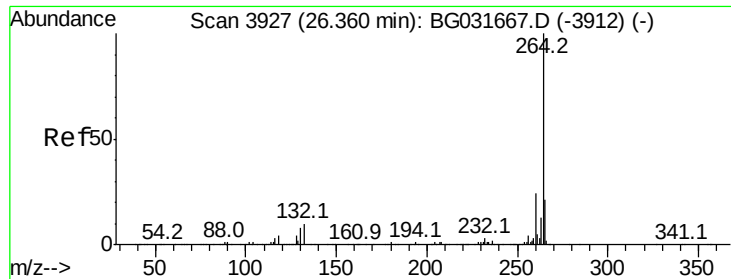

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 26.33 min Scan# 3922
 Delta R.T. -0.03 min
 Lab File: BG031753.D
 Acq: 23 Dec 2017 17:41

Instrument :
 BNA_G
 ClientSampleId :
 160

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.7	17.4	26.0
265	21.8	17.7	26.5



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

