
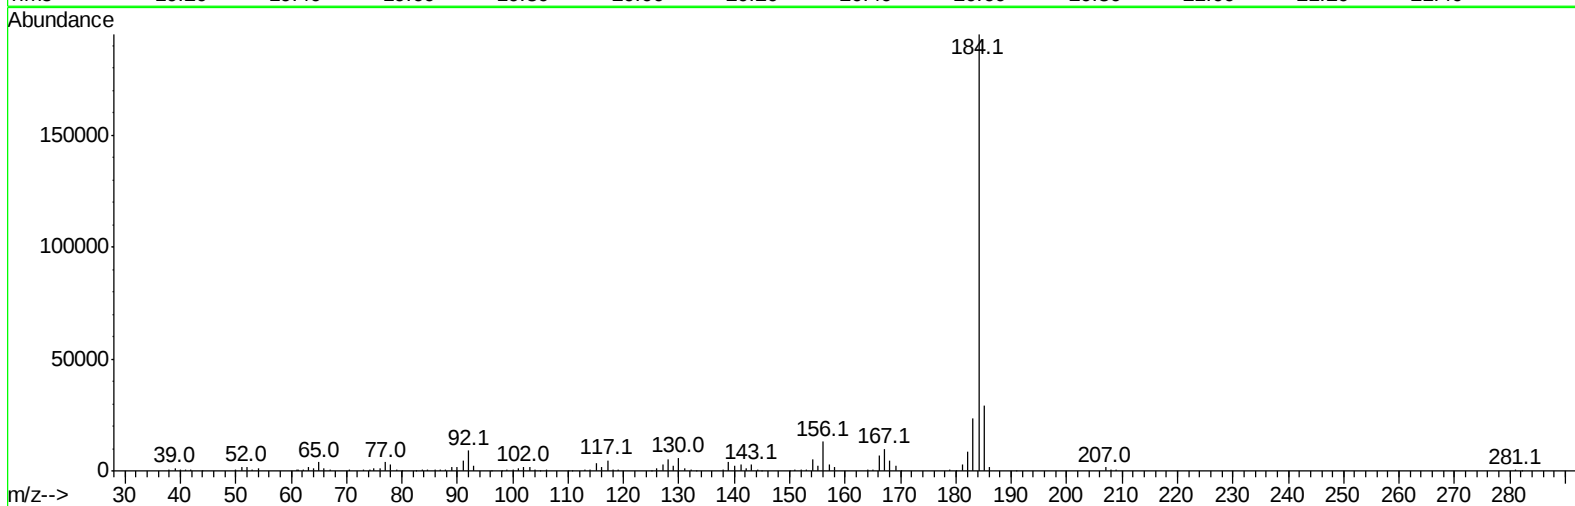


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122217\
Data File : BG031713.D
Acq On : 22 Dec 2017 16:16
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 01:09:53 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 11:08:55 2017
Response via : Initial Calibration

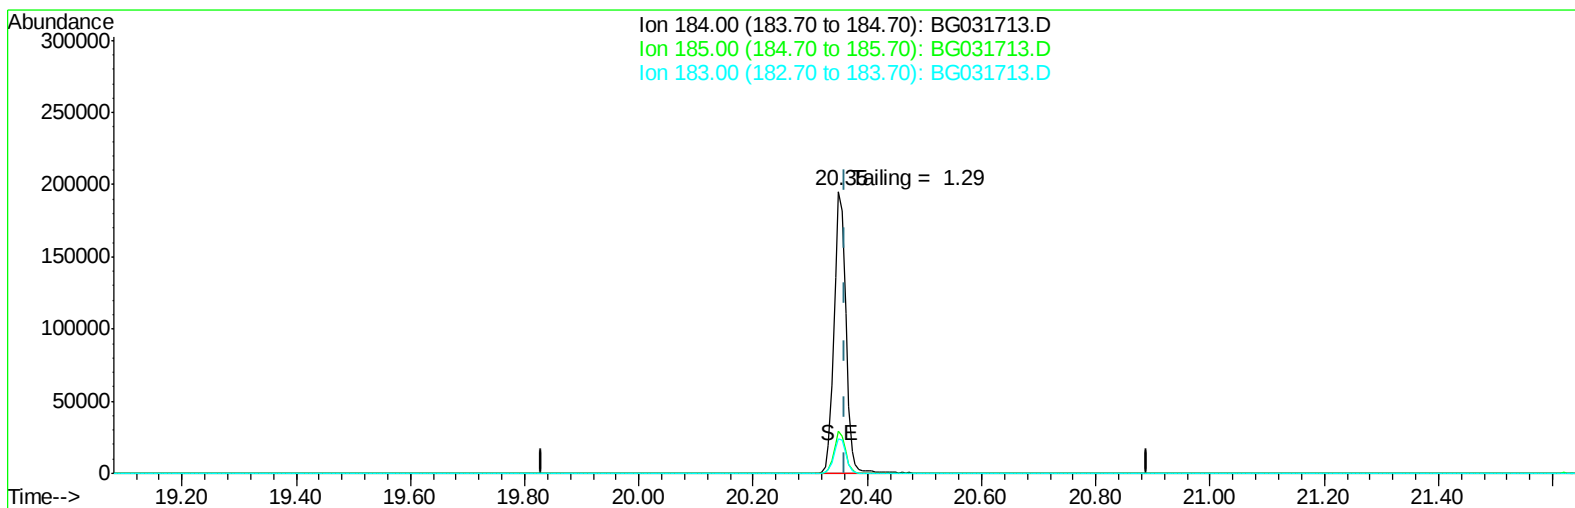

TIC: BG031713.D

(76) Benzidine



20.350min (-0.011) 0.00ng

response 280559

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.07
183.00	13.30	12.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122217\
Data File : BG031713.D
Acq On : 22 Dec 2017 16:16
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 01:09:53 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 11:08:55 2017
Response via : Initial Calibration

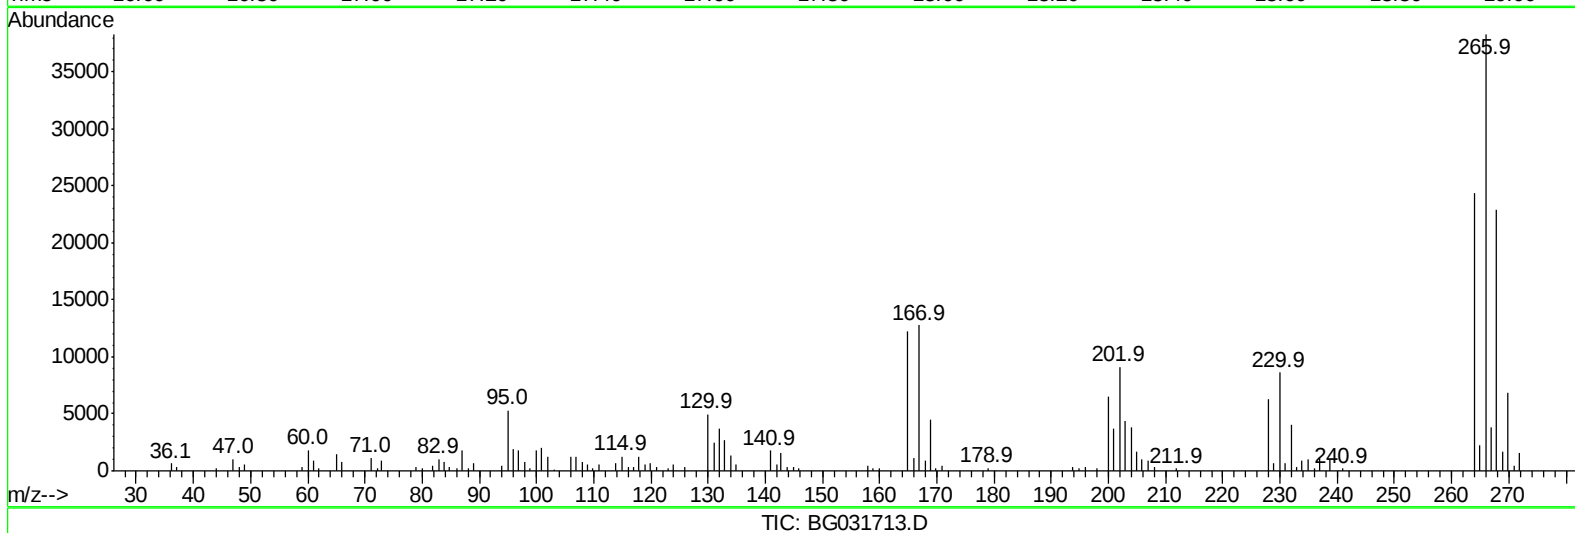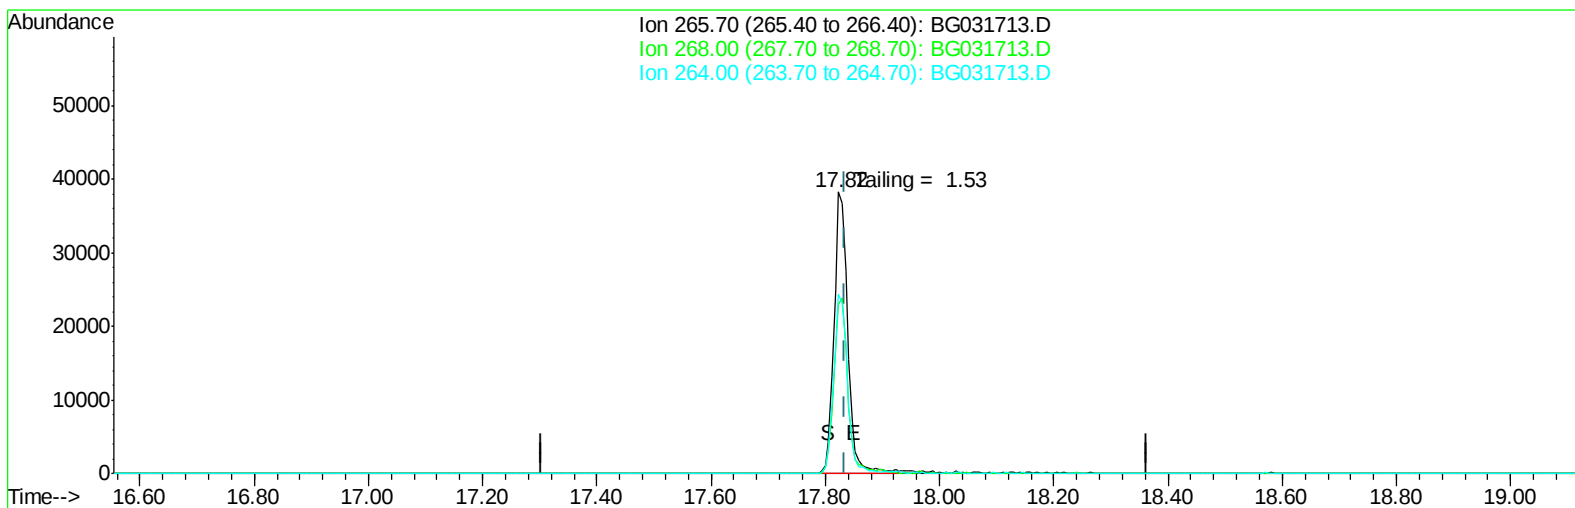

TIC: BG031713.D

(69) Pentachlorophenol (C)

17.823min (-0.011) 35364.22ng

response 63285

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.83
264.00	62.00	63.78
0.00	0.00	0.00