
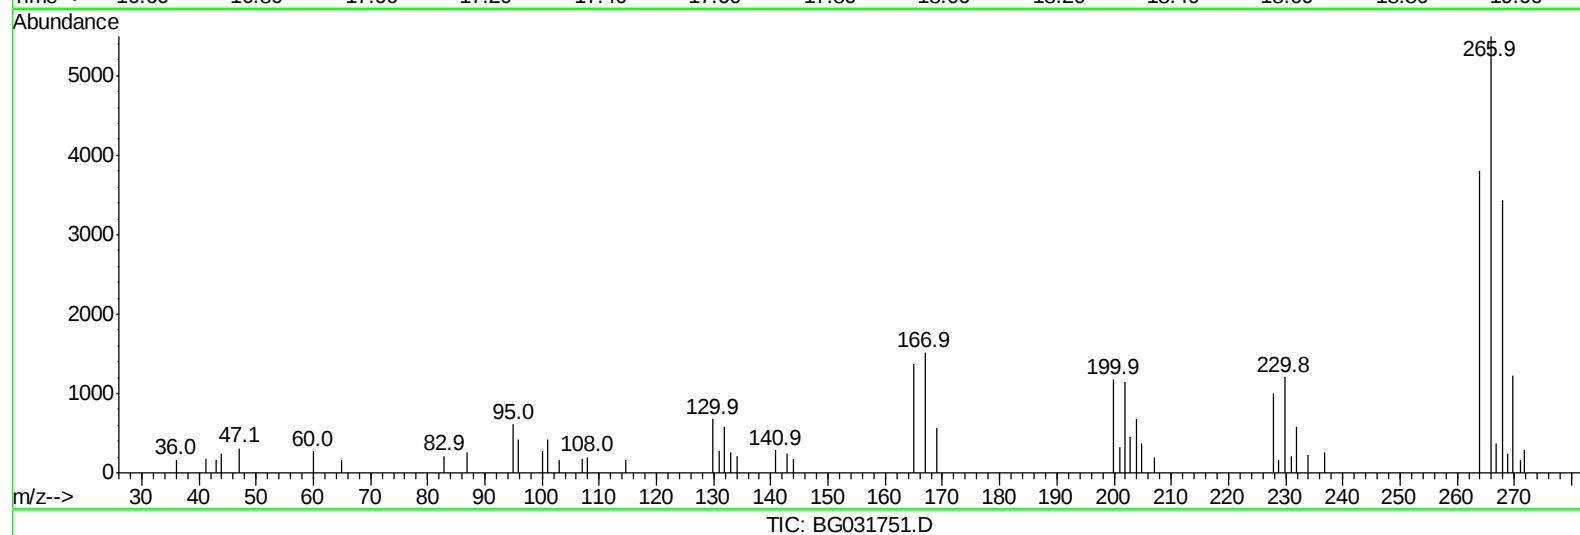


Data Path : Z:\HPCHEM1\BNA G\DATA\BG122217\
Data File : BG031751.D
Acq On : 23 Dec 2017 16:26
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 01:12:43 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 11:08:55 2017
Response via : Initial Calibration

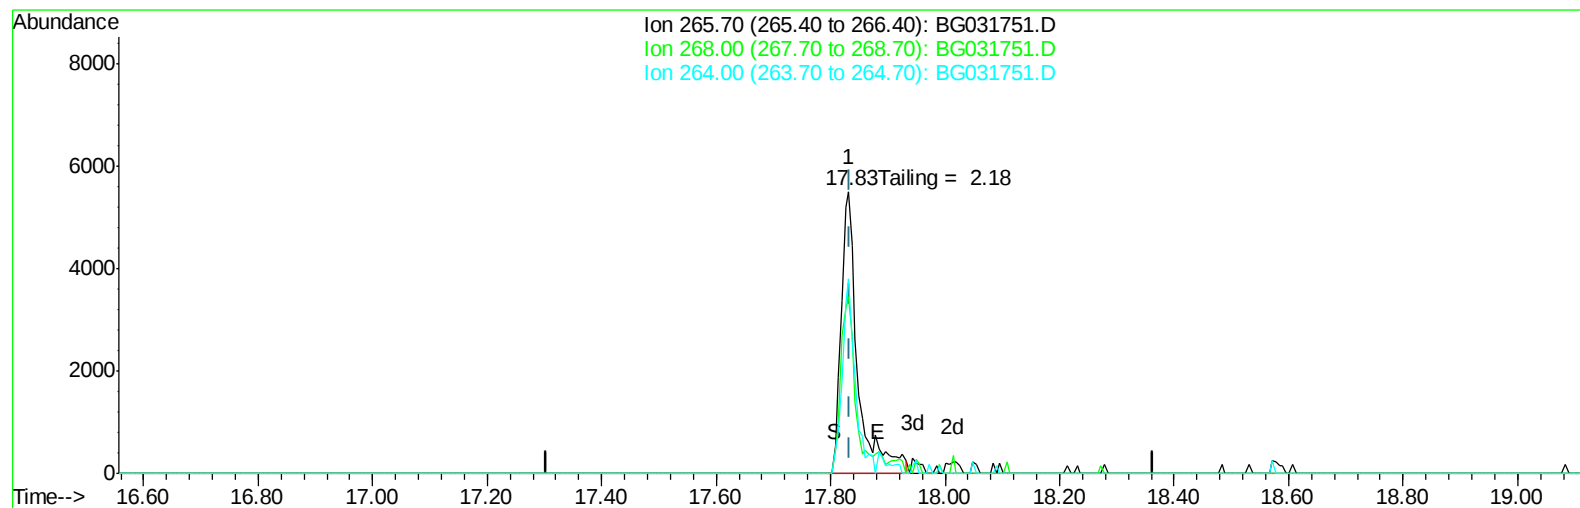

(69) Pentachlorophenol (C)



17.832min (-0.003) 2322.58ng

response 9824

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.56
264.00	62.00	69.24
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG122217\
 Data File : BG031751.D
 Acq On : 23 Dec 2017 16:26
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 01:12:43 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 22 11:08:55 2017
 Response via : Initial Calibration

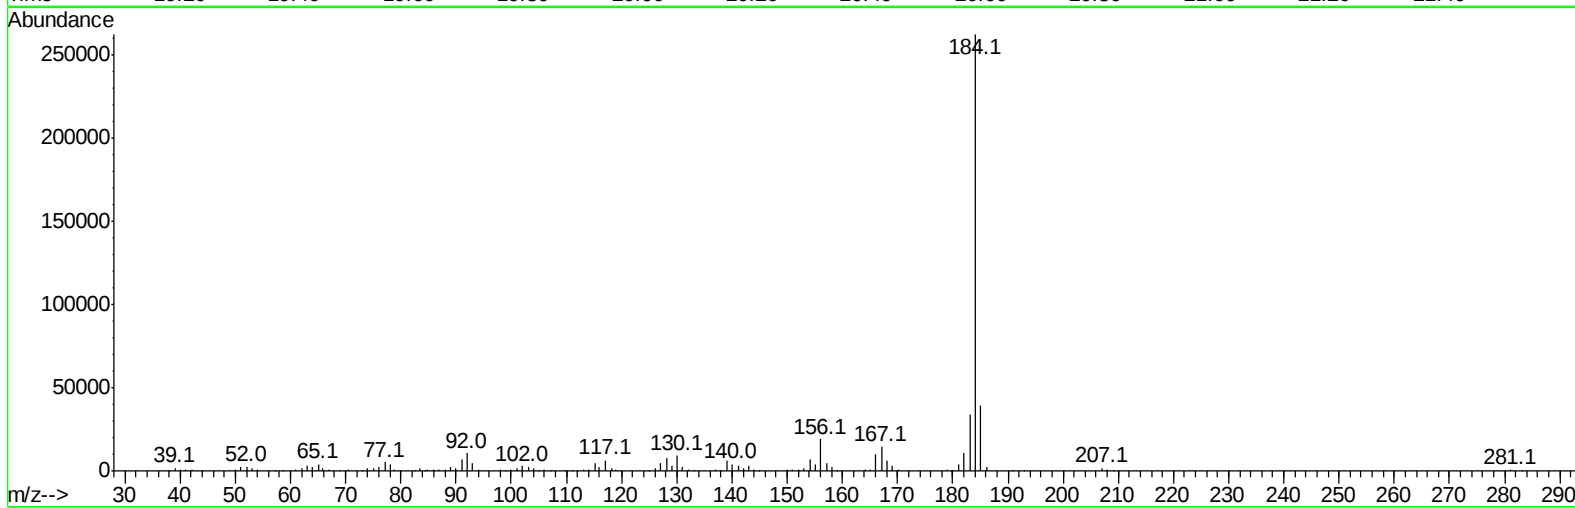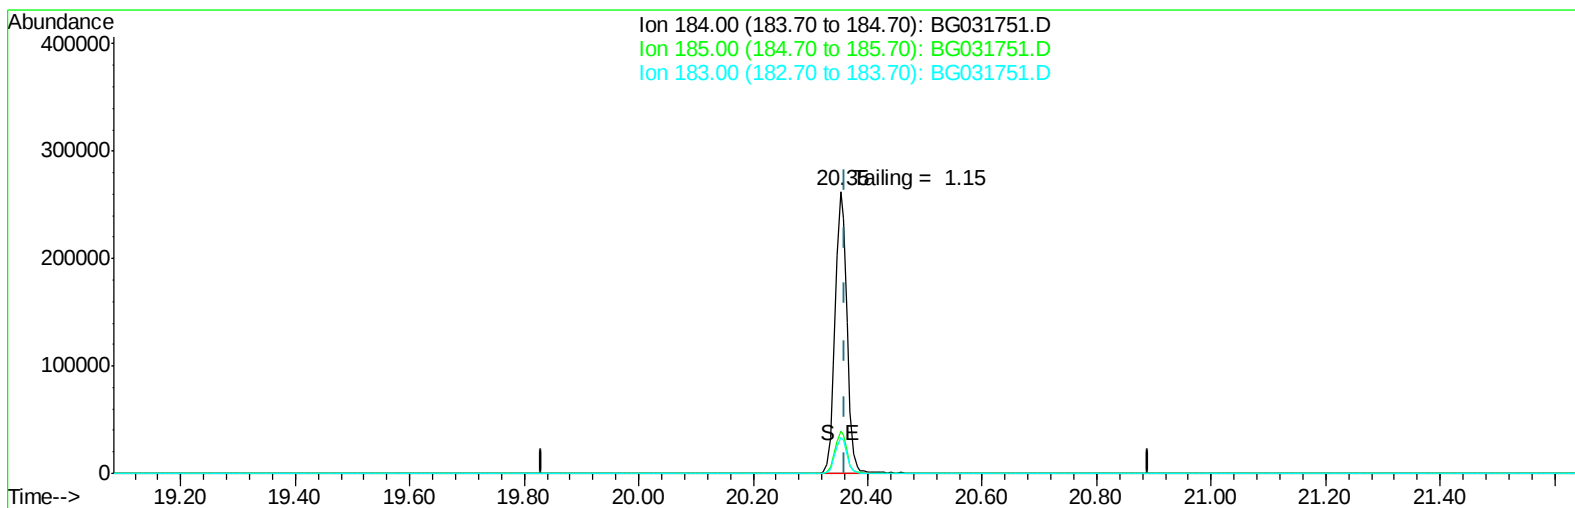

TIC: BG031751.D

(76) Benzidine

20.352min (-0.009) 220708.99ng

response 381487

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.90
183.00	13.30	12.94
0.00	0.00	0.00