


Data Path : Z:\HPCHEM1\BNA_G\Data\BG122217\
 Data File : BG031732.D
 Acq On : 23 Dec 2017 4:11
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 22 11:08:55 2017

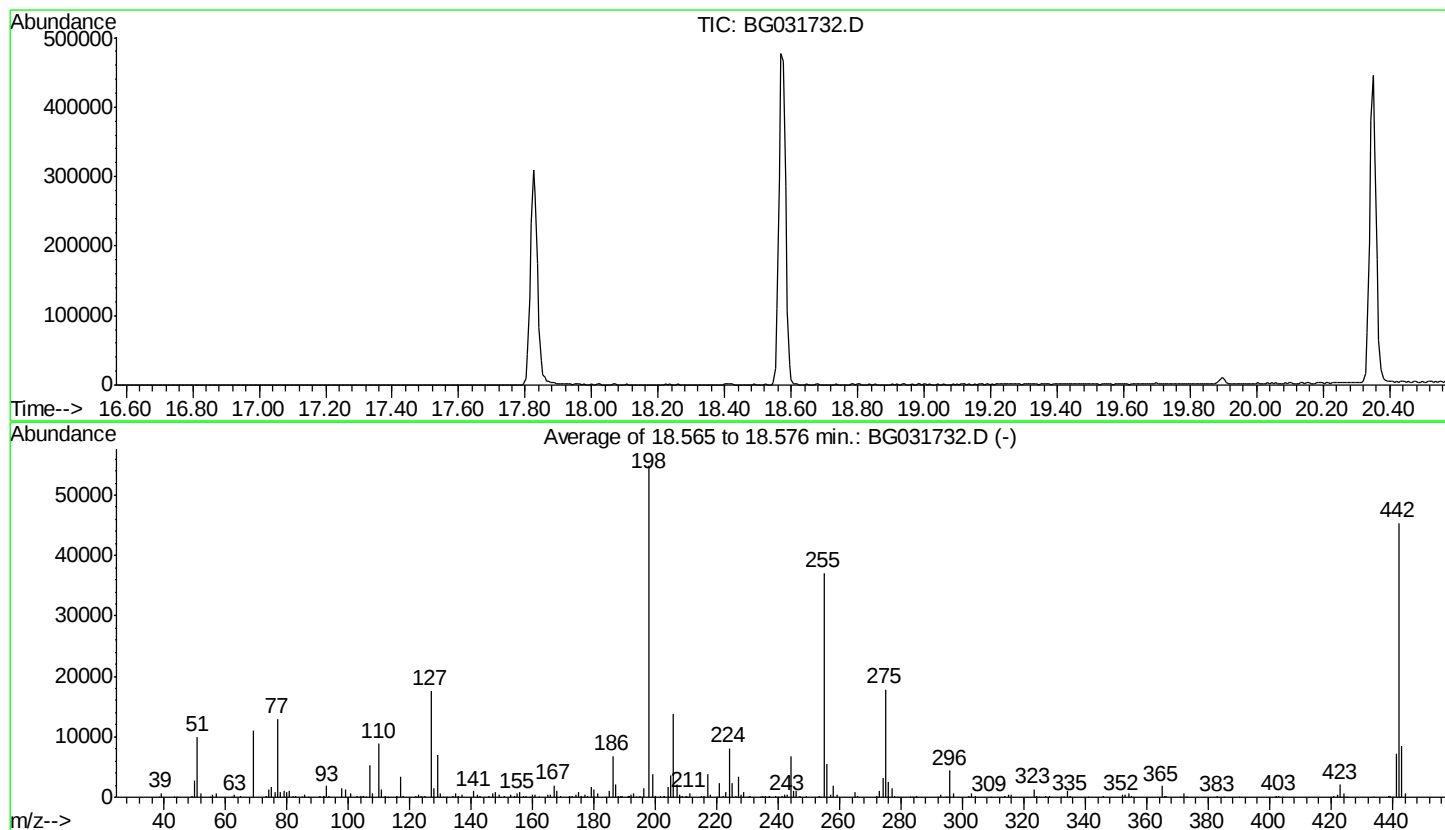

AutoFind: Scans 2600, 2601, 2602; Background Corrected with Scan 2594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.2	9982	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	20.1	11055	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.2	17644	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54869	PASS
199	198	5	9	7.0	3852	PASS
275	198	10	60	32.4	17796	PASS
365	198	1	100	3.5	1895	PASS
441	442	0.01	24	15.7	7126	PASS
442	198	50	100	82.6	45346	PASS
443	442	15	24	18.5	8376	PASS