


Data Path : Z:\HPCHEM1\BNA_G\Data\BG122217\
 Data File : BG031751.D
 Acq On : 23 Dec 2017 16:26
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 22 11:08:55 2017

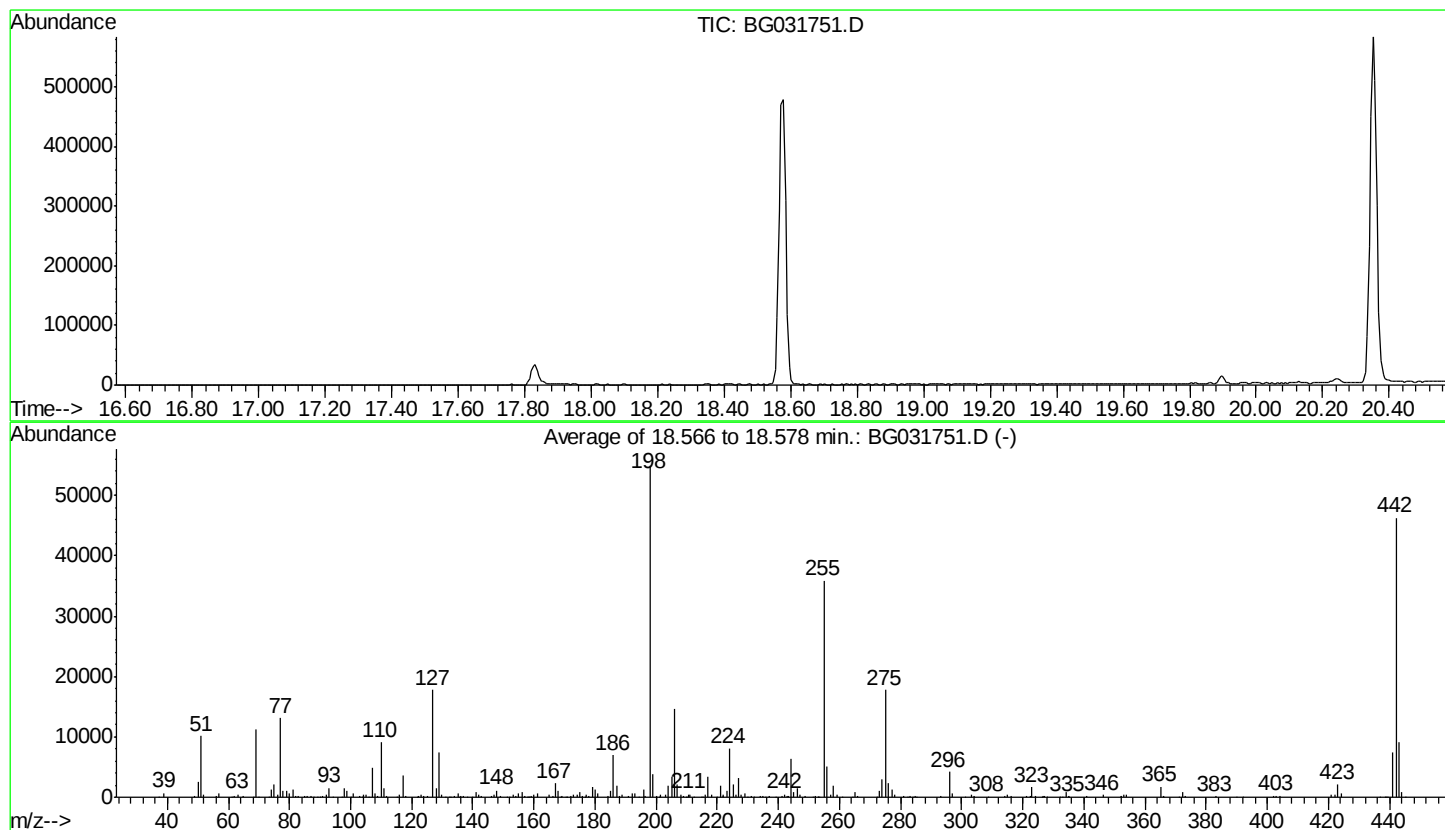

AutoFind: Scans 2600, 2601, 2602; Background Corrected with Scan 2593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.4	10097	PASS
68	69	0.00	2	0.9	100	PASS
69	198	0.00	100	20.4	11208	PASS
70	69	0.00	2	0.5	51	PASS
127	198	10	80	32.3	17738	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54930	PASS
199	198	5	9	6.9	3772	PASS
275	198	10	60	32.3	17744	PASS
365	198	1	100	3.1	1719	PASS
441	442	0.01	24	15.8	7325	PASS
442	198	50	100	84.2	46277	PASS
443	442	15	24	19.6	9050	PASS