
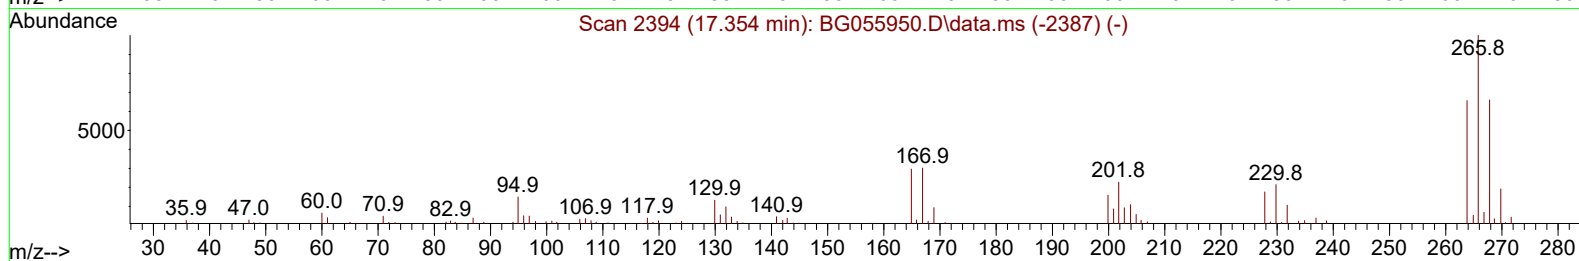
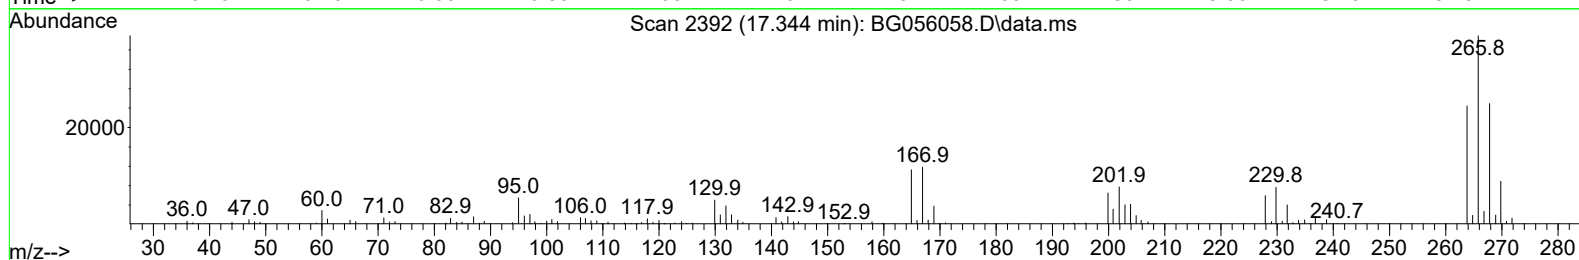


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122222\
Data File : BG056058.D
Acq On : 22 Dec 2022 10:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 08:34:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 05:09:54 2022
Response via : Initial Calibration

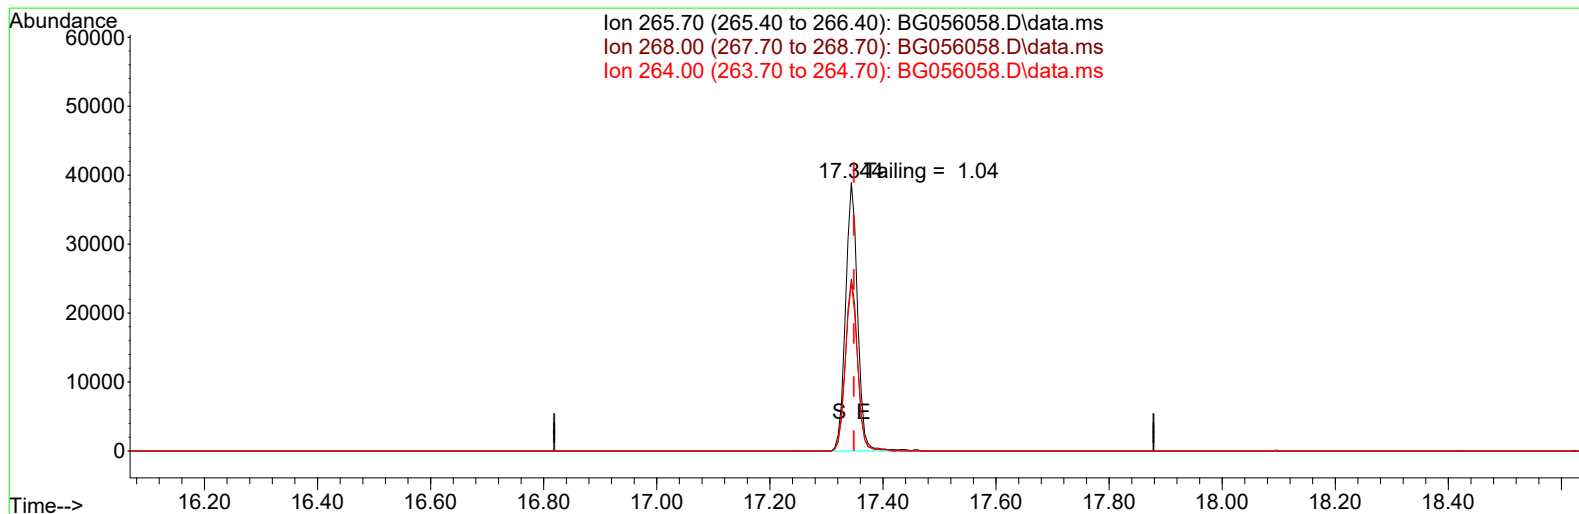

TIC: BG056058.D\data.ms

(70) Pentachlorophenol (C)




17.344min (-0.004) 40517.16 ng

response 57276

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.40	64.04
264.00	65.70	62.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122222\
Data File : BG056058.D
Acq On : 22 Dec 2022 10:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 08:34:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 05:09:54 2022
Response via : Initial Calibration

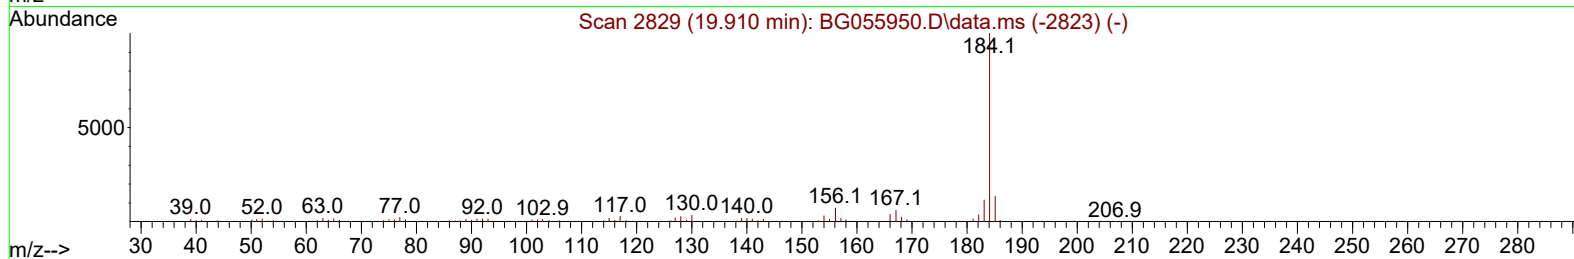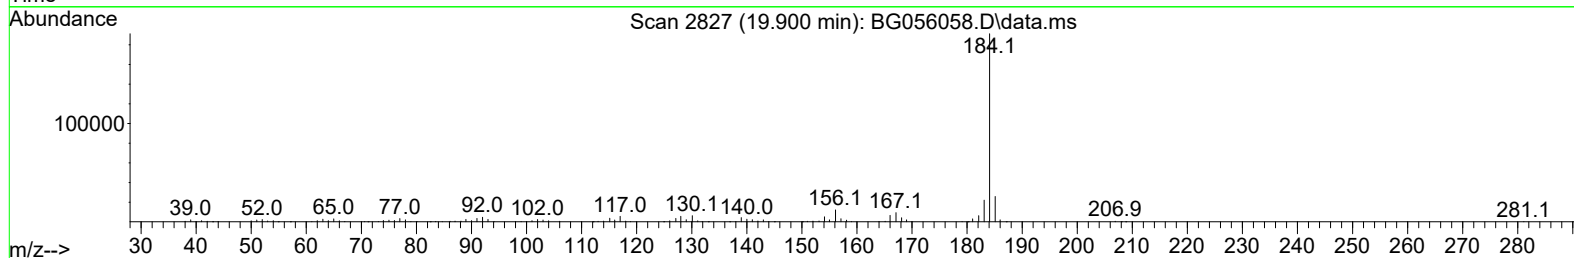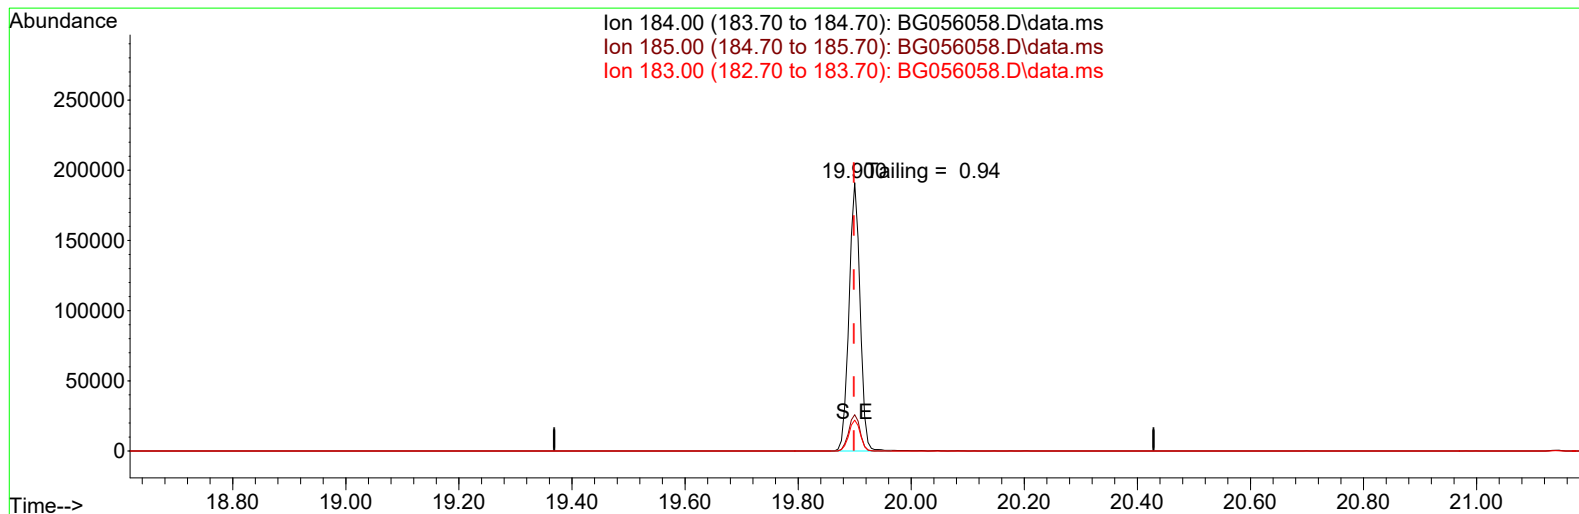

TIC: BG056058.D\data.ms

(77) Benzidine**19.900min (+ 0.002) 0.00 ng****response 259369**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.53
183.00	11.50	11.54
0.00	0.00	0.00