
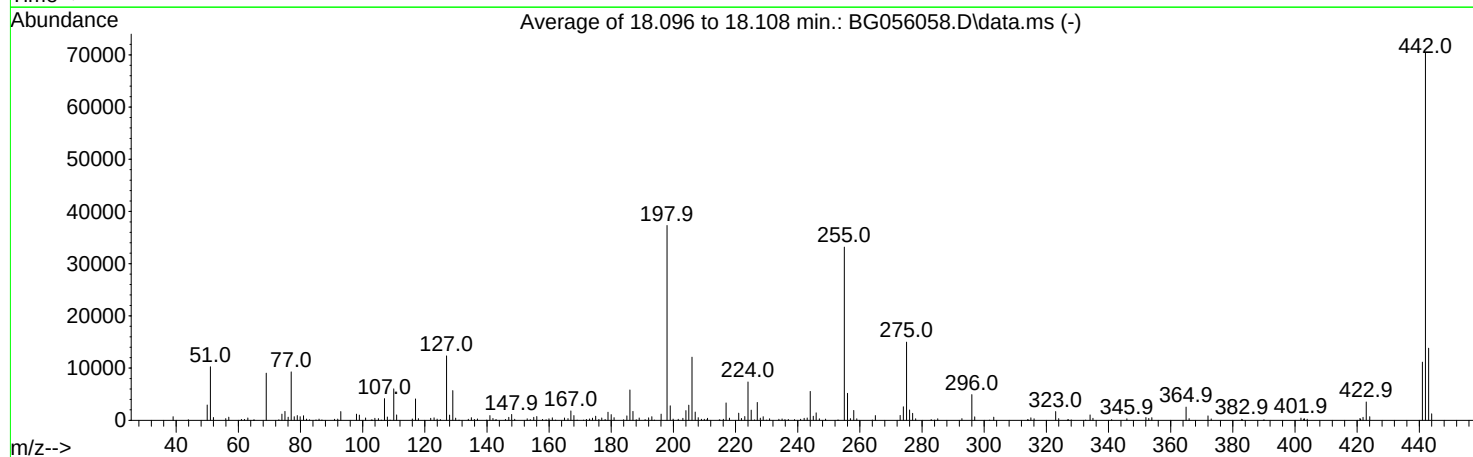


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122222\
 Data File : BG056058.D
 Acq On : 22 Dec 2022 10:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 23 05:09:54 2022

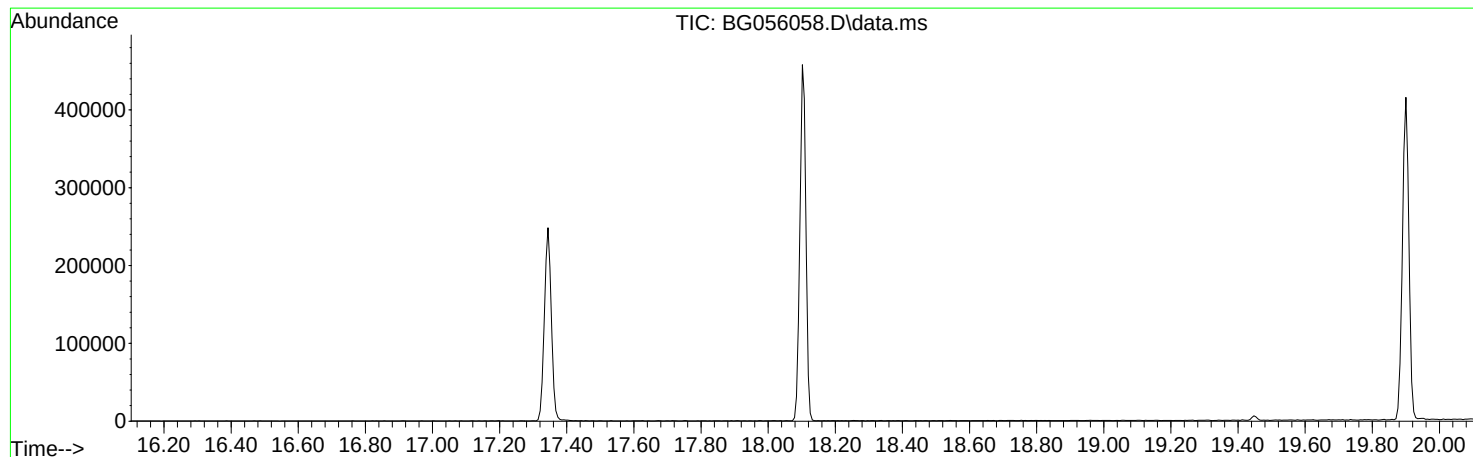




AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.5	10243	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	24.2	9015	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.0	12326	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	37304	PASS
199	198	5	9	7.4	2772	PASS
275	198	10	60	40.2	14986	PASS
365	198	1	100	6.8	2524	PASS
441	198	0.01	100	29.8	11133	PASS
442	442	50	100	100.0	70467	PASS
443	442	15	24	19.6	13823	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122222\
Data File : BG056058.D
Acq On : 22 Dec 2022 10:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 23 08:34:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 05:09:54 2022
Response via : Initial Calibration

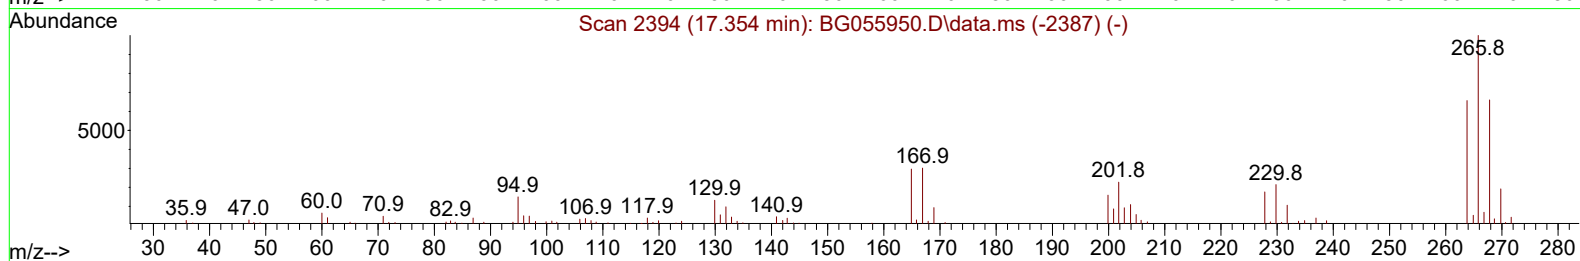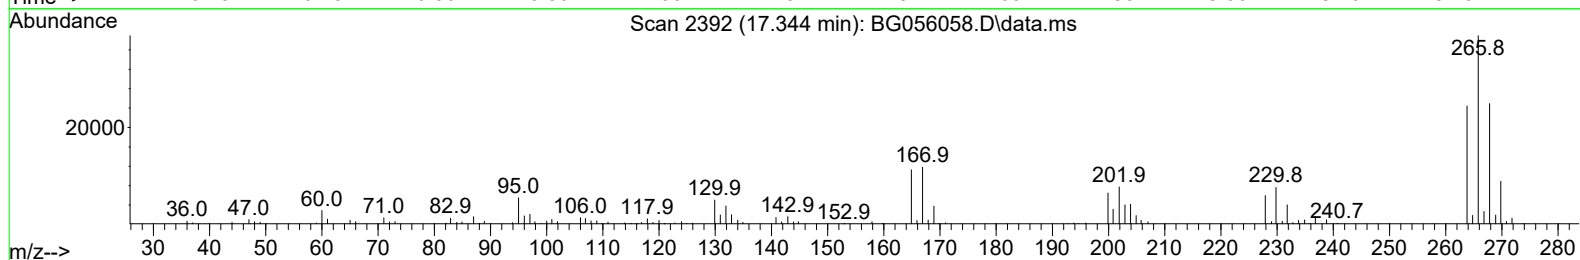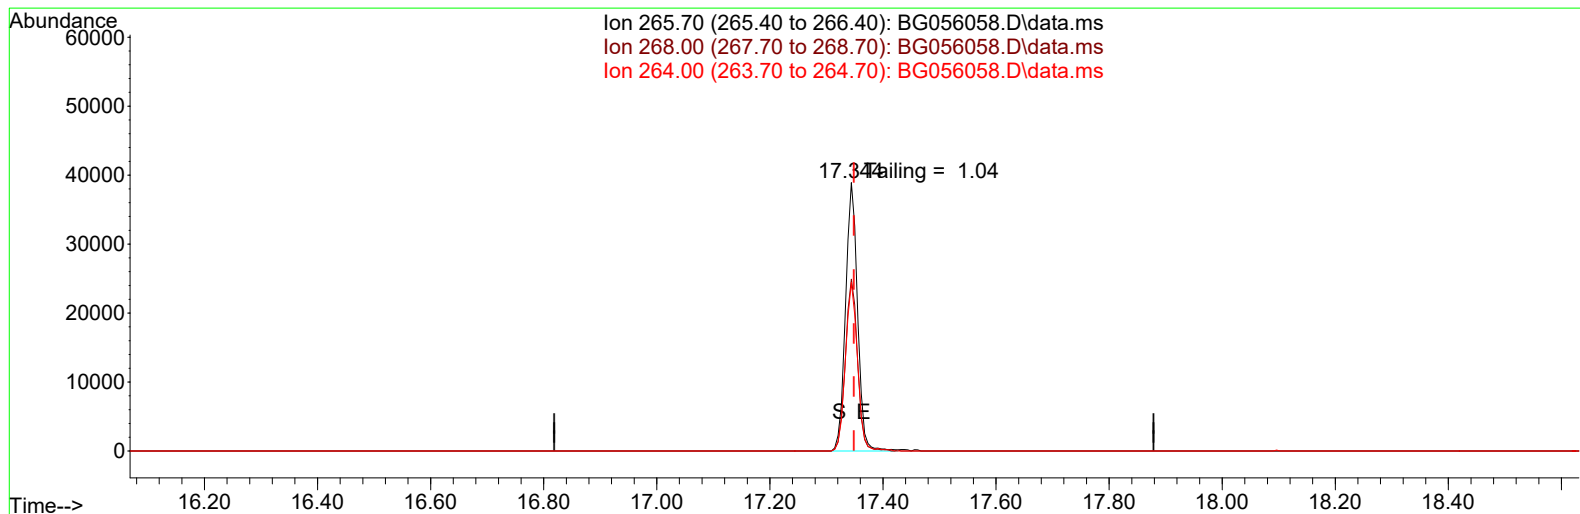

TIC: BG056058.D\data.ms

(70) Pentachlorophenol (C)

17.344min (-0.004) 40517.16 ng




response 57276

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.40	64.04
264.00	65.70	62.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122222\
Data File : BG056058.D
Acq On : 22 Dec 2022 10:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 23 08:34:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 05:09:54 2022
Response via : Initial Calibration

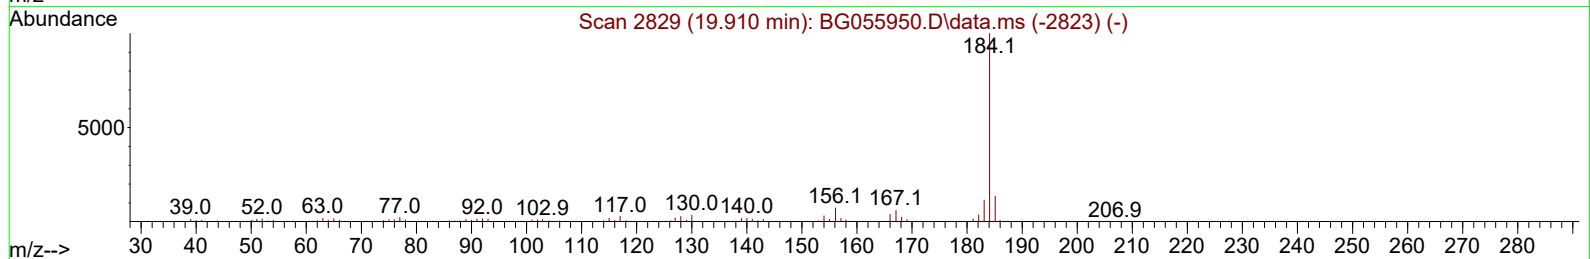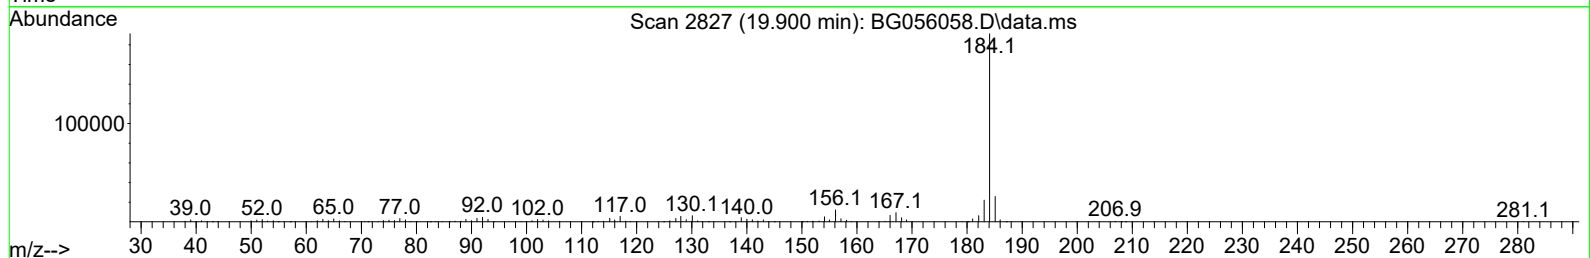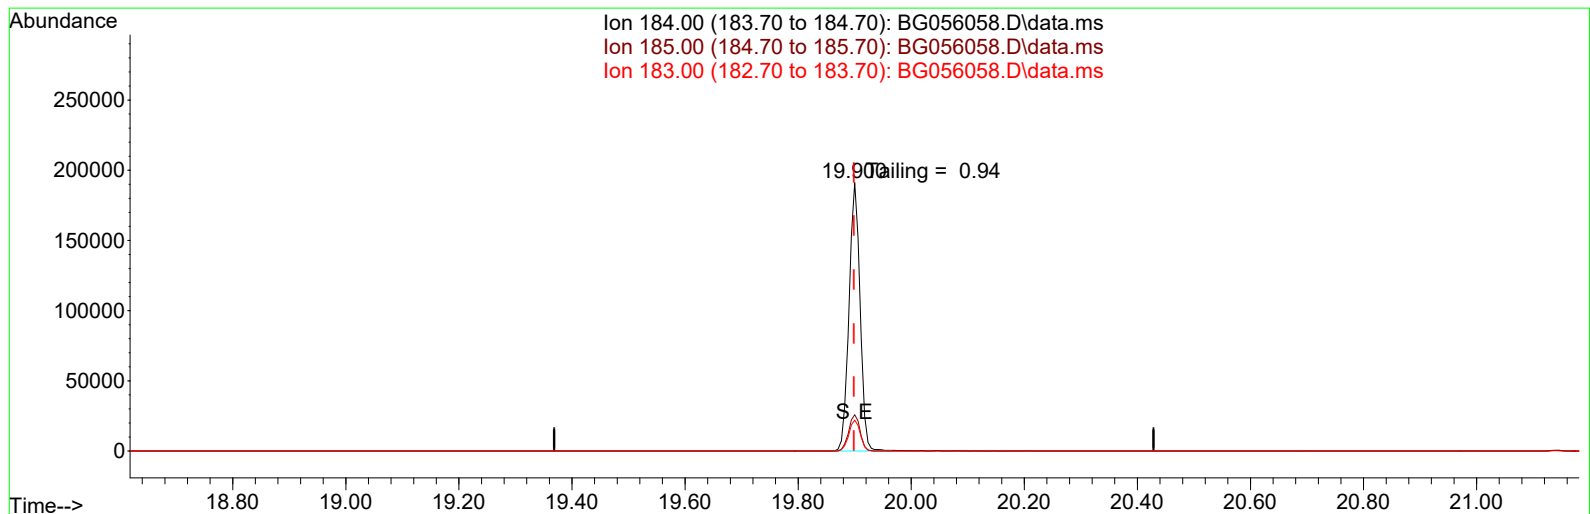

TIC: BG056058.D\data.ms

(77) Benzidine

19.900min (+ 0.002) 0.00 ng

response 259369

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.53
183.00	11.50	11.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/22/2022	BNA_G	BG056058.D
Compound Name	Response	Retention Time
DDT	143116	21.14
DDD	4273	20.681
DDE	0	20.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4273	147389	2.90

Instrument :
BNA_G
ClientSampleId :
DFTPP