
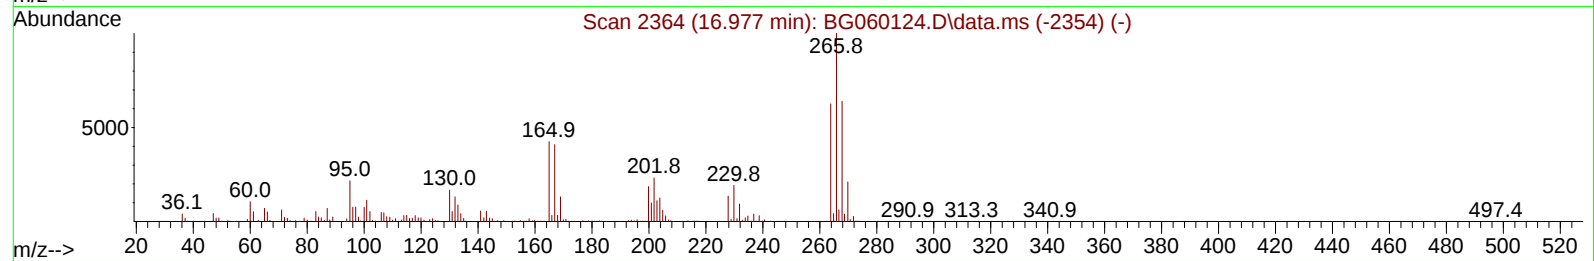
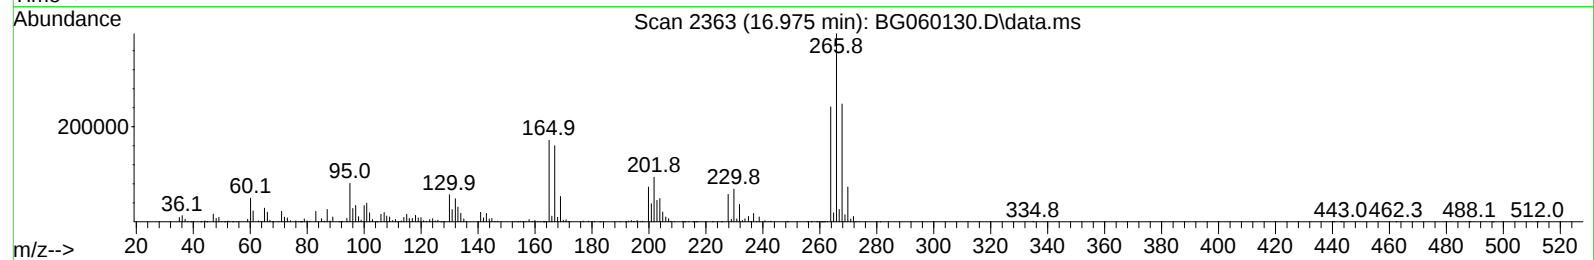


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122223\  
Data File : BG060130.D  
Acq On    : 22 Dec 2023    8:45  
Operator  : MA/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Dec 22 10:10:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 03:42:04 2023
Response via : Initial Calibration

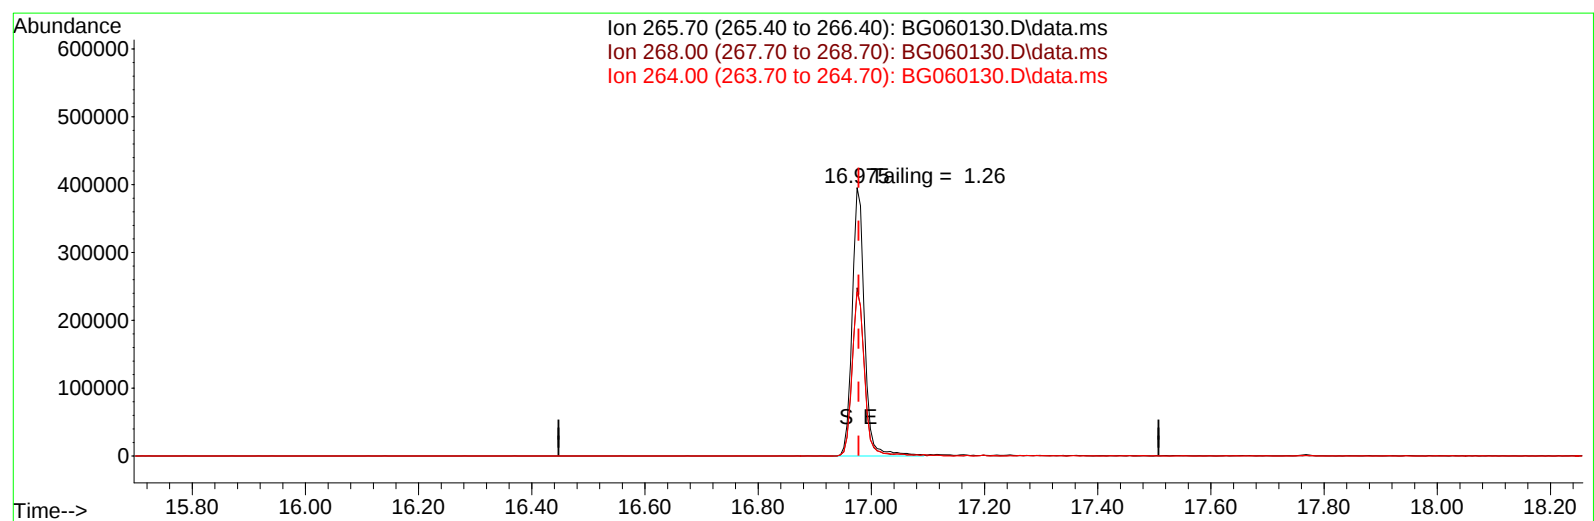

TIC: BG060130.D\data.ms

(70) Pentachlorophenol (C)




16.975min (-0.002) 23920.88 ng

response 600367

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.80	62.65
264.00	62.50	61.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122223\
Data File : BG060130.D
Acq On : 22 Dec 2023 8:45
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 10:10:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 03:42:04 2023
Response via : Initial Calibration

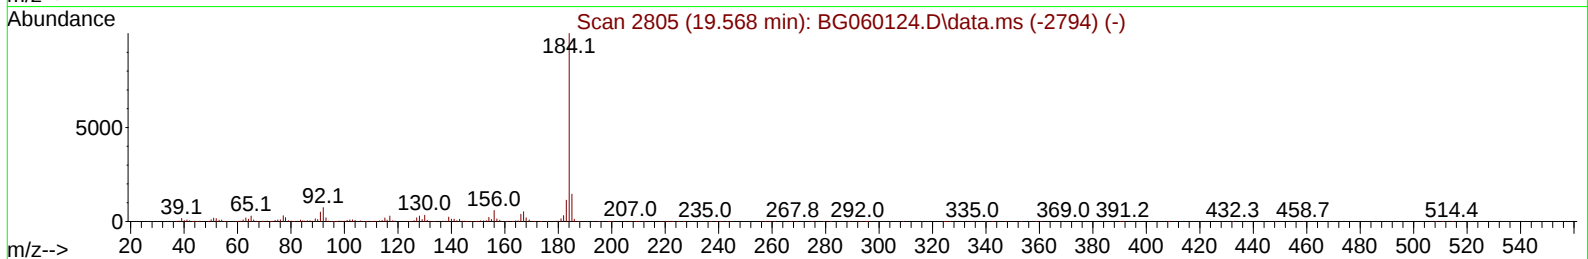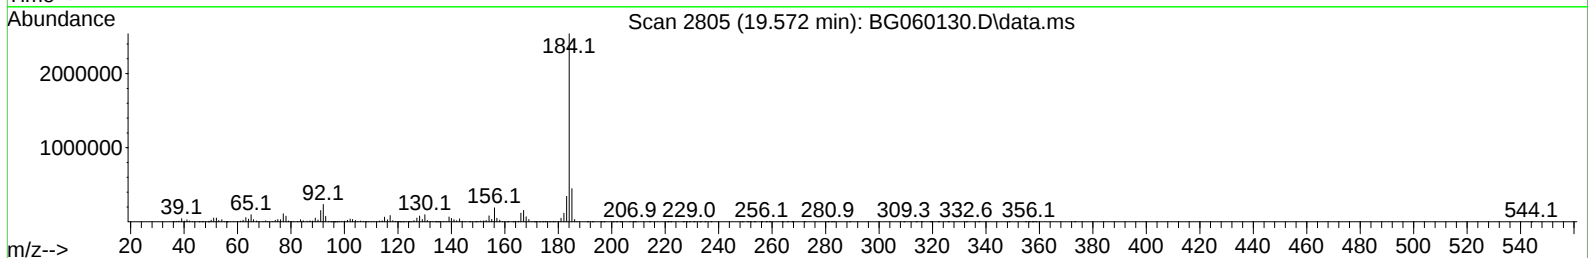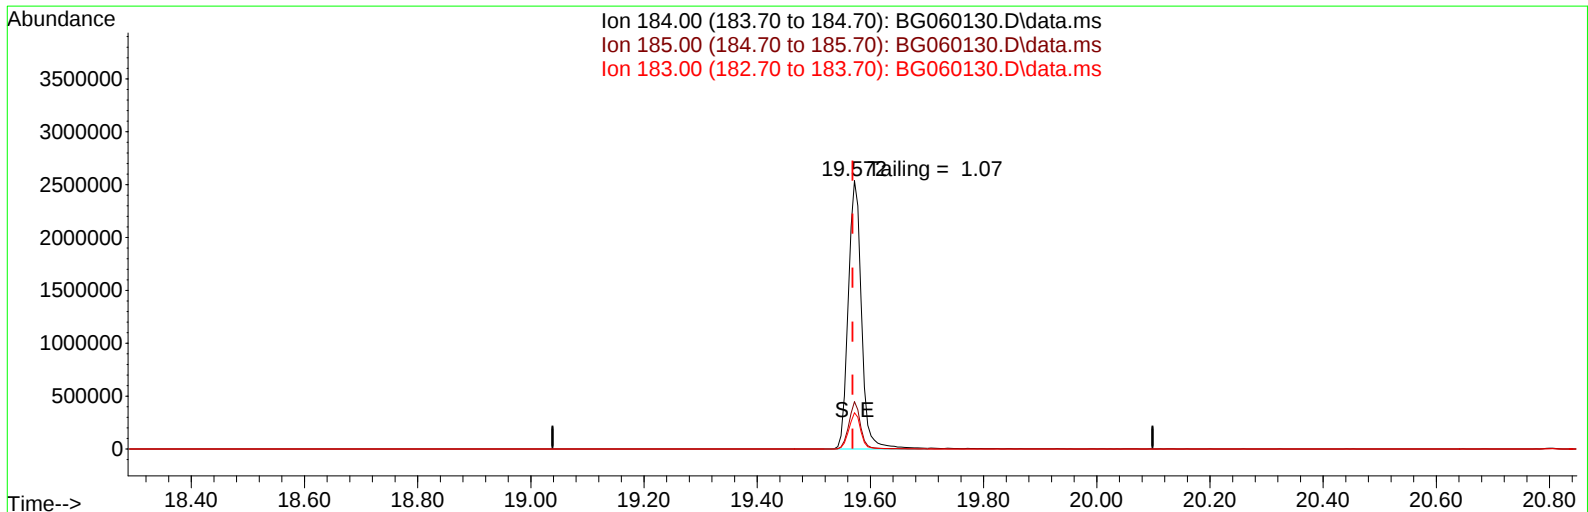

TIC: BG060130.D\data.ms

(77) Benzidine**19.572min (+ 0.003) 321698.43 ng****response 4114112**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	17.65#
183.00	11.30	13.55
0.00	0.00	0.00