
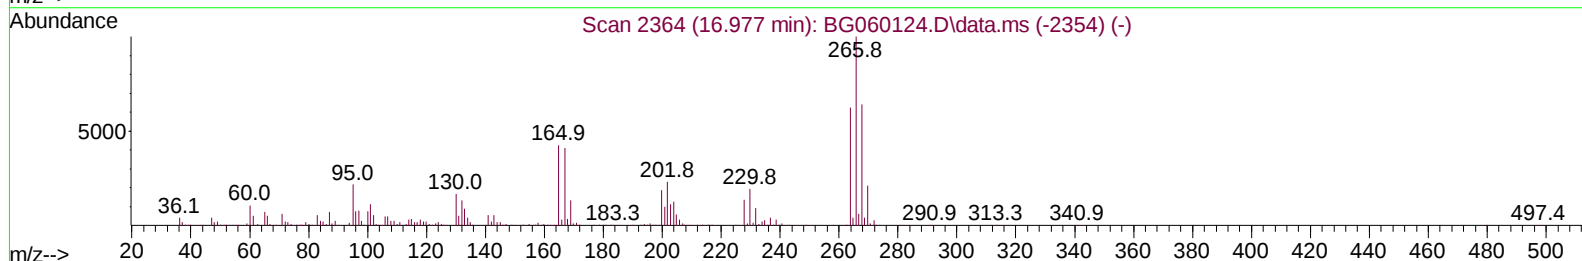
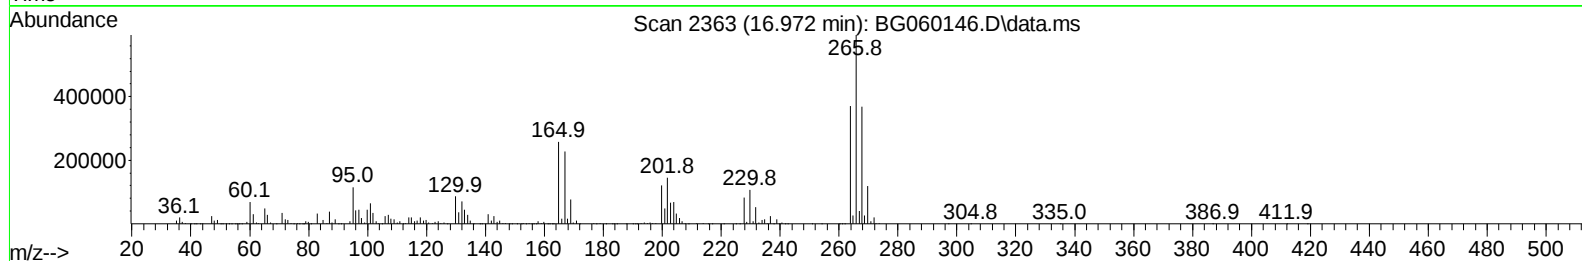


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122223\  
Data File : BG060146.D  
Acq On : 22 Dec 2023 20:54  
Operator : MA/JU  
Sample : DFTTP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 06:04:57 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 22 03:42:04 2023  
Response via : Initial Calibration

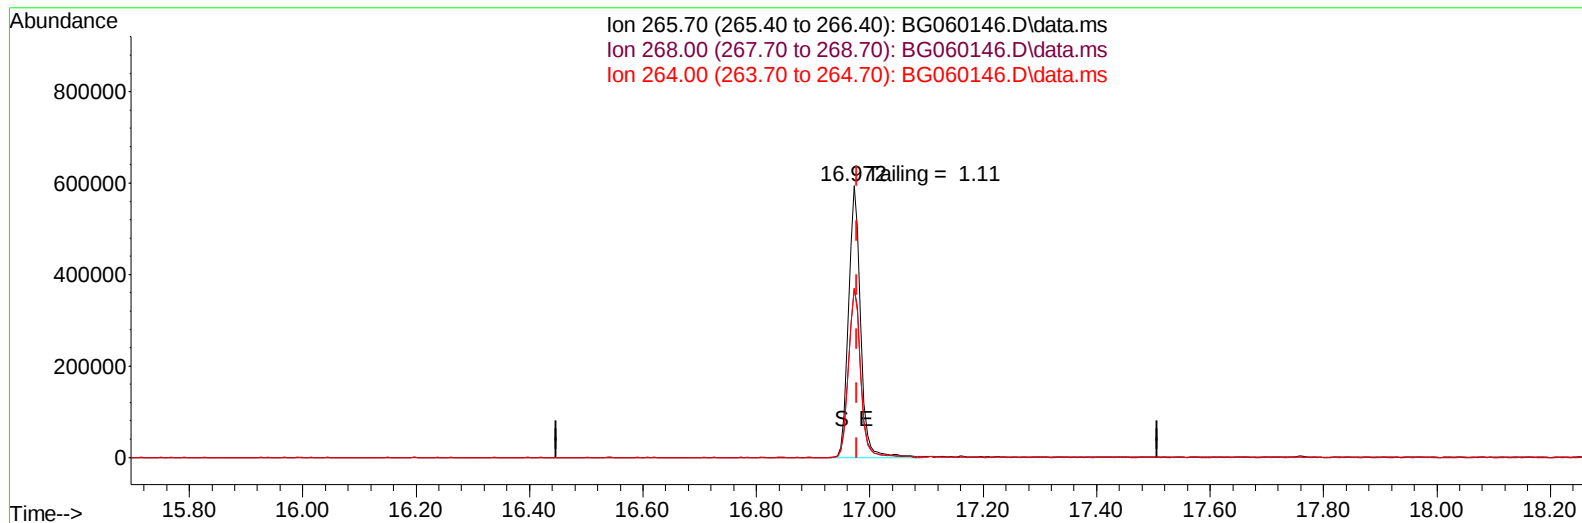

TIC: BG060146.D\data.ms

**(70) Pentachlorophenol (C)**




**16.972min (-0.005) 608348.68 ng**

**response 881648**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 67.80  | 66.44  |
| 264.00 | 62.50  | 62.42  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122223\  
Data File : BG060146.D  
Acq On : 22 Dec 2023 20:54  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 06:04:57 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 22 03:42:04 2023  
Response via : Initial Calibration

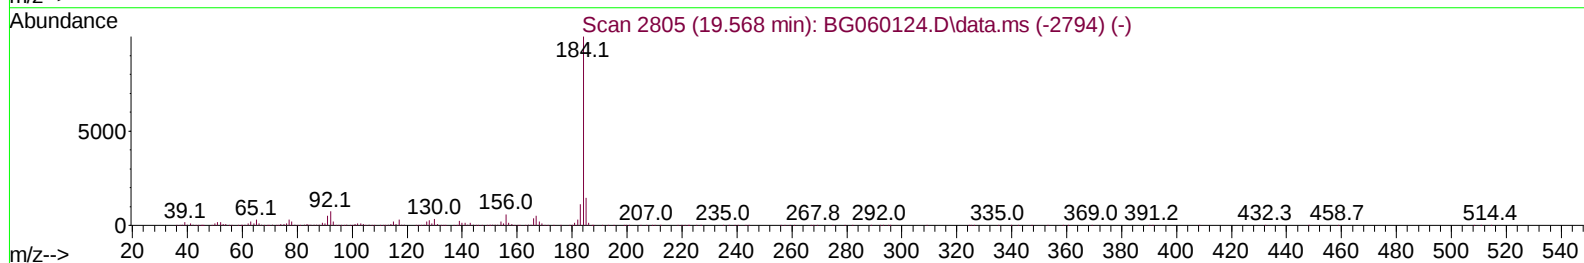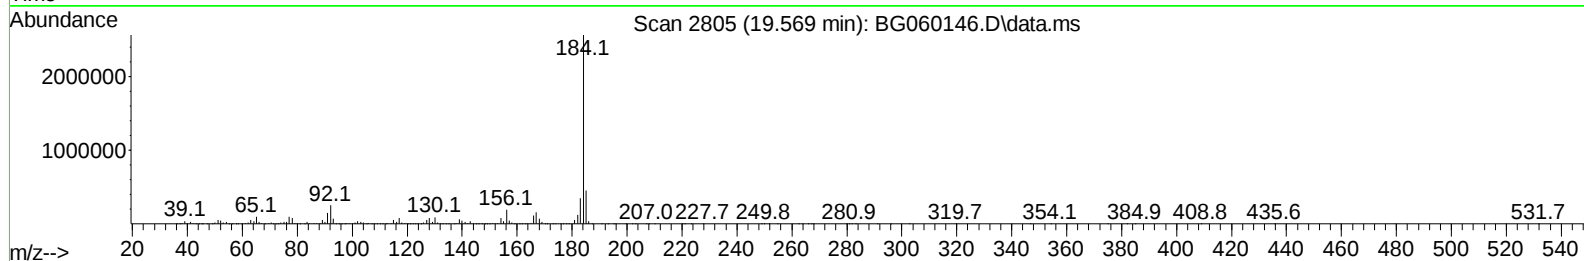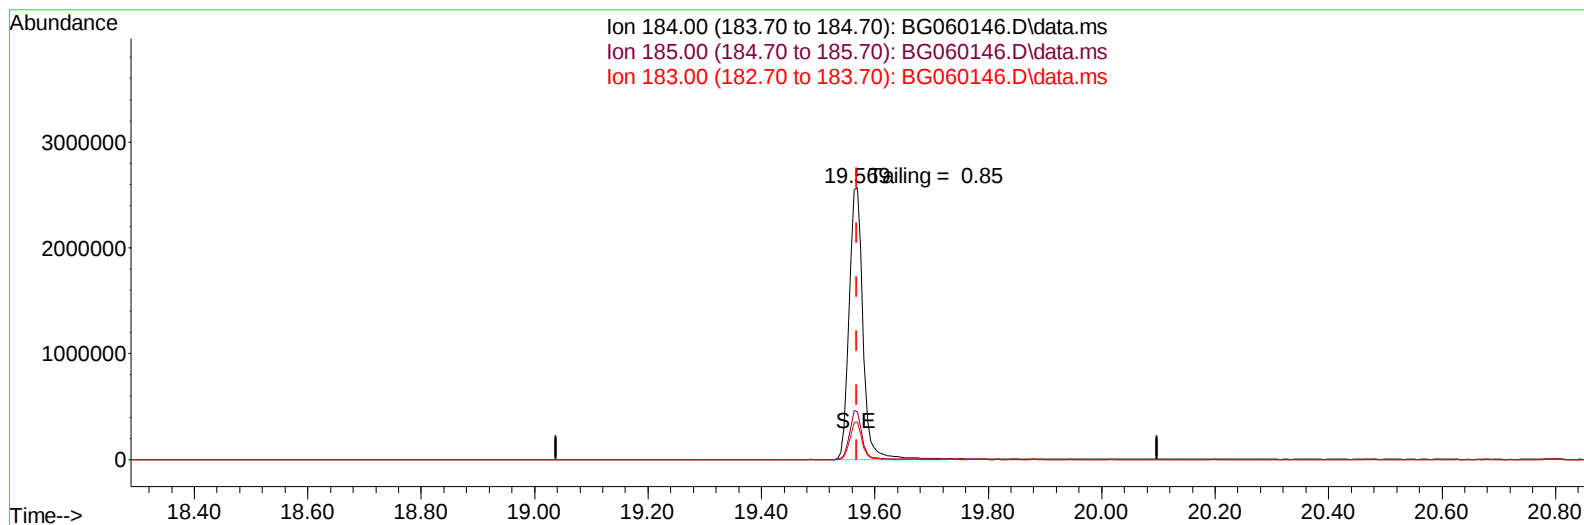

TIC: BG060146.D\data.ms

**(77) Benzidine****19.569min (+ 0.001) 191515.68 ng****response 4385850**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.60  | 17.54# |
| 183.00 | 11.30  | 13.74# |
| 0.00   | 0.00   | 0.00   |