

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122223\
 Data File : BG060132.D
 Acq On : 22 Dec 2023 10:47
 Operator : MA/JU
 Sample : PB157953BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB157953BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060132.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.514	405	413	429	rBV	3949144	6613437	27.79%	7.877%
2	7.106	675	684	706	rBV	4438567	7736669	32.51%	9.214%
3	7.941	819	826	839	rBV	577306	980993	4.12%	1.168%
4	9.104	1013	1024	1034	rBV	2546460	4482215	18.83%	5.338%
5	10.743	1296	1303	1313	rBV	873579	1561553	6.56%	1.860%
6	13.199	1714	1721	1735	rBV	7648645	12318324	51.76%	14.671%
7	14.574	1948	1955	1966	rBV	1816029	2878479	12.09%	3.428%
8	16.067	2201	2209	2232	rBV	6837776	10616743	44.61%	12.645%
9	17.324	2416	2423	2436	rBV	2919946	4349003	18.27%	5.180%
10	19.950	2863	2870	2882	rBV	16627944	23799720	100.00%	28.345%
11	21.590	3142	3149	3160	rBV	2904311	4685729	19.69%	5.581%
12	24.762	3680	3689	3703	rVB	1369813	3940153	16.56%	4.693%




Sum of corrected areas: 83963018

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122223\
Data File : BG060132.D
Acq On : 22 Dec 2023 10:47
Operator : MA/JU
Sample : PB157953BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

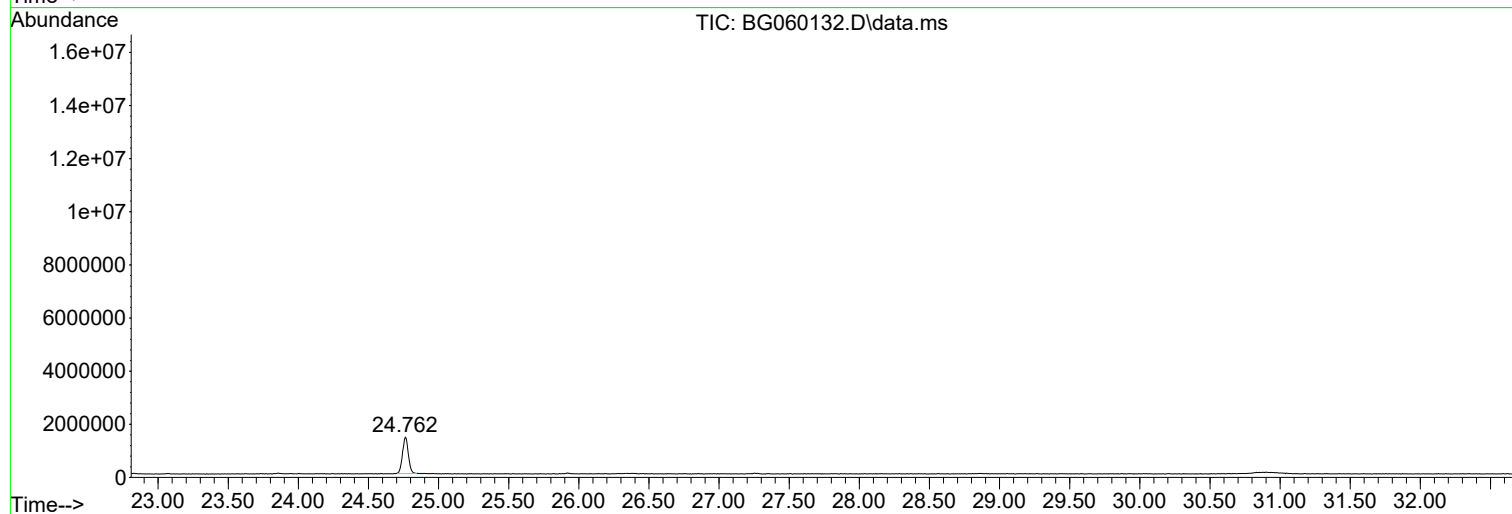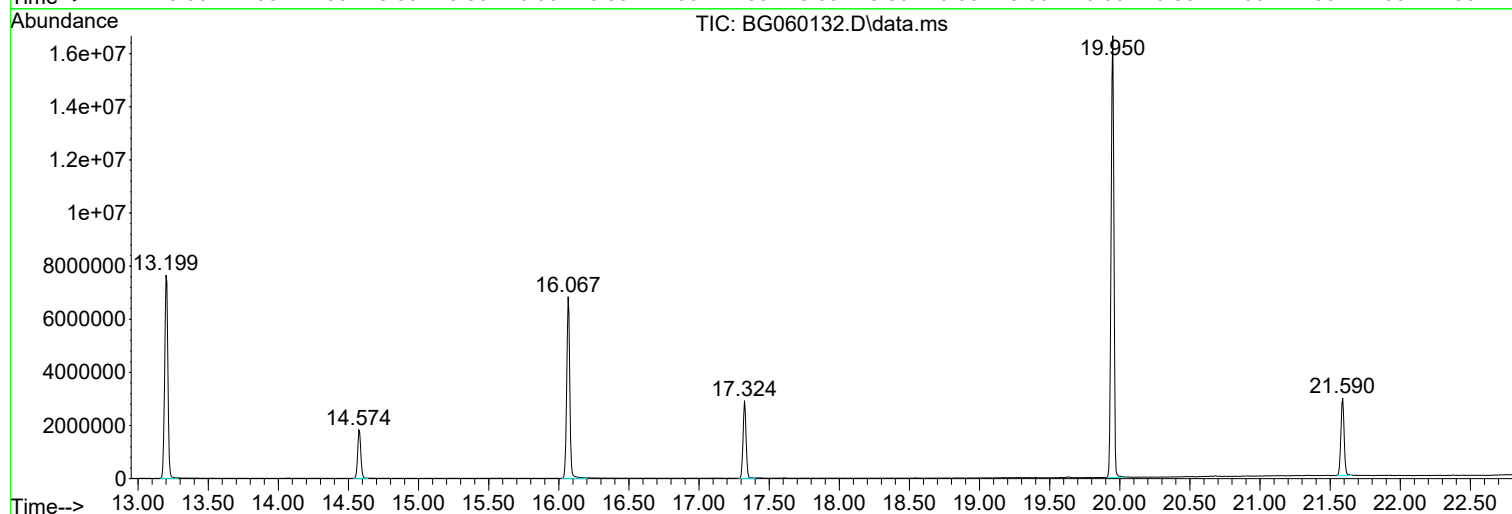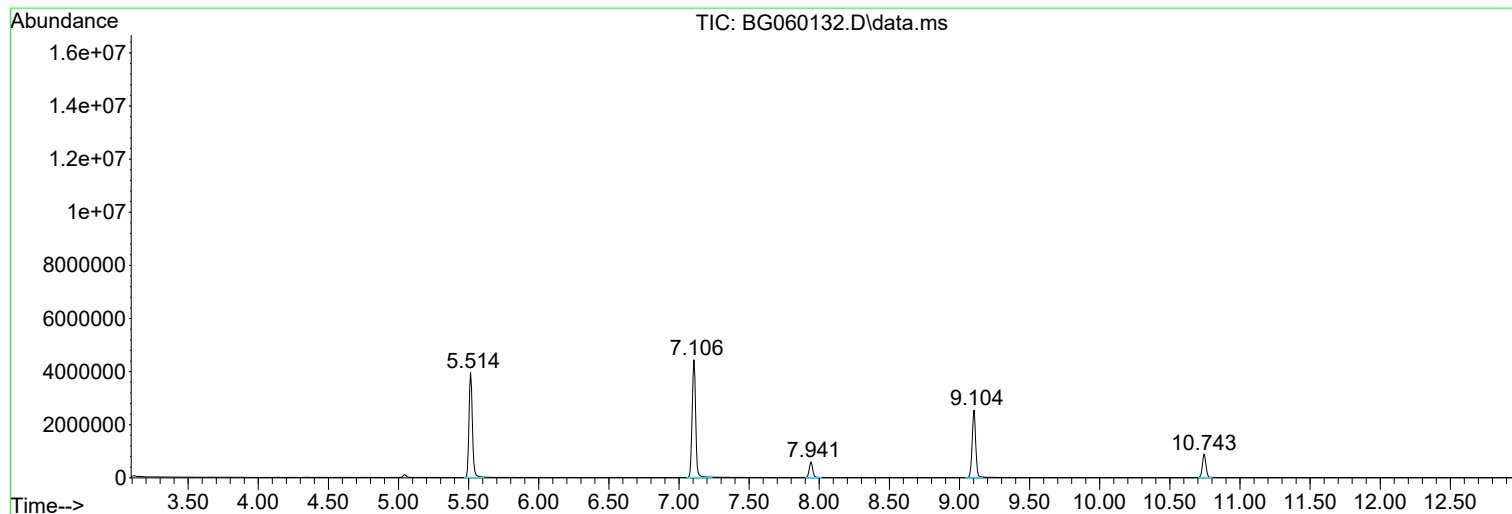

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122223\
Data File : BG060132.D
Acq On : 22 Dec 2023 10:47
Operator : MA/JU
Sample : PB157953BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122223\
Data File : BG060132.D
Acq On : 22 Dec 2023 10:47
Operator : MA/JU
Sample : PB157953BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB157953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------