
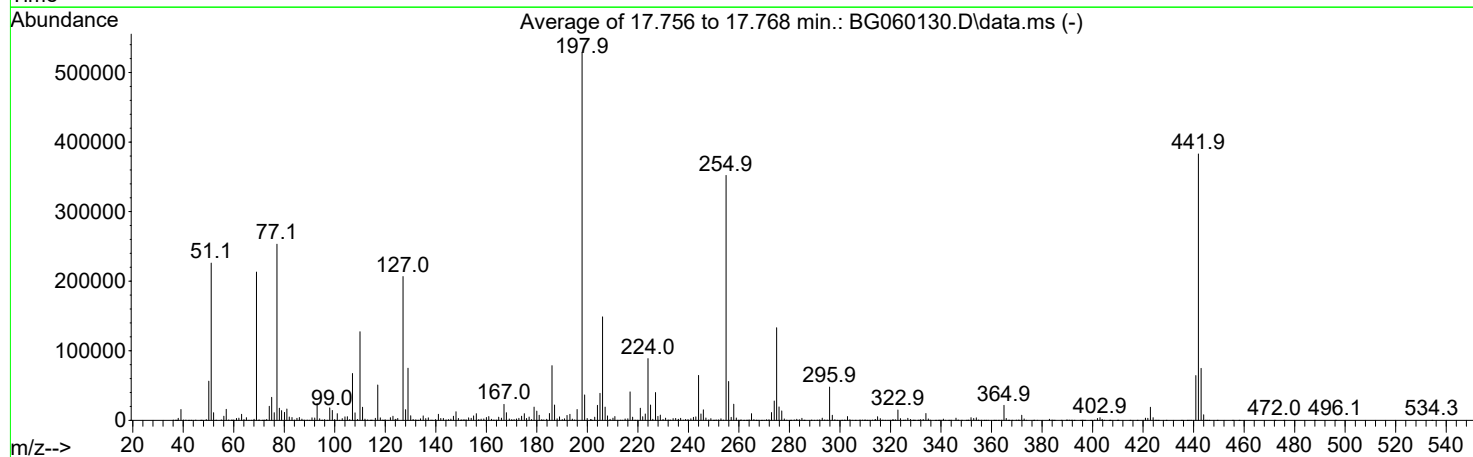


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122223\  
 Data File : BG060130.D  
 Acq On : 22 Dec 2023 8:45  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122123.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Dec 22 03:42:04 2023

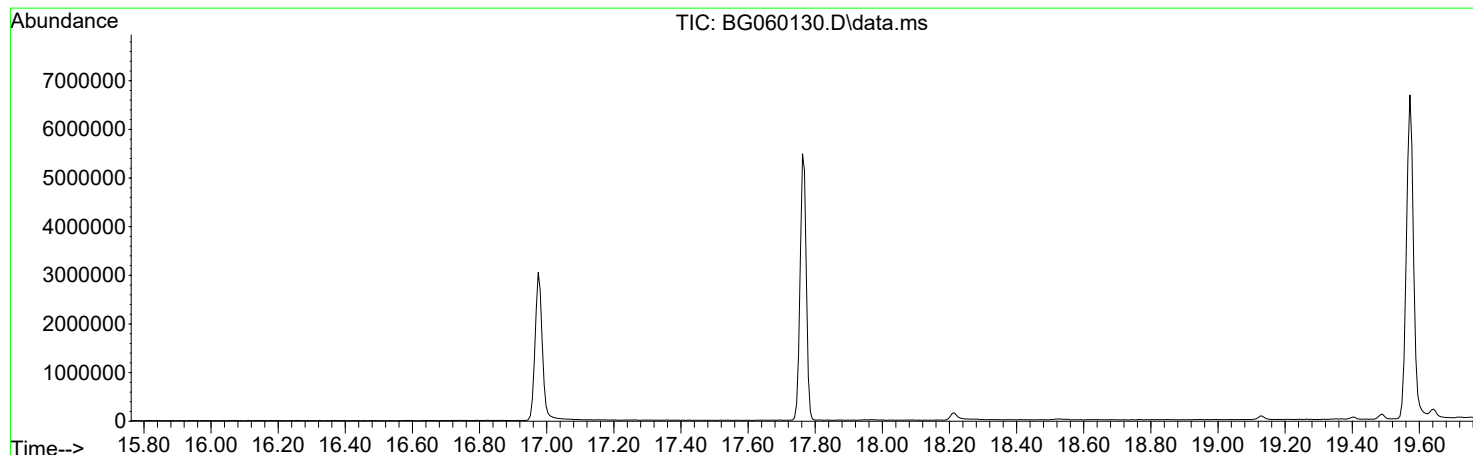

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	226027	PASS
68	69	0.00	2	0.8	1652	PASS
69	198	0.00	100	40.3	213119	PASS
70	69	0.00	2	0.3	636	PASS
127	198	10	80	39.1	206827	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	528704	PASS
199	198	5	9	6.9	36563	PASS
275	198	10	60	25.2	133165	PASS
365	198	1	100	4.1	21616	PASS
441	198	0.01	100	12.2	64536	PASS
442	442	50	100	100.0	382869	PASS
443	442	15	24	19.6	74877	PASS

**DDT Breakdown**




Date	Instrument Name	DFTPP Data File
12/22/2023	BNA_G	<u>BG060130.D</u>
Compound Name	Response	Retention Time
DDT	1905993	20.8
DDD	32643	20.412
DDE	555	19.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33198	1939191	1.71

Instrument :  
 BNA\_G  
 Client:Sampled :  
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122223\  
 Data File : BG060130.D  
 Acq On : 22 Dec 2023 8:45  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Quant Time: Dec 22 10:10:12 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122123.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Dec 22 03:42:04 2023  
 Response via : Initial Calibration

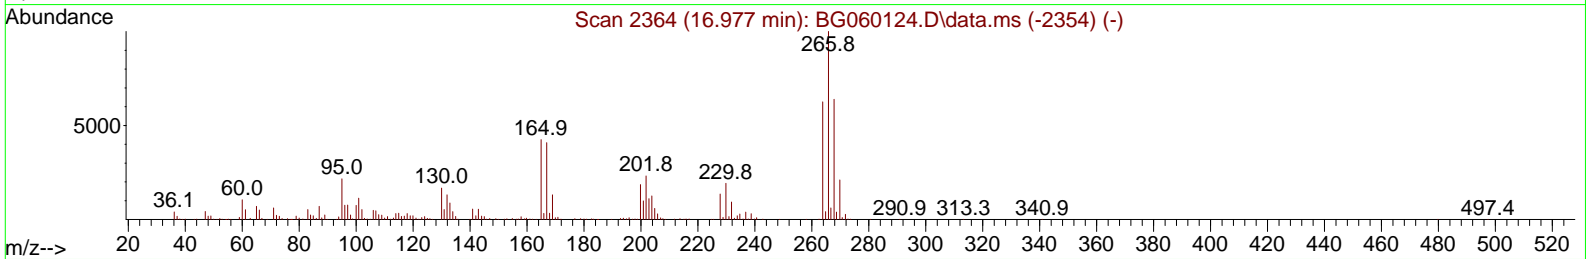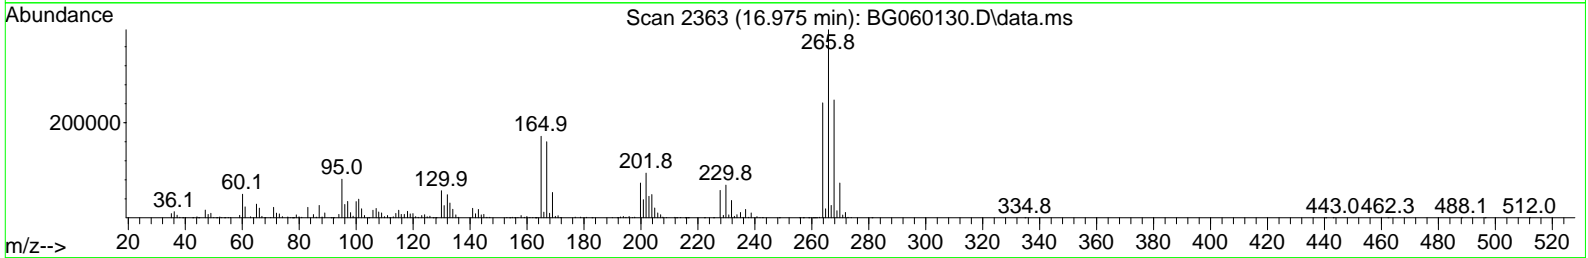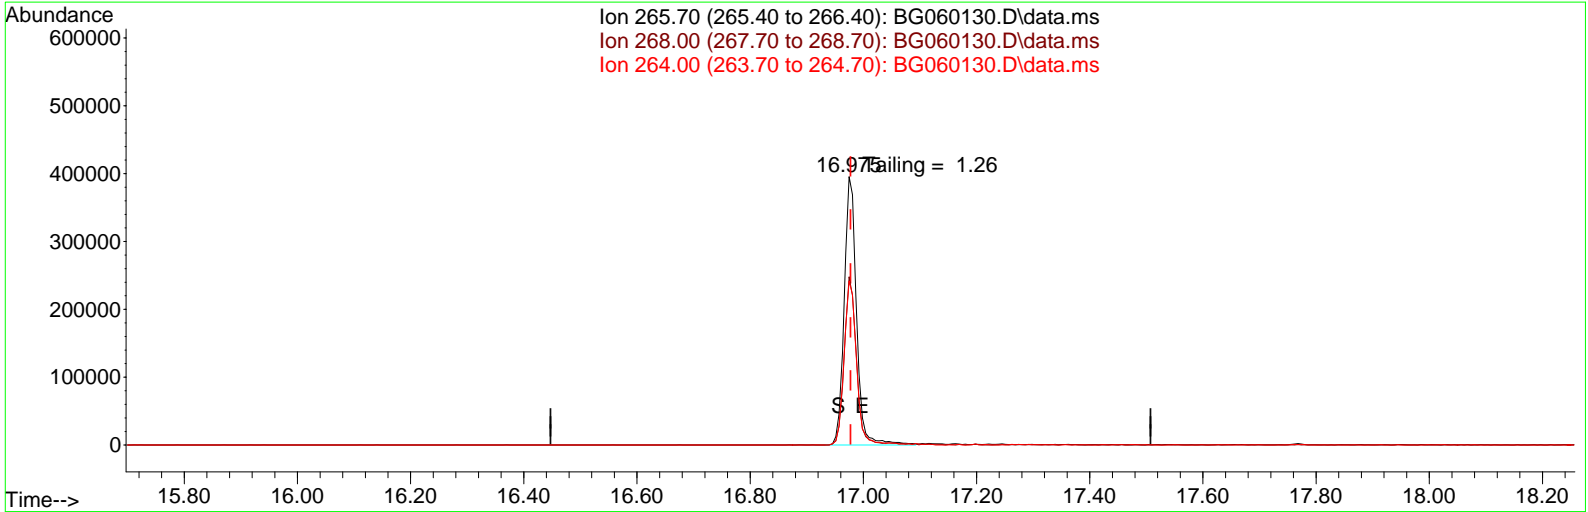

TIC: BG060130.D\data.ms

(70) Pentachlorophenol (C)

16.975min (-0.002) 23920.88 ng




response 600367

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.80	62.65
264.00	62.50	61.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG122223\  
 Data File : BG060130.D  
 Acq On : 22 Dec 2023 8:45  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 BNA\_G  
**ClientSampleId :**  
 DFTPP

Quant Time: Dec 22 10:10:12 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122123.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Dec 22 03:42:04 2023  
 Response via : Initial Calibration

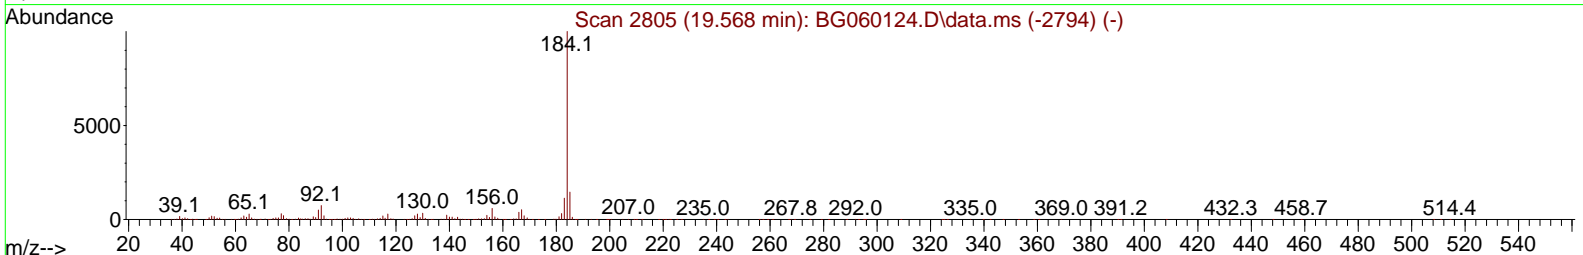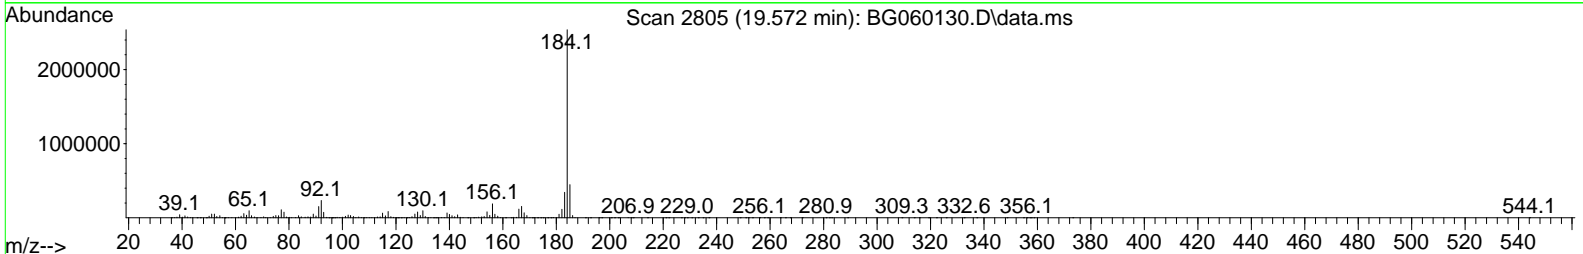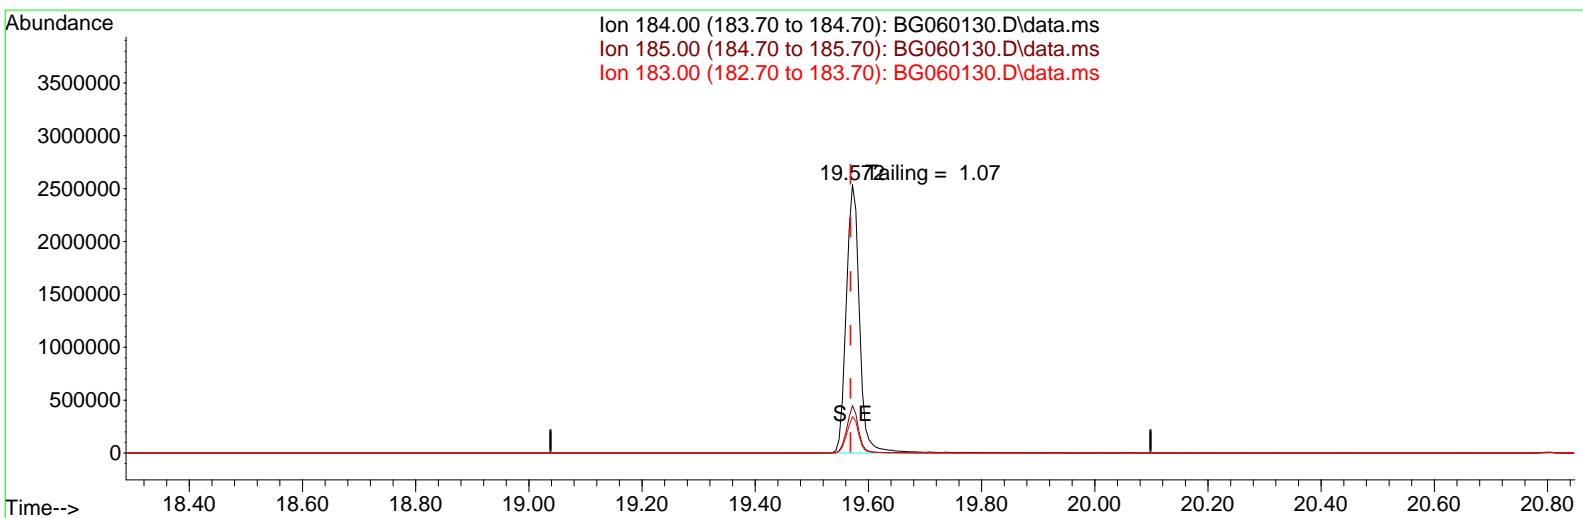

TIC: BG060130.D\data.ms

(77) Benzidine

19.572min (+ 0.003) 321698.43 ng

response 4114112

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	17.65#
183.00	11.30	13.55
0.00	0.00	0.00