
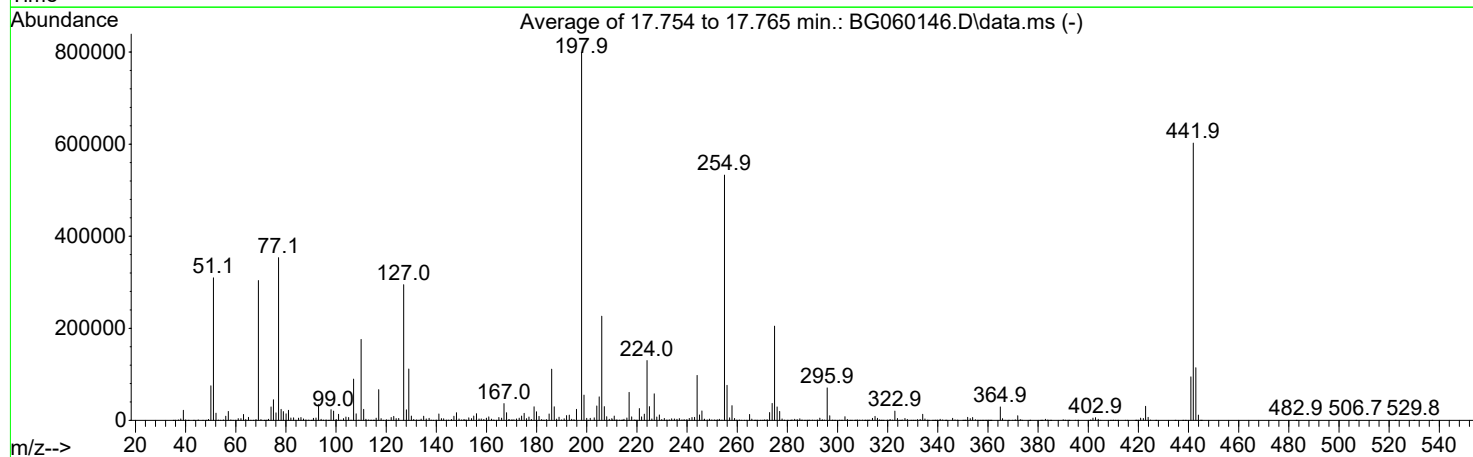


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122223\
Data File : BG060146.D
Acq On : 22 Dec 2023 20:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 22 03:42:04 2023

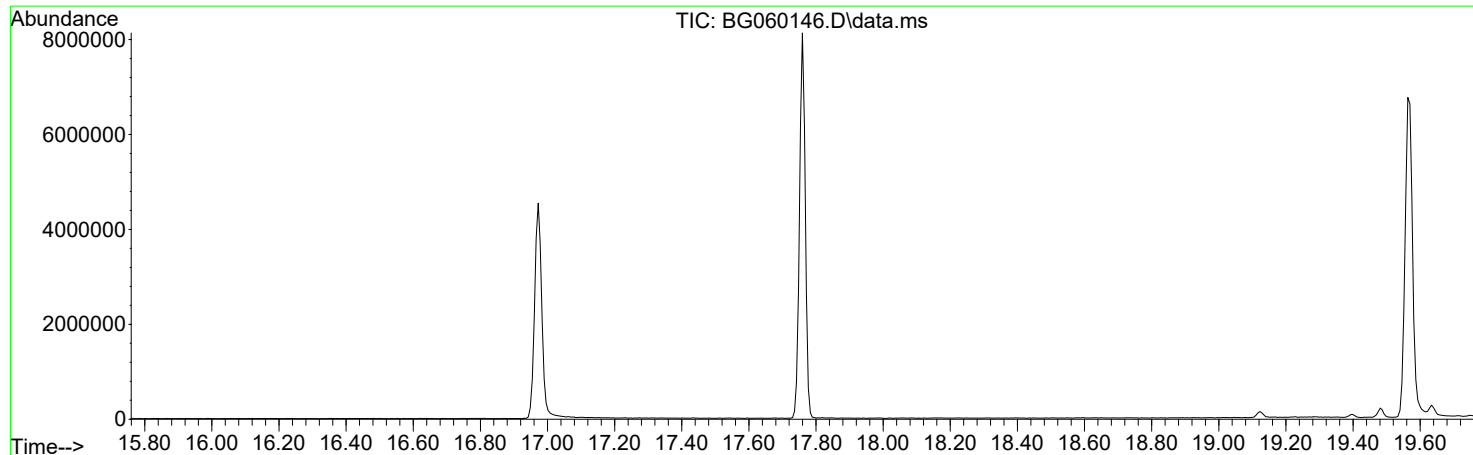

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	309584	PASS
68	69	0.00	2	0.6	1824	PASS
69	198	0.00	100	38.0	303726	PASS
70	69	0.00	2	0.6	1927	PASS
127	198	10	80	36.9	294912	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	799061	PASS
199	198	5	9	6.9	54821	PASS
275	198	10	60	25.6	204672	PASS
365	198	1	100	3.6	29163	PASS
441	198	0.01	100	11.8	94536	PASS
442	442	50	100	100.0	602283	PASS
443	442	15	24	19.0	114216	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/22/2023	BNA_G	BG060146.D
Compound Name	Response	Retention Time
DDT	1940496	20.797
DDD	99085	20.356
DDE	1817	19.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
100902	2041398	4.94

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122223\
Data File : BG060146.D
Acq On : 22 Dec 2023 20:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 23 06:04:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 03:42:04 2023
Response via : Initial Calibration

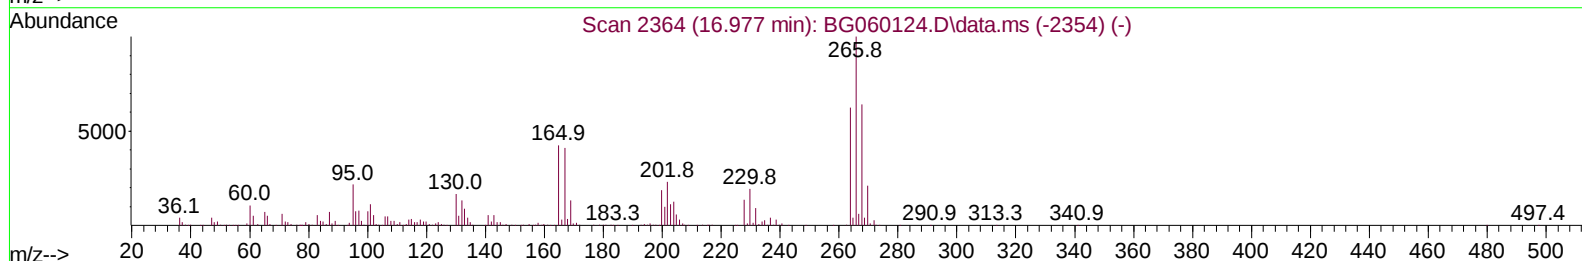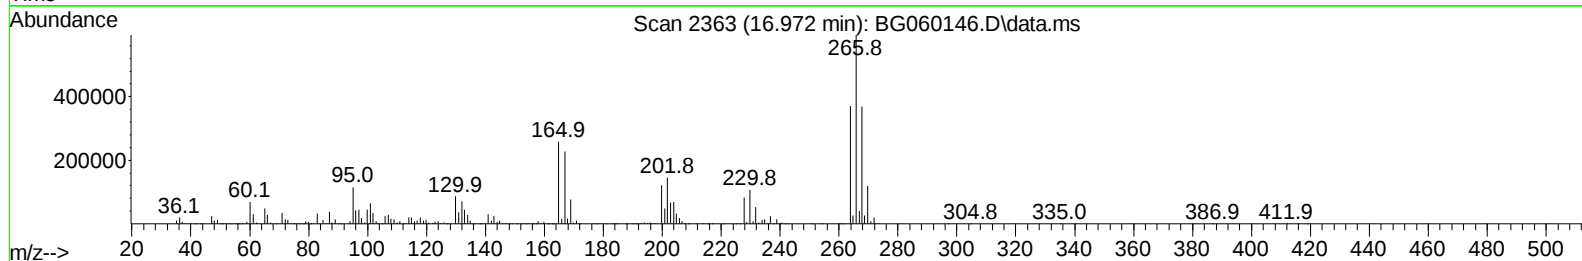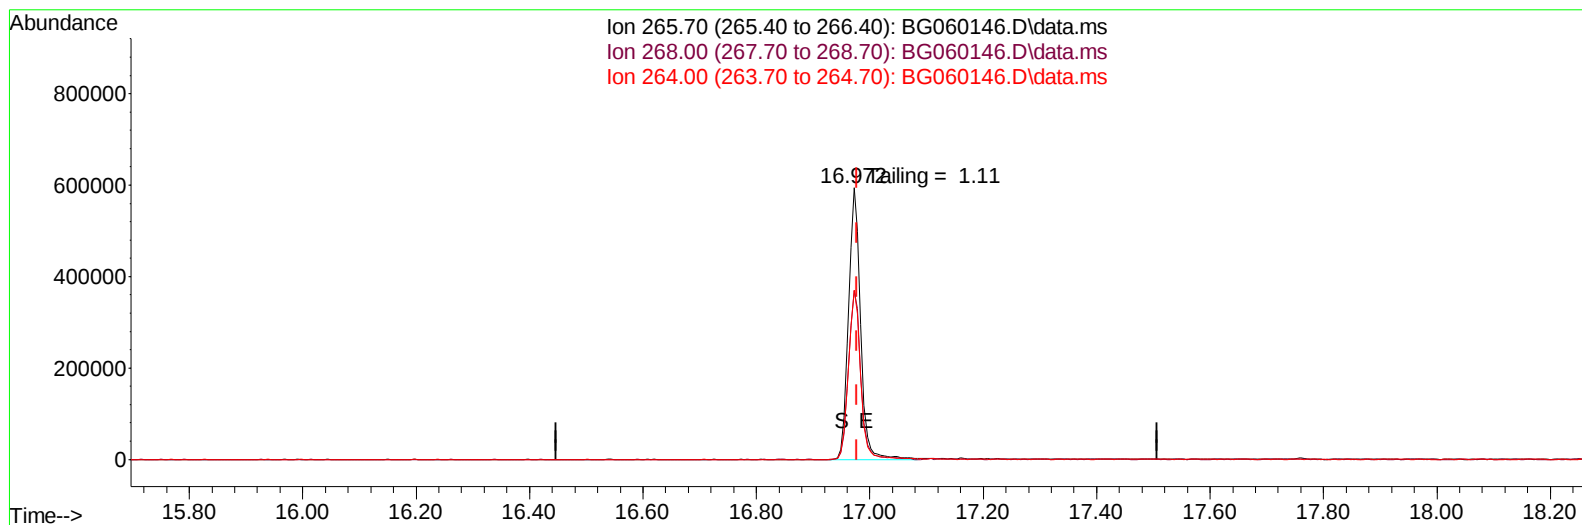

TIC: BG060146.D\data.ms

(70) Pentachlorophenol (C)

16.972min (-0.005) 608348.68 ng




response 881648

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.80	66.44
264.00	62.50	62.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122223\
Data File : BG060146.D
Acq On : 22 Dec 2023 20:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 23 06:04:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 22 03:42:04 2023
Response via : Initial Calibration

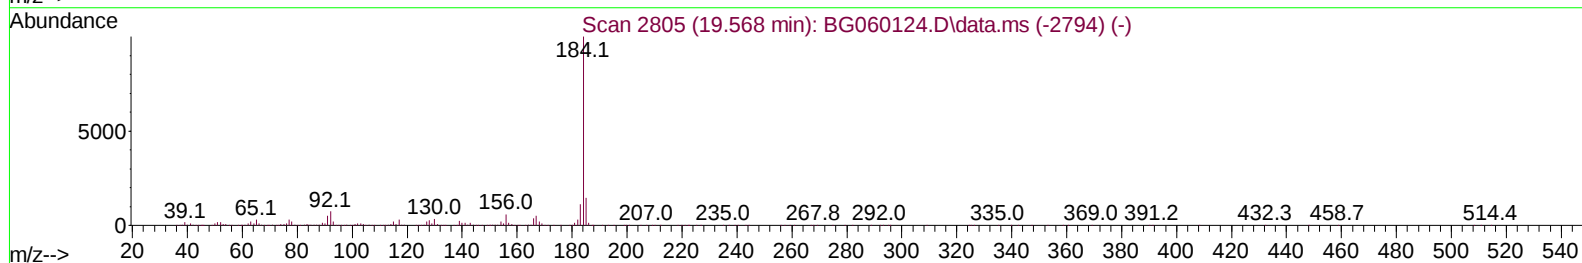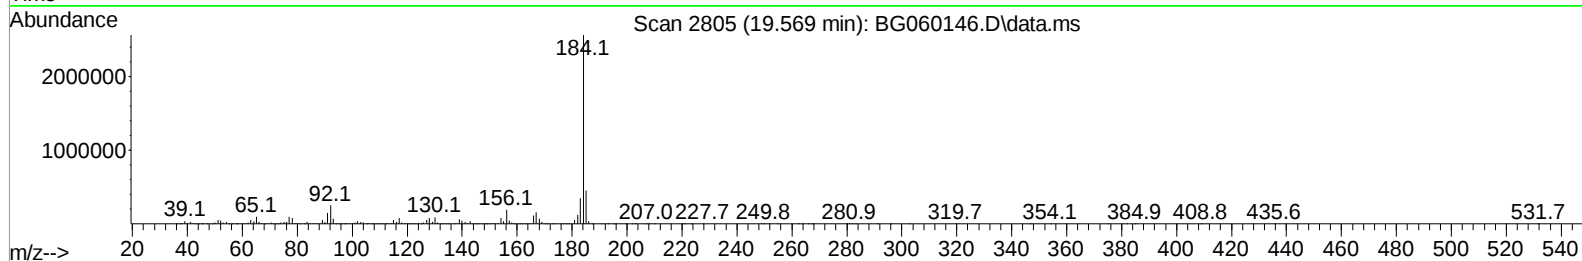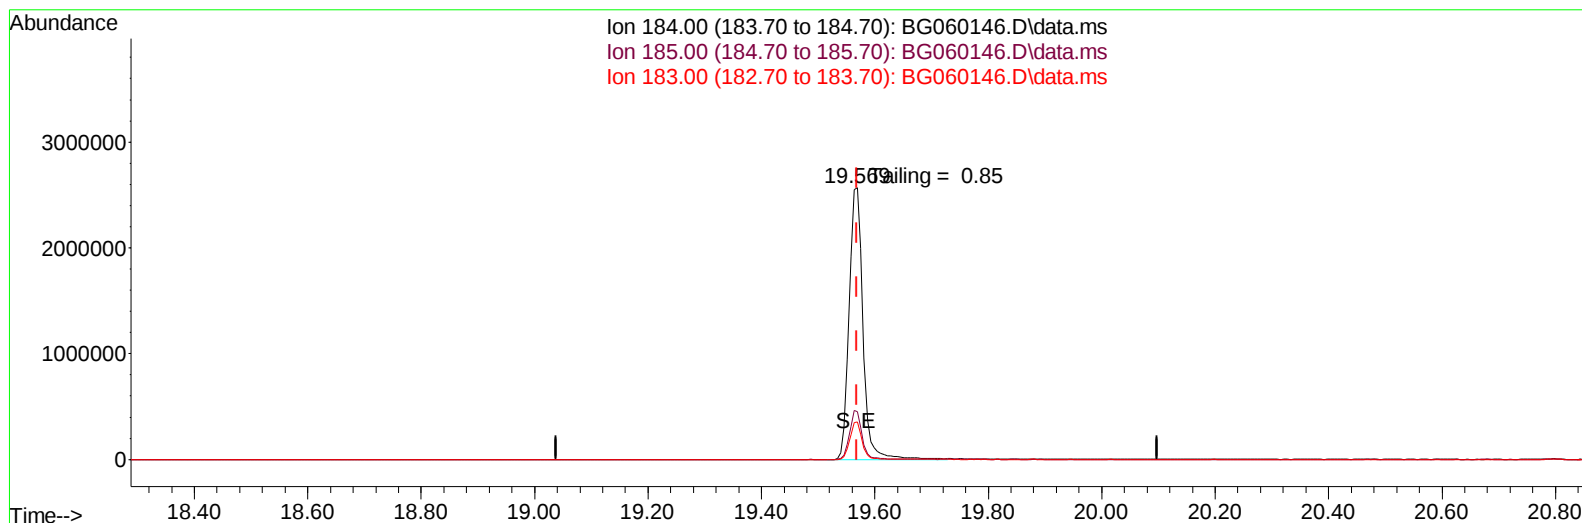

TIC: BG060146.D\data.ms

(77) Benzidine

19.569min (+ 0.001) 191515.68 ng

response 4385850

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	17.54#
183.00	11.30	13.74#
0.00	0.00	0.00