

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG122320\
 Data File : BG047814.D
 Acq On : 24 Dec 2020 1:20
 Operator : CG/JU
 Sample : L5112-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A54S9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.816	77	81	84	rVB	2555	4308	0.67%	0.072%
2	3.851	84	87	89	rBV2	1588	1950	0.30%	0.032%
3	3.957	104	105	110	rVB2	2444	2294	0.36%	0.038%
4	4.068	121	124	127	rVB3	3785	4432	0.69%	0.074%
5	4.139	134	136	138	rBV3	2566	2805	0.44%	0.047%
6	4.198	141	146	151	rVB4	4206	7194	1.12%	0.120%
7	4.380	173	177	179	rVB2	2184	2875	0.45%	0.048%
8	4.456	186	190	192	rBV2	1932	2448	0.38%	0.041%
9	4.685	226	229	230	rBV2	2446	2344	0.36%	0.039%
10	5.249	323	325	327	rVB2	3788	2034	0.32%	0.034%
11	6.254	493	496	497	rBV	2095	2024	0.31%	0.034%
12	7.335	673	680	693	rVB2	96729	176596	27.45%	2.936%
13	7.511	704	710	717	rBV2	57049	96494	15.00%	1.604%
14	7.723	740	746	753	rBV2	93356	161446	25.09%	2.684%
15	8.052	795	802	805	rBV	1110	2019	0.31%	0.034%
16	8.199	819	827	834	rBV	128822	212469	33.02%	3.532%
17	8.892	938	945	957	rVB2	94584	166614	25.90%	2.770%
18	9.021	962	967	970	rVB3	3027	4816	0.75%	0.080%
19	9.362	1018	1025	1036	rVB	94723	169803	26.39%	2.823%
20	9.768	1090	1094	1100	rVB2	4357	7005	1.09%	0.116%
21	10.091	1142	1149	1157	rBV3	90654	155035	24.10%	2.577%
22	10.631	1234	1241	1249	rBV2	125382	224097	34.83%	3.725%
23	11.025	1296	1308	1315	rBV	152693	284620	44.24%	4.731%
24	11.148	1322	1329	1336	rBV	88841	165436	25.71%	2.750%
25	11.307	1354	1356	1360	rBV	1815	2113	0.33%	0.035%
26	11.806	1437	1441	1443	rBV	1415	1921	0.30%	0.032%
27	12.470	1552	1554	1557	rVB	1924	1922	0.30%	0.032%
28	12.517	1557	1562	1565	rBV	1544	2513	0.39%	0.042%
29	12.588	1568	1574	1579	rBV3	2153	4888	0.76%	0.081%
30	12.958	1635	1637	1640	rBV3	2145	1918	0.30%	0.032%
31	13.175	1672	1674	1677	rVB3	2859	3085	0.48%	0.051%
32	13.428	1714	1717	1720	rVB2	2487	2794	0.43%	0.046%
33	13.510	1729	1731	1734	rVB2	2273	1887	0.29%	0.031%
34	13.628	1750	1751	1758	rVB2	2406	2932	0.46%	0.049%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG122320\
 Data File : BG047814.D
 Acq On : 24 Dec 2020 1:20
 Operator : CG/JU
 Sample : L5112-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A54S9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

35	13.692	1758	1762	1766	rBV3	5045	7099	1.10%	0.118%
36	14.209	1844	1850	1855	rBV	228566	331141	51.47%	5.505%
37	14.256	1855	1858	1864	rVB	35725	54011	8.39%	0.898%
38	14.515	1892	1902	1911	rBV	235306	373147	57.99%	6.203%
39	14.820	1948	1954	1961	rVB	254281	406871	63.24%	6.764%
40	14.991	1977	1983	1992	rBV2	57457	100871	15.68%	1.677%
41	15.056	1992	1994	1999	rVB2	2469	3230	0.50%	0.054%
42	15.208	2017	2020	2021	rBV	5662	5686	0.88%	0.095%
43	15.808	2115	2122	2128	rBV	303522	474394	73.73%	7.886%
44	15.913	2134	2140	2146	rBV2	78912	116233	18.06%	1.932%
45	16.043	2159	2162	2163	rBV	2716	2519	0.39%	0.042%
46	16.319	2205	2209	2214	rBV	1441	3244	0.50%	0.054%
47	16.477	2233	2236	2237	rBV	1847	1776	0.28%	0.030%
48	16.642	2262	2264	2266	rBV	2574	1826	0.28%	0.030%
49	16.836	2293	2297	2300	rVB	1772	2131	0.33%	0.035%
50	17.006	2324	2326	2327	rBV	2737	2325	0.36%	0.039%
51	17.083	2336	2339	2346	rVB4	7940	10745	1.67%	0.179%
52	17.200	2356	2359	2360	rBV4	2659	2168	0.34%	0.036%
53	17.558	2413	2420	2425	rBV	336447	522945	81.28%	8.693%
54	17.652	2430	2436	2447	rVB2	334397	516275	80.24%	8.583%
55	17.811	2461	2463	2466	rBV	3015	3119	0.48%	0.052%
56	17.940	2483	2485	2488	rVB	2427	2807	0.44%	0.047%
57	18.305	2545	2547	2549	rBV	1761	1813	0.28%	0.030%
58	18.358	2552	2556	2557	rBV	3020	3676	0.57%	0.061%
59	18.481	2572	2577	2578	rBV2	3838	4640	0.72%	0.077%
60	18.604	2597	2598	2599	rBV	3385	2075	0.32%	0.034%
61	18.734	2618	2620	2621	rBV	2641	1854	0.29%	0.031%
62	19.098	2679	2682	2684	rVB2	3404	3373	0.52%	0.056%
63	19.145	2687	2690	2695	rBV4	4276	9485	1.47%	0.158%
64	19.773	2795	2797	2798	rBV2	5297	3632	0.56%	0.060%
65	19.926	2817	2823	2833	rVB	454814	643421	100.00%	10.696%
66	21.830	3141	3147	3154	rBV2	305708	509771	79.23%	8.474%


Sum of corrected areas: 6015434

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG122320\
Data File : BG047814.D
Acq On : 24 Dec 2020 1:20
Operator : CG/JU
Sample : L5112-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A54S9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

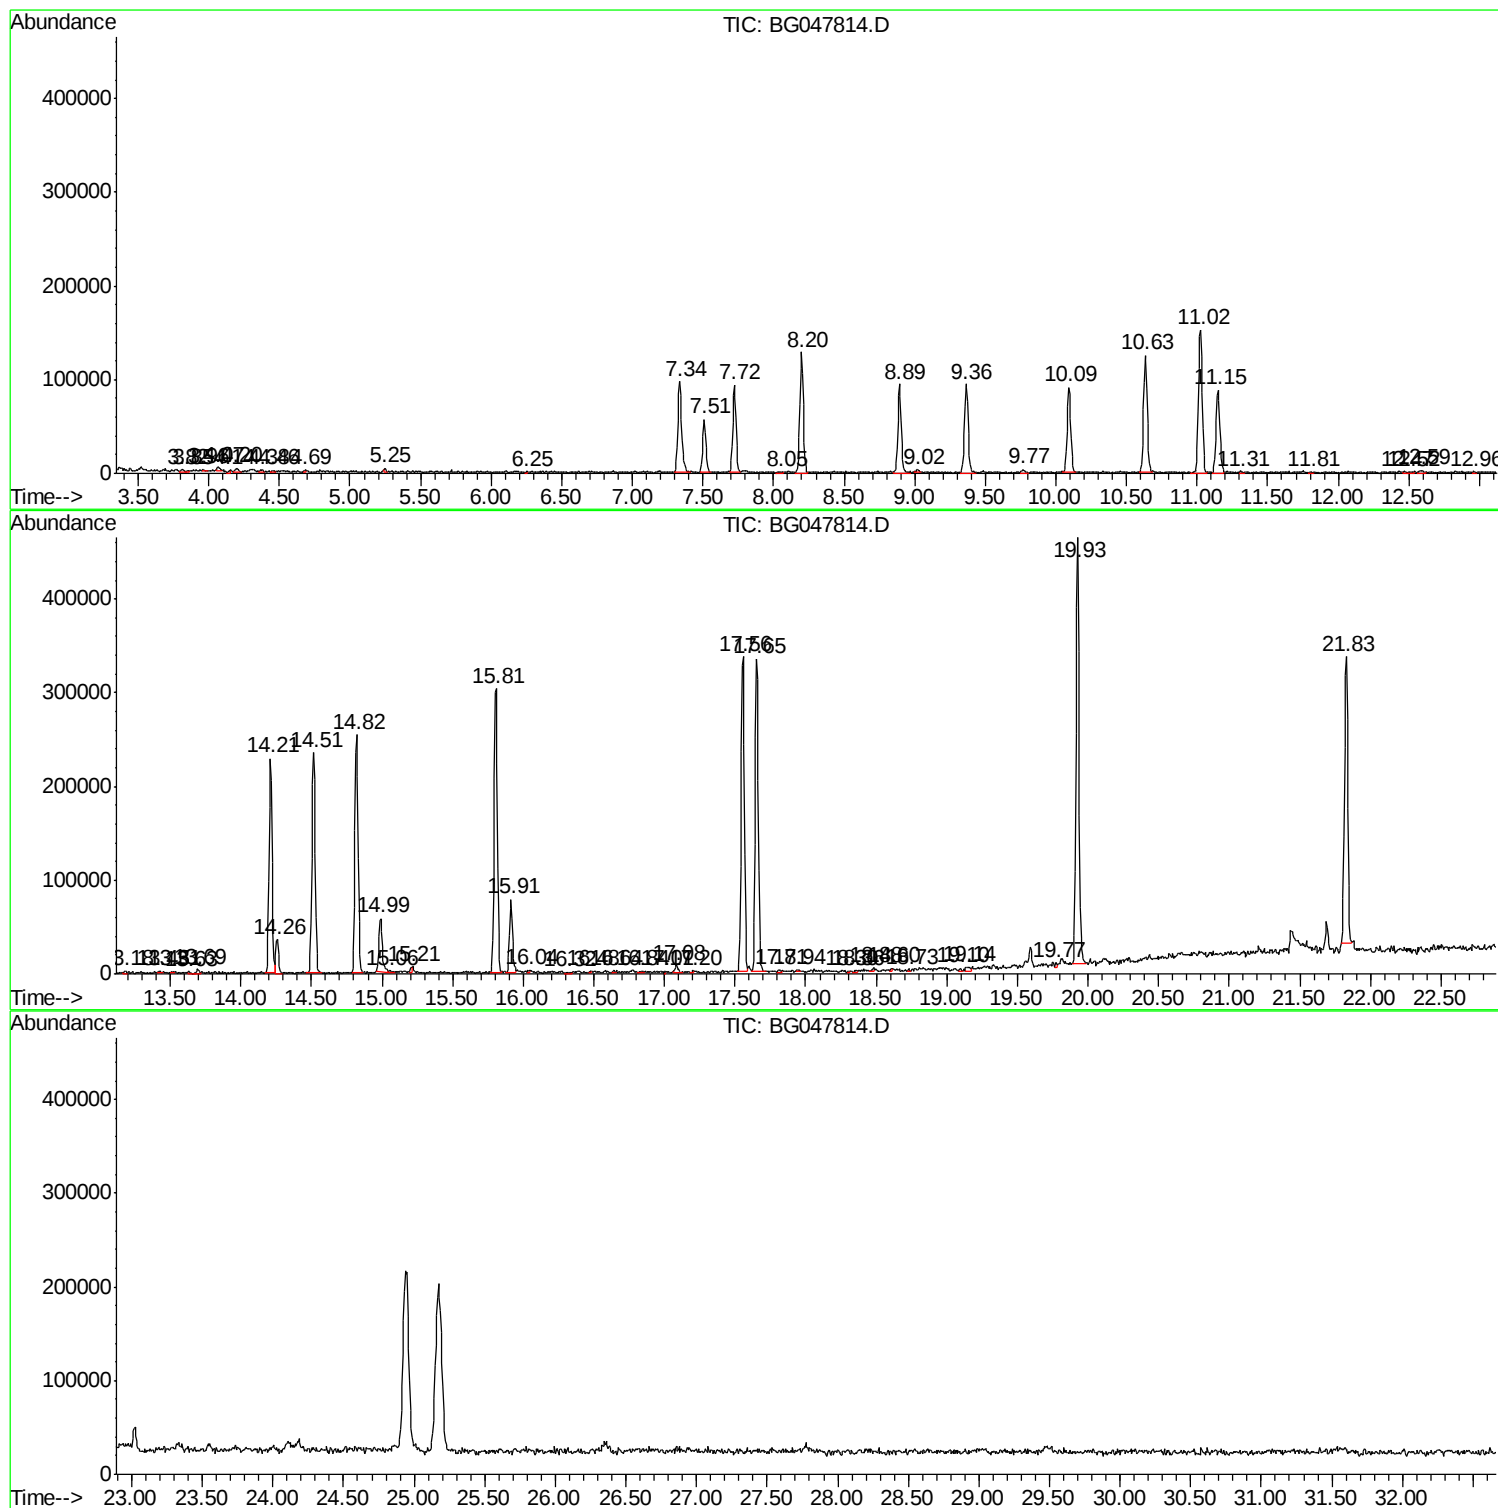

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG122320\
Data File : BG047814.D
Acq On : 24 Dec 2020 1:20
Operator : CG/JU
Sample : L5112-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A54S9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG122320\
Data File : BG047814.D
Acq On : 24 Dec 2020 1:20
Operator : CG/JU
Sample : L5112-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A54S9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc