

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG122320\
 Data File : BG047818.D
 Acq On : 24 Dec 2020 4:42
 Operator : CG/JU
 Sample : PB133750BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.422	12	14	16	rBV2	3568	3167	0.30%	0.031%
2	3.475	20	23	24	rVV2	2974	2883	0.27%	0.028%
3	3.528	28	32	39	rVB5	7300	11707	1.10%	0.114%
4	3.616	45	47	51	rVB	2376	2479	0.23%	0.024%
5	3.904	90	96	98	rBV2	2324	4434	0.42%	0.043%
6	3.921	98	99	102	rVB2	3328	2154	0.20%	0.021%
7	4.233	149	152	155	rBV3	2833	2494	0.23%	0.024%
8	4.262	155	157	160	rBV2	2014	1985	0.19%	0.019%
9	4.297	160	163	165	rBV2	2388	2526	0.24%	0.025%
10	4.356	171	173	176	rBV	2031	2103	0.20%	0.021%
11	4.562	206	208	211	rVB	1853	2359	0.22%	0.023%
12	4.914	266	268	274	rBV2	1951	3662	0.34%	0.036%
13	5.073	292	295	299	rBV2	1486	2926	0.27%	0.029%
14	5.754	407	411	416	rBV2	1366	2697	0.25%	0.026%
15	6.025	455	457	460	rVB3	2134	2106	0.20%	0.021%
16	6.436	524	527	529	rBV3	1945	1866	0.17%	0.018%
17	7.082	636	637	640	rBV	2012	1838	0.17%	0.018%
18	7.247	663	665	671	rVB	1288	1781	0.17%	0.017%
19	7.335	671	680	688	rBV2	157568	286349	26.83%	2.799%
20	7.511	703	710	718	rVB2	91672	161634	15.15%	1.580%
21	7.658	733	735	738	rVB	2407	1778	0.17%	0.017%
22	7.723	738	746	754	rBV	167824	289997	27.18%	2.835%
23	7.952	781	785	787	rVB	1350	1823	0.17%	0.018%
24	8.122	813	814	818	rVB	1795	1814	0.17%	0.018%
25	8.199	820	827	834	rVV	109293	182624	17.11%	1.785%
26	8.334	847	850	851	rBV	2609	2027	0.19%	0.020%
27	8.892	938	945	954	rBV2	189749	333664	31.27%	3.262%
28	9.362	1017	1025	1034	rBV	150962	277773	26.03%	2.715%
29	9.644	1069	1073	1075	rBV	2033	2015	0.19%	0.020%
30	9.667	1075	1077	1080	rBV	1629	1889	0.18%	0.018%
31	9.791	1096	1098	1102	rBV	1632	2157	0.20%	0.021%
32	9.944	1121	1124	1127	rBV	1969	2260	0.21%	0.022%
33	10.090	1142	1149	1158	rBV	151061	274664	25.74%	2.685%
34	10.472	1210	1214	1216	rBV	1604	1935	0.18%	0.019%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG122320\
 Data File : BG047818.D
 Acq On : 24 Dec 2020 4:42
 Operator : CG/JU
 Sample : PB133750BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

35	10.631	1234	1241	1252	rBV	203885	378393	35.46%	3.699%
36	10.801	1267	1270	1273	rBV	2343	2472	0.23%	0.024%
37	11.025	1300	1308	1316	rBV	132206	234620	21.99%	2.293%
38	11.148	1322	1329	1336	rBV2	180884	333430	31.25%	3.259%
39	11.783	1434	1437	1440	rBV2	1559	2392	0.22%	0.023%
40	12.170	1498	1503	1505	rVB2	1953	2139	0.20%	0.021%
41	12.582	1570	1573	1574	rBV2	3977	3511	0.33%	0.034%
42	12.599	1574	1576	1581	rVB2	4342	4656	0.44%	0.046%
43	12.746	1598	1601	1604	rVB2	1699	2138	0.20%	0.021%
44	12.770	1604	1605	1610	rBV2	1448	2017	0.19%	0.020%
45	13.087	1654	1659	1660	rBV2	1372	2138	0.20%	0.021%
46	13.698	1759	1763	1766	rVB2	1558	2122	0.20%	0.021%
47	14.209	1844	1850	1859	rBV	389561	561387	52.61%	5.488%
48	14.515	1895	1902	1912	rVB	366596	594514	55.71%	5.812%
49	14.744	1940	1941	1944	rVB	2205	1839	0.17%	0.018%
50	14.820	1947	1954	1963	rVB2	217495	341886	32.04%	3.342%
51	14.985	1975	1982	1996	rBV3	184413	318202	29.82%	3.111%
52	15.096	1998	2001	2005	rVB2	1556	2431	0.23%	0.024%
53	15.337	2040	2042	2045	rBV2	2343	2344	0.22%	0.023%
54	15.537	2071	2076	2078	rBV2	1249	1786	0.17%	0.017%
55	15.584	2083	2084	2087	rBV2	1889	1809	0.17%	0.018%
56	15.807	2114	2122	2131	rBV	490707	735584	68.93%	7.191%
57	15.913	2135	2140	2148	rBV	175771	271082	25.40%	2.650%
58	16.048	2159	2163	2167	rVB2	5534	7727	0.72%	0.076%
59	16.583	2251	2254	2255	rBV	2253	1849	0.17%	0.018%
60	16.671	2268	2269	2272	rBV	1863	1874	0.18%	0.018%
61	17.558	2412	2420	2428	rBV	286351	448875	42.06%	4.388%
62	17.652	2430	2436	2446	rVV2	548841	877312	82.21%	8.576%
63	17.723	2446	2448	2451	rVV	2902	2293	0.21%	0.022%
64	17.934	2478	2484	2485	rBV	1883	2336	0.22%	0.023%
65	18.093	2509	2511	2514	rBV	1771	2149	0.20%	0.021%
66	18.340	2550	2553	2556	rVB	2129	2210	0.21%	0.022%
67	18.710	2613	2616	2618	rBV3	1946	2124	0.20%	0.021%
68	18.845	2635	2639	2643	rVB2	2325	3856	0.36%	0.038%
69	18.886	2643	2646	2649	rBV	1983	2376	0.22%	0.023%
70	18.945	2653	2656	2657	rVB	2376	2076	0.19%	0.020%
71	19.074	2674	2678	2680	rBV	1422	1879	0.18%	0.018%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG122320\
 Data File : BG047818.D
 Acq On : 24 Dec 2020 4:42
 Operator : CG/JU
 Sample : PB133750BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

72	19.192	2695	2698	2700	rBV	2530	2248	0.21%	0.022%
73	19.244	2703	2707	2708	rBV	1515	1985	0.19%	0.019%
74	19.262	2708	2710	2713	rBV	2050	2260	0.21%	0.022%
75	19.438	2736	2740	2743	rBV3	2568	4393	0.41%	0.043%
76	19.562	2757	2761	2765	rBV4	8632	13387	1.25%	0.131%
77	19.726	2787	2789	2793	rVB2	1906	1832	0.17%	0.018%
78	19.808	2800	2803	2808	rVB	7743	10564	0.99%	0.103%
79	19.850	2808	2810	2813	rBV4	3059	3308	0.31%	0.032%
80	19.926	2816	2823	2830	rBV2	741279	1067116	100.00%	10.431%
81	20.143	2858	2860	2861	rBV	4395	2974	0.28%	0.029%
82	20.267	2879	2881	2882	rBV	3620	3494	0.33%	0.034%
83	20.749	2961	2963	2966	rBV4	4693	5459	0.51%	0.053%
84	20.801	2971	2972	2975	rVB3	7480	4412	0.41%	0.043%
85	21.495	3088	3090	3093	rBV3	4695	3771	0.35%	0.037%
86	21.636	3113	3114	3117	rBV3	6434	3975	0.37%	0.039%
87	21.830	3140	3147	3156	rVB2	284216	500308	46.88%	4.891%
88	21.918	3160	3162	3163	rBV2	5400	2685	0.25%	0.026%
89	22.347	3233	3235	3237	rBV3	4835	3678	0.34%	0.036%
90	23.140	3368	3370	3371	rVB	6250	3126	0.29%	0.031%
91	24.180	3545	3547	3554	rVB7	19700	34069	3.19%	0.333%
92	24.944	3668	3677	3689	rVB	339609	963181	90.26%	9.415%
93	25.179	3706	3717	3727	rVB2	178806	520782	48.80%	5.091%
94	25.690	3802	3804	3806	rBV3	4547	3754	0.35%	0.037%
95	25.872	3833	3835	3839	rBV5	5686	5935	0.56%	0.058%
96	28.111	4214	4216	4217	rBV2	5194	4178	0.39%	0.041%
97	28.152	4221	4223	4226	rVV4	4604	4624	0.43%	0.045%
98	28.722	4318	4320	4321	rVB	6088	4105	0.38%	0.040%
99	30.719	4658	4660	4661	rBV2	5951	4310	0.40%	0.042%
100	32.388	4943	4944	4945	rBV	4988	2564	0.24%	0.025%


Sum of corrected areas: 10229875

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG122320\
Data File : BG047818.D
Acq On : 24 Dec 2020 4:42
Operator : CG/JU
Sample : PB133750BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK50

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

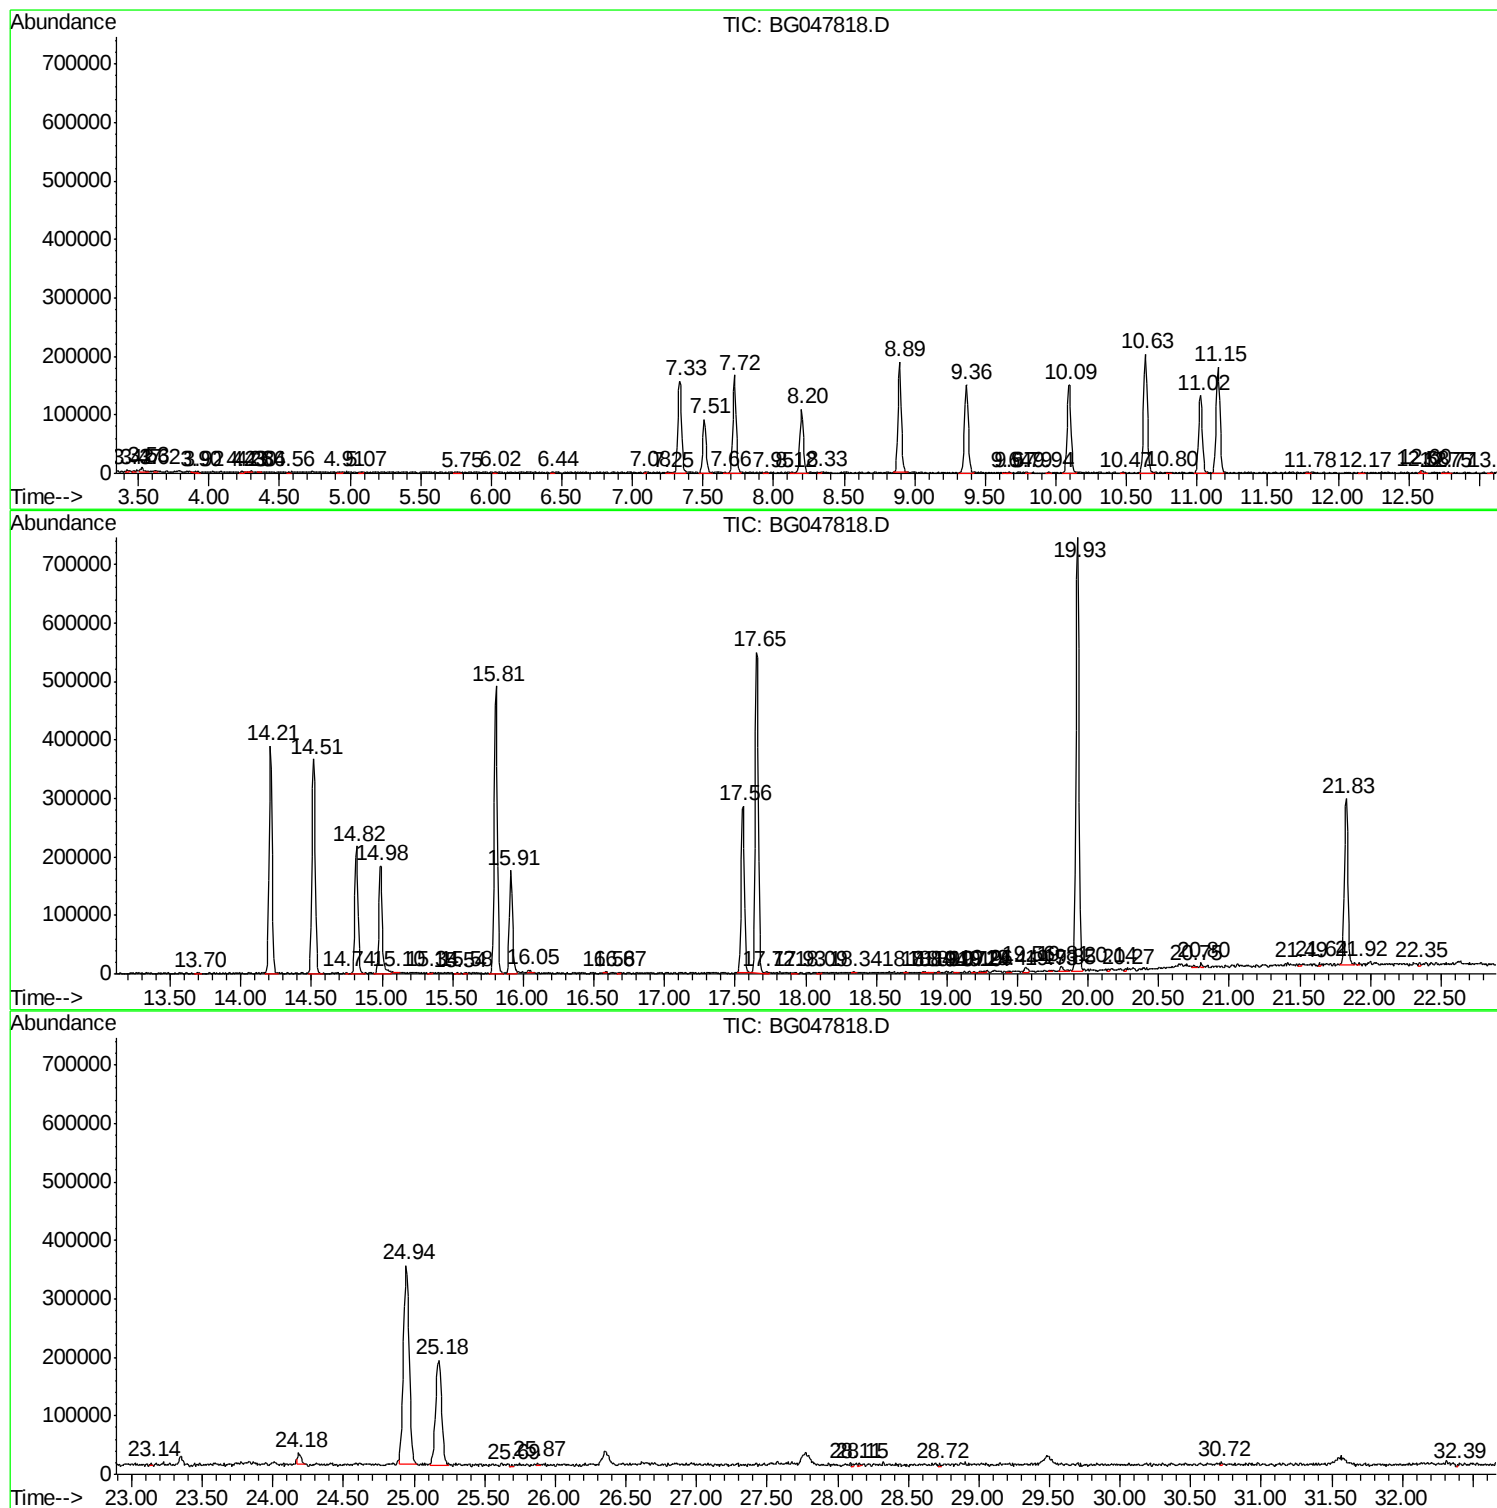

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG122320\
Data File : BG047818.D
Acq On : 24 Dec 2020 4:42
Operator : CG/JU
Sample : PB133750BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK50

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG122320\
Data File : BG047818.D
Acq On : 24 Dec 2020 4:42
Operator : CG/JU
Sample : PB133750BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK50

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
