

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG122320\
 Data File : BG047826.D
 Acq On : 24 Dec 2020 10:52
 Operator : CG/JU
 Sample : PB133749BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK49

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.516	28	30	31	rBV2	4503	3201	0.31%	0.032%
2	3.616	46	47	50	rVB2	2830	1990	0.19%	0.020%
3	4.016	113	115	117	rBV2	3392	3122	0.30%	0.031%
4	4.280	158	160	163	rBV	2517	2317	0.22%	0.023%
5	4.304	163	164	170	rVV3	2075	3086	0.30%	0.031%
6	4.374	174	176	179	rVV2	2291	2708	0.26%	0.027%
7	4.421	183	184	187	rVB	2718	2105	0.20%	0.021%
8	4.556	205	207	208	rVB	2892	1865	0.18%	0.019%
9	4.592	211	213	220	rVB2	2257	3444	0.33%	0.035%
10	4.791	245	247	250	rVB	2119	2007	0.19%	0.020%
11	4.862	257	259	261	rBV	2540	2207	0.21%	0.022%
12	4.938	270	272	275	rVB2	2935	2040	0.20%	0.021%
13	5.097	296	299	301	rBV	2053	2372	0.23%	0.024%
14	5.232	321	322	329	rVB	1299	1878	0.18%	0.019%
15	5.326	335	338	340	rBV	2098	2036	0.20%	0.020%
16	6.572	549	550	552	rBV	2149	1907	0.18%	0.019%
17	6.742	576	579	582	rVB	1506	2410	0.23%	0.024%
18	6.971	613	618	623	rBV	1228	2371	0.23%	0.024%
19	7.042	626	630	632	rBV	1498	2198	0.21%	0.022%
20	7.335	673	680	687	rBV	164632	287143	27.77%	2.888%
21	7.512	701	710	717	rVV	97573	162967	15.76%	1.639%
22	7.588	721	723	728	rVB	1931	2817	0.27%	0.028%
23	7.670	734	737	739	rVB	2109	1865	0.18%	0.019%
24	7.723	739	746	755	rBV	158689	282407	27.31%	2.840%
25	8.046	799	801	806	rBV	1427	2059	0.20%	0.021%
26	8.199	821	827	835	rVB2	102217	181096	17.51%	1.821%
27	8.370	852	856	858	rVB2	2120	2061	0.20%	0.021%
28	8.399	858	861	866	rVB2	1249	2319	0.22%	0.023%
29	8.434	866	867	872	rBV2	1669	2221	0.21%	0.022%
30	8.558	882	888	890	rBV2	1294	1905	0.18%	0.019%
31	8.892	938	945	952	rBV2	191860	323401	31.27%	3.253%
32	9.368	1019	1026	1033	rBV	161846	282528	27.32%	2.841%
33	9.533	1050	1054	1057	rVB	1806	2690	0.26%	0.027%
34	9.568	1057	1060	1065	rBV	2334	3862	0.37%	0.039%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG122320\
 Data File : BG047826.D
 Acq On : 24 Dec 2020 10:52
 Operator : CG/JU
 Sample : PB133749BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK49

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

35	9.932	1118	1122	1124	rBV	1330	1965	0.19%	0.020%
36	10.097	1141	1150	1162	rVV2	145116	271715	26.28%	2.733%
37	10.632	1234	1241	1252	rBV	206746	381033	36.85%	3.832%
38	10.867	1279	1281	1284	rBV	1837	2042	0.20%	0.021%
39	11.025	1300	1308	1315	rBV	130564	235874	22.81%	2.372%
40	11.149	1321	1329	1338	rBV	184165	328751	31.79%	3.306%
41	11.213	1338	1340	1345	rVB	1784	2570	0.25%	0.026%
42	11.689	1418	1421	1424	rBV	1611	1968	0.19%	0.020%
43	12.441	1544	1549	1550	rBV	1735	1856	0.18%	0.019%
44	12.576	1569	1572	1573	rBV	3104	2363	0.23%	0.024%
45	12.776	1604	1606	1610	rVB	2046	1975	0.19%	0.020%
46	13.093	1656	1660	1664	rBV	1785	3186	0.31%	0.032%
47	13.223	1675	1682	1684	rBV	1991	2418	0.23%	0.024%
48	13.352	1702	1704	1707	rVB	2327	1917	0.19%	0.019%
49	13.704	1761	1764	1769	rBV	1883	2829	0.27%	0.028%
50	14.075	1821	1827	1828	rBV	1716	2915	0.28%	0.029%
51	14.210	1844	1850	1857	rVB	381164	535495	51.78%	5.386%
52	14.515	1895	1902	1910	rVV	392720	594733	57.51%	5.981%
53	14.586	1910	1914	1919	rVB	1671	2866	0.28%	0.029%
54	14.821	1945	1954	1960	rBV	215438	339289	32.81%	3.412%
55	14.991	1976	1983	1993	rBV	181250	304951	29.49%	3.067%
56	15.167	2011	2013	2015	rBV	2586	2169	0.21%	0.022%
57	15.261	2026	2029	2031	rVB	1773	1886	0.18%	0.019%
58	15.391	2048	2051	2055	rVB	1985	2202	0.21%	0.022%
59	15.561	2079	2080	2084	rVB	3041	1995	0.19%	0.020%
60	15.808	2114	2122	2130	rBV	477395	731109	70.70%	7.353%
61	15.914	2134	2140	2147	rBV	155373	243223	23.52%	2.446%
62	16.043	2158	2162	2166	rVB2	6911	8824	0.85%	0.089%
63	16.589	2250	2255	2259	rBV2	3114	6294	0.61%	0.063%
64	16.724	2275	2278	2280	rBV	1676	1947	0.19%	0.020%
65	16.818	2293	2294	2297	rVB	2497	1882	0.18%	0.019%
66	17.136	2344	2348	2350	rBV	1438	2127	0.21%	0.021%
67	17.236	2363	2365	2368	rVB	2519	1980	0.19%	0.020%
68	17.559	2412	2420	2427	rBV	284749	447104	43.24%	4.497%
69	17.653	2429	2436	2443	rBV	560187	871490	84.28%	8.765%
70	17.741	2450	2451	2454	rVB	2312	2021	0.20%	0.020%
71	18.017	2494	2498	2500	rBV	1842	3164	0.31%	0.032%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG122320\
 Data File : BG047826.D
 Acq On : 24 Dec 2020 10:52
 Operator : CG/JU
 Sample : PB133749BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK49

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
 Title : SVOA CALIBRATION

72	18.129	2515	2517	2520	rVB	2356	2738	0.26%	0.028%
73	18.176	2523	2525	2527	rBV	2781	2564	0.25%	0.026%
74	18.240	2533	2536	2539	rBV	1665	2473	0.24%	0.025%
75	18.422	2563	2567	2569	rBV	1857	2535	0.25%	0.025%
76	18.687	2610	2612	2614	rBV2	2433	2472	0.24%	0.025%
77	18.793	2629	2630	2634	rBV	2855	3585	0.35%	0.036%
78	18.875	2640	2644	2646	rVB	1837	1859	0.18%	0.019%
79	19.057	2672	2675	2677	rBV	3068	3646	0.35%	0.037%
80	19.080	2677	2679	2682	rVV3	2635	2743	0.27%	0.028%
81	19.116	2682	2685	2687	rVB2	1971	1959	0.19%	0.020%
82	19.145	2687	2690	2693	rBV2	3207	4549	0.44%	0.046%
83	19.198	2698	2699	2702	rVB	3409	2232	0.22%	0.022%
84	19.227	2702	2704	2707	rBV2	2556	2988	0.29%	0.030%
85	19.321	2719	2720	2722	rBV	2654	2148	0.21%	0.022%
86	19.462	2742	2744	2747	rBV2	2529	2526	0.24%	0.025%
87	19.562	2757	2761	2765	rVV2	6819	9719	0.94%	0.098%
88	19.592	2765	2766	2768	rVV	5223	2740	0.26%	0.028%
89	19.615	2768	2770	2771	rVB2	4029	2374	0.23%	0.024%
90	19.809	2800	2803	2807	rVB2	6668	8580	0.83%	0.086%
91	19.927	2816	2823	2832	rBV	702134	1034092	100.00%	10.400%
92	20.056	2840	2845	2848	rBV7	4403	7417	0.72%	0.075%
93	20.526	2923	2925	2926	rBV2	4633	2397	0.23%	0.024%
94	20.831	2975	2977	2978	rBV2	5659	3771	0.36%	0.038%
95	21.830	3140	3147	3154	rBV2	282521	476811	46.11%	4.795%
96	23.199	3378	3380	3381	rBV2	5687	3234	0.31%	0.033%
97	24.944	3666	3677	3690	rBV	326253	934050	90.33%	9.394%
98	25.173	3707	3716	3727	rVB2	154402	463884	44.86%	4.665%
99	28.846	4339	4341	4344	rBV4	6771	8289	0.80%	0.083%
100	31.971	4871	4873	4878	rBV6	5819	6013	0.58%	0.060%


Sum of corrected areas: 9943121

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG122320\
Data File : BG047826.D
Acq On : 24 Dec 2020 10:52
Operator : CG/JU
Sample : PB133749BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK49

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

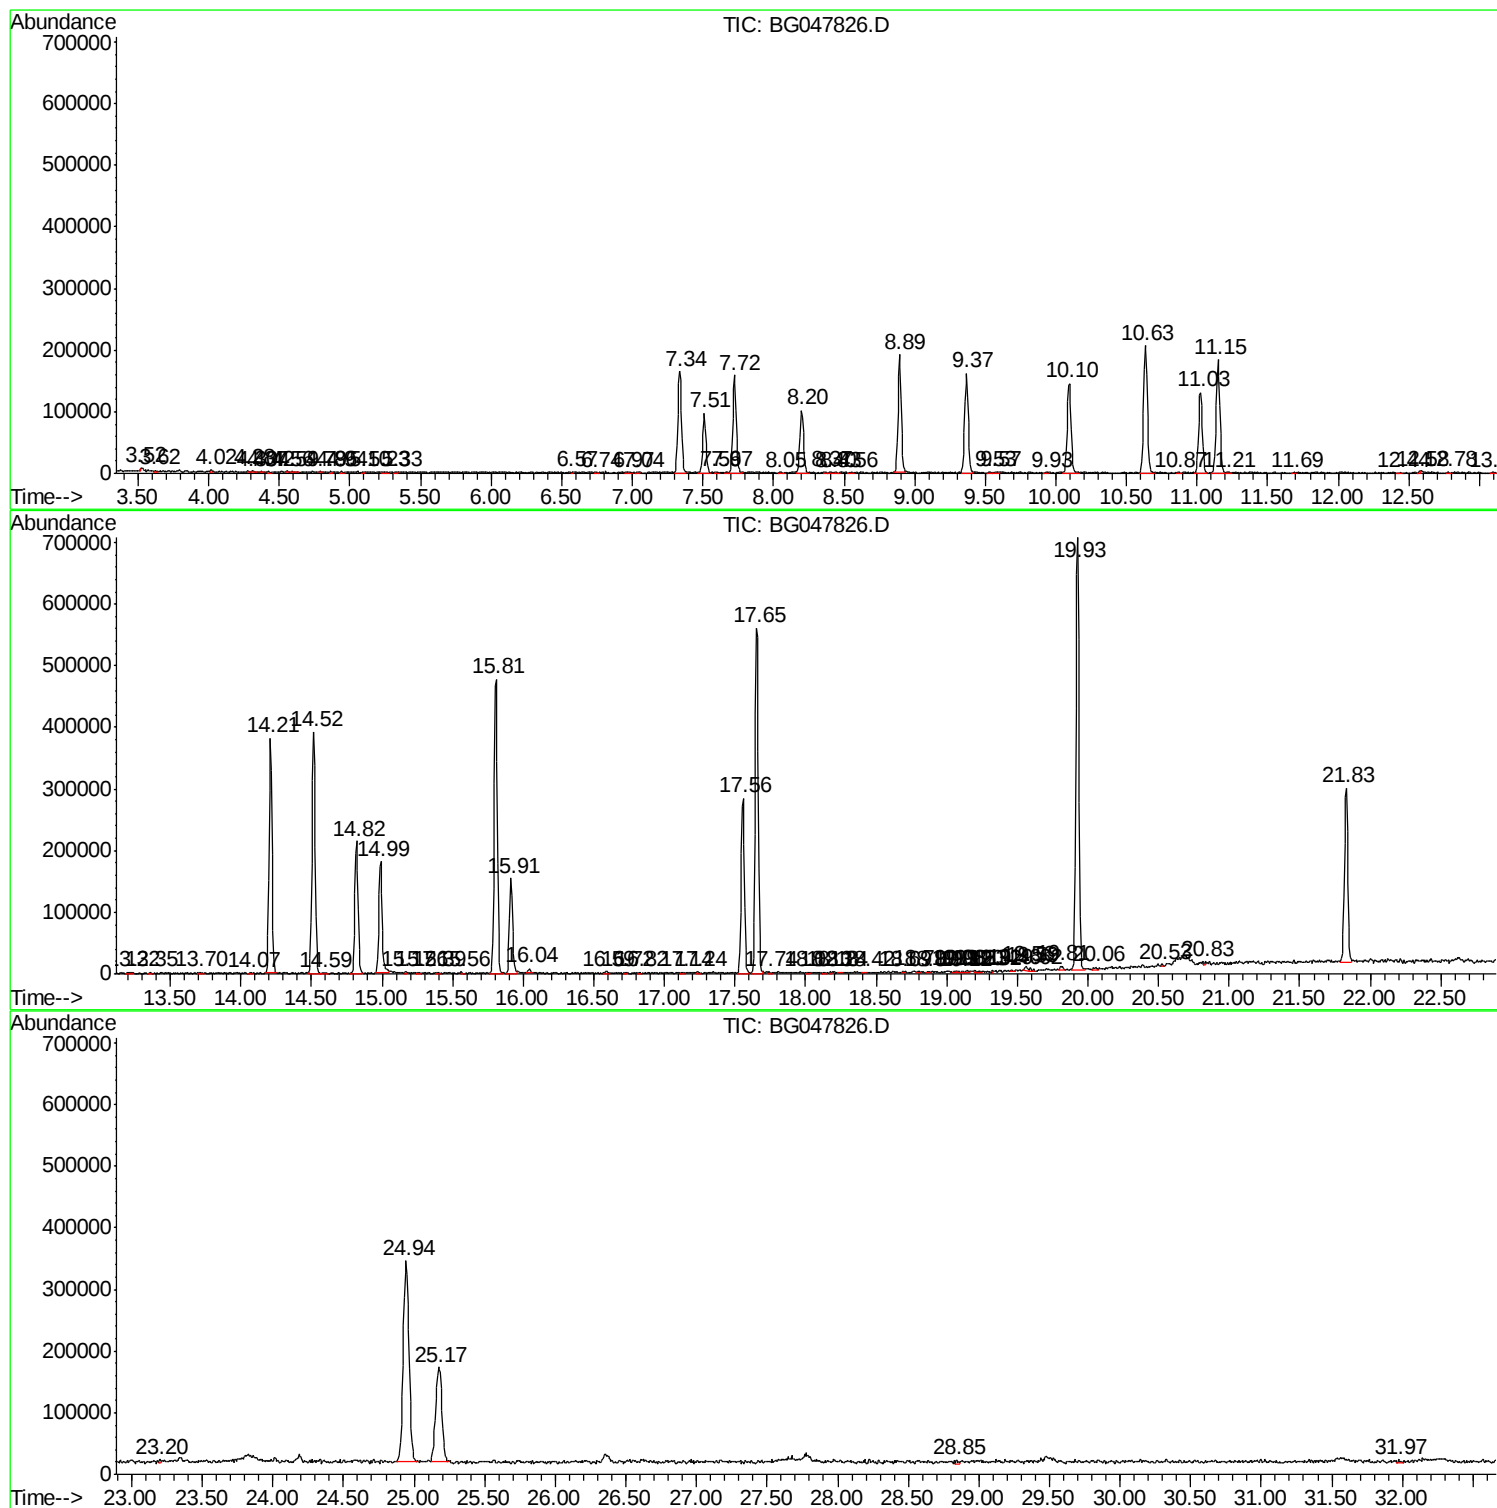

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG122320\
Data File : BG047826.D
Acq On : 24 Dec 2020 10:52
Operator : CG/JU
Sample : PB133749BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK49

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG122320\
Data File : BG047826.D
Acq On : 24 Dec 2020 10:52
Operator : CG/JU
Sample : PB133749BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK49

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG120720MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc